




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027148.D
 Acq On : 19 Sep 2023 15:28
 Operator : SY/MD
 Sample : 04472-17
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM6

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

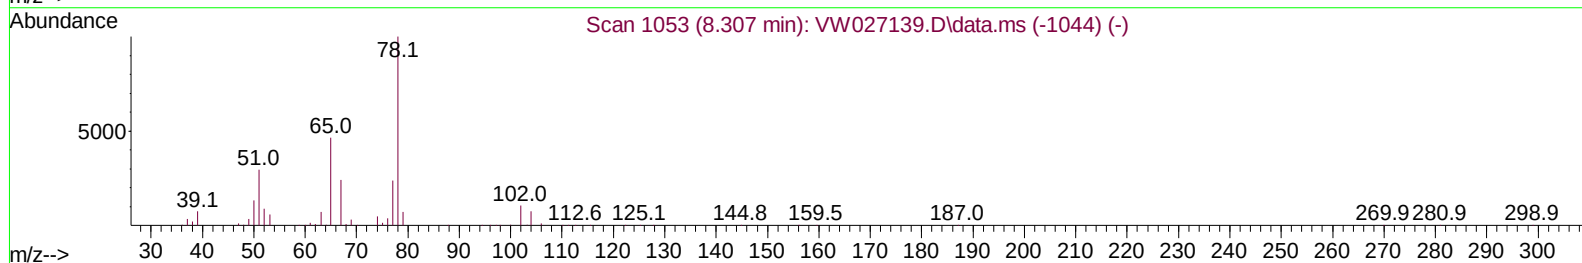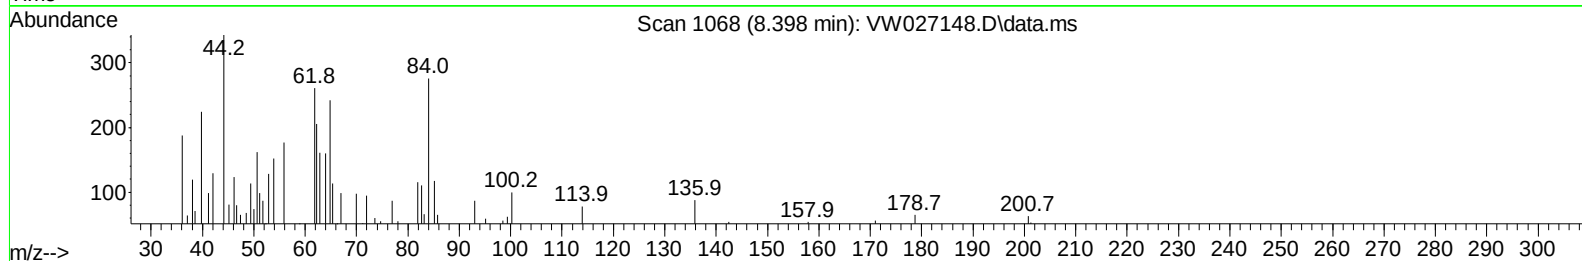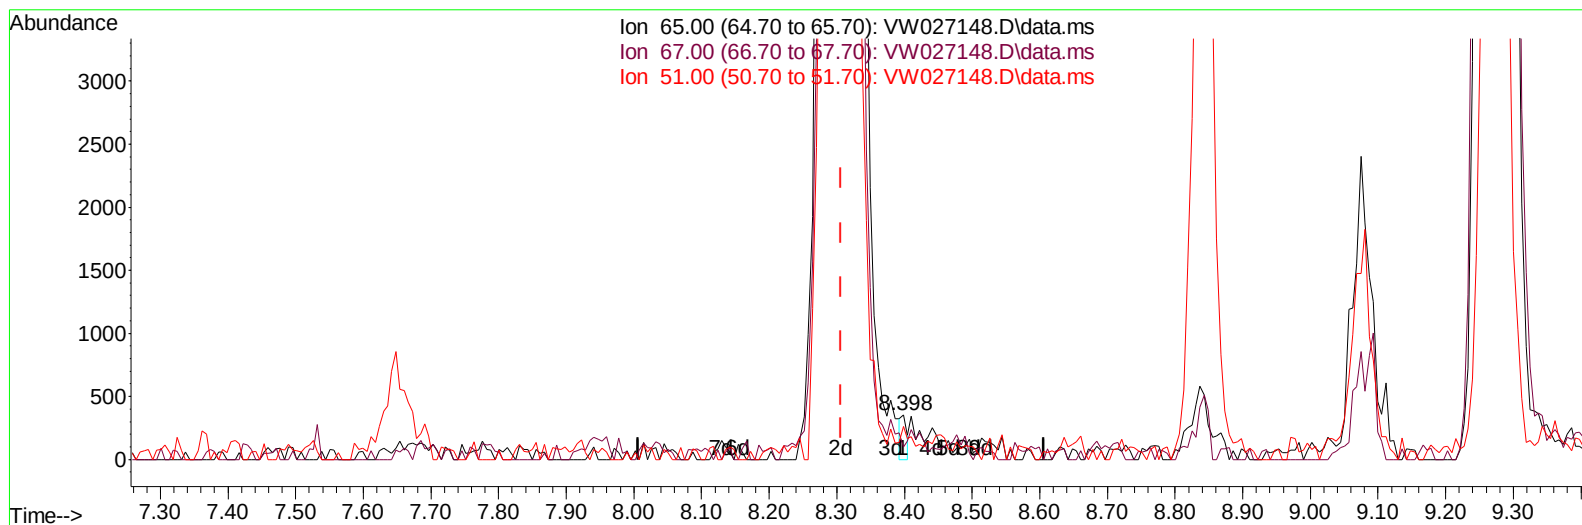

TIC: VW027148.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.398min (+ 0.091) 0.02 ug/L

response 200

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.30	65.00
51.00	101.20	117.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027148.D
 Acq On : 19 Sep 2023 15:28
 Operator : SY/MD
 Sample : 04472-17
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM6

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

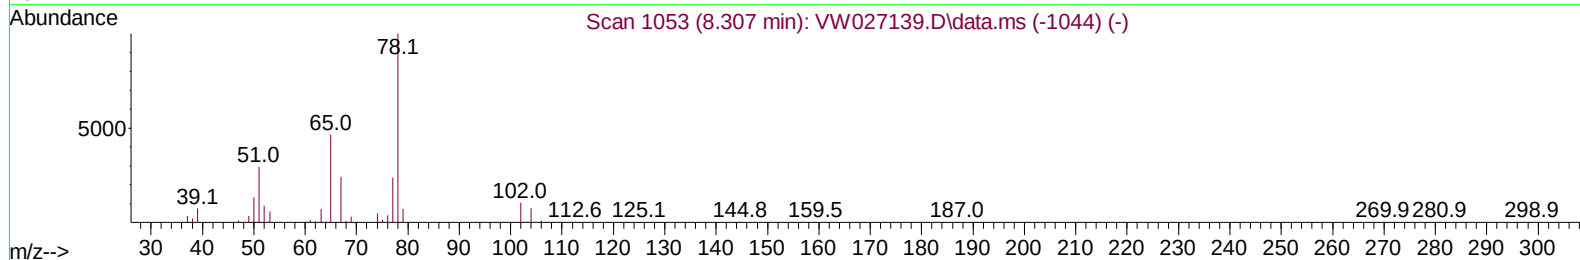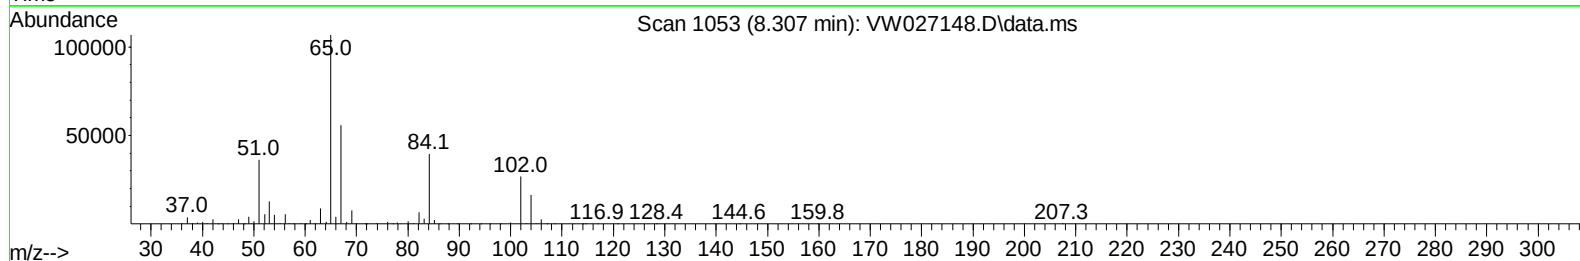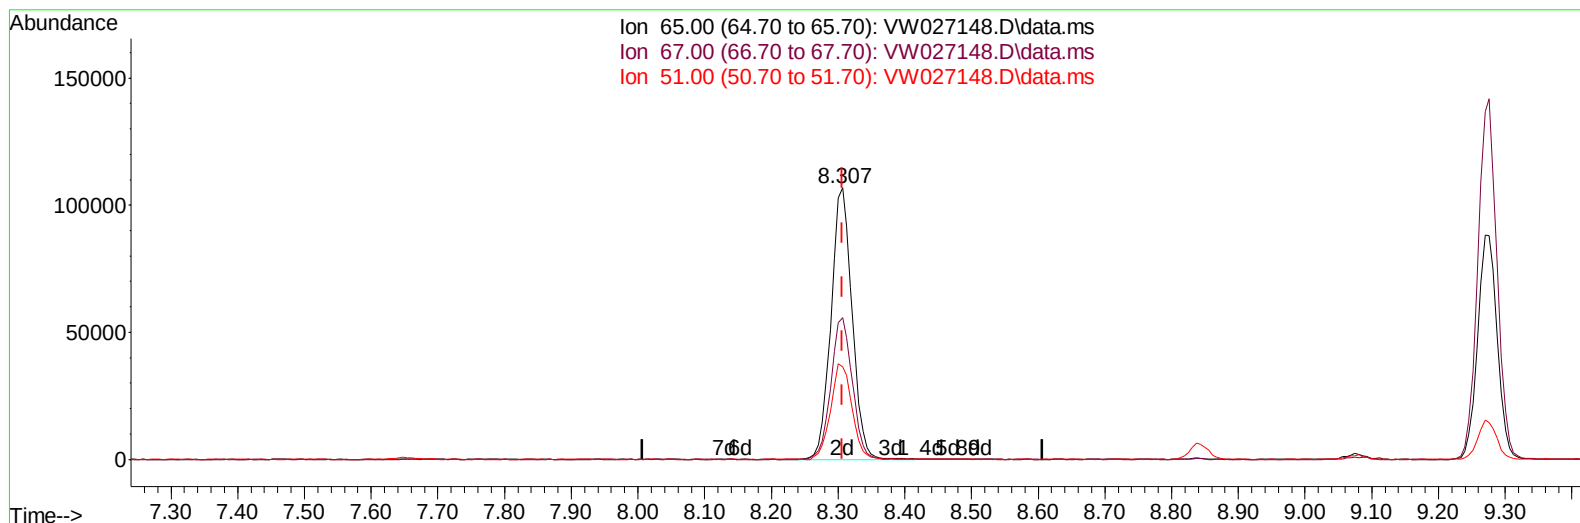

TIC: VW027148.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (0.000) 21.39 ug/L m

response 234572

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.30	0.06#
51.00	101.20	0.10#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027148.D
 Acq On : 19 Sep 2023 15:28
 Operator : SY/MD
 Sample : 04472-17
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM6

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

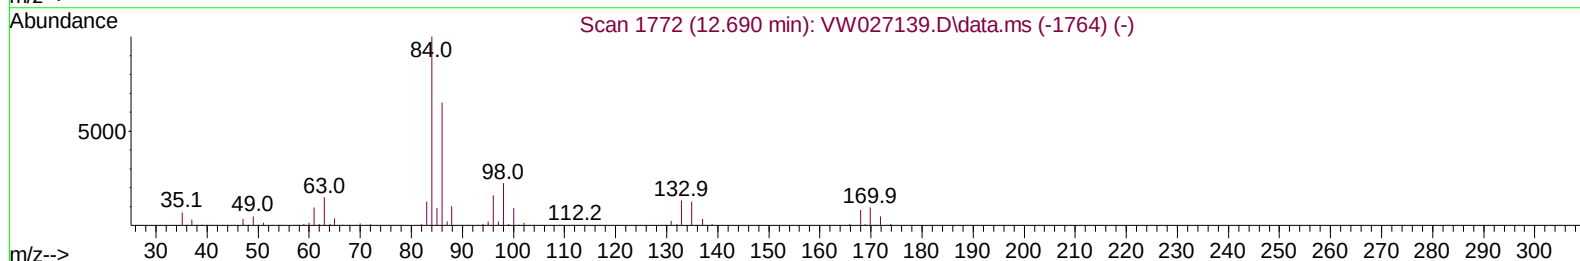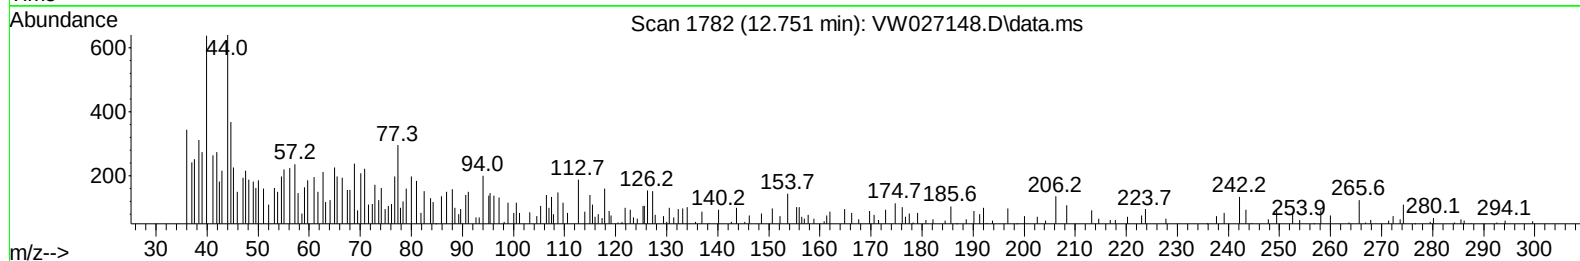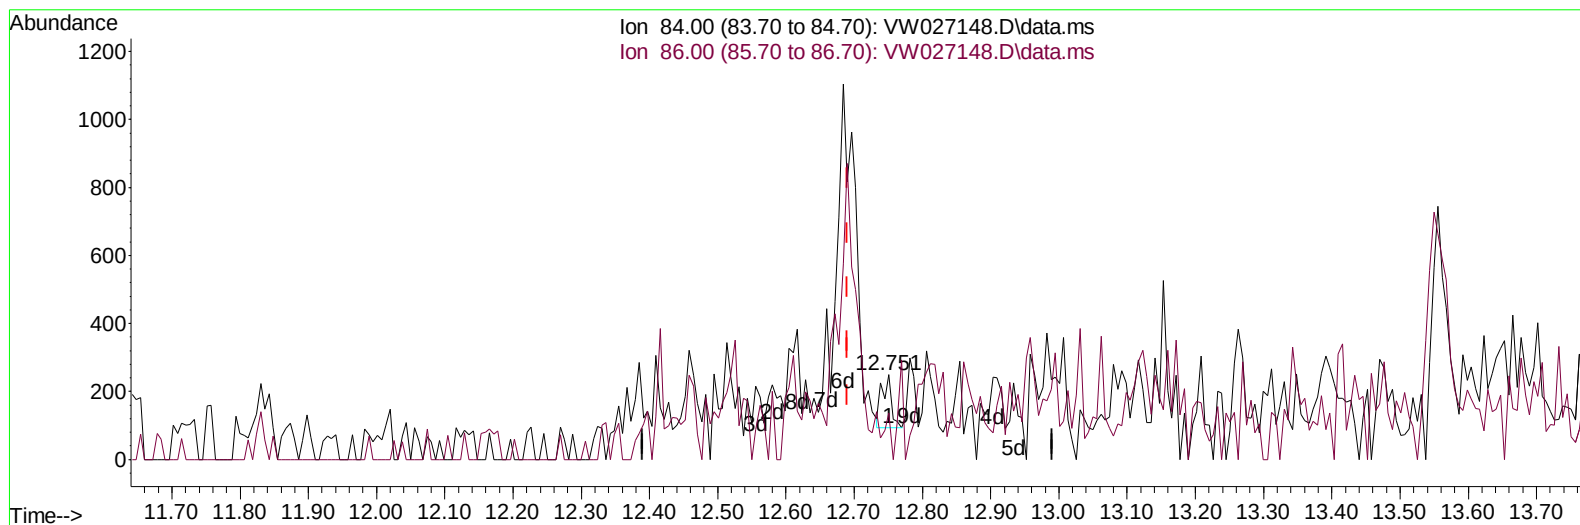

TIC: VW027148.D\data.ms

(56) 1,1,2,2-Tetrachloroethane-d2 (S)

12.751min (+ 0.061) 0.01 ug/L

response 151

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.90	53.64
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027148.D
 Acq On : 19 Sep 2023 15:28
 Operator : SY/MD
 Sample : 04472-17
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		747989	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		724100	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		299159	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		154258	12.818	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery =	51.280%		
7) Chloroethane-d5	2.899	69		215156	23.151	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	92.600%		
11) 1,1-Dichloroethene-d2	4.021	65		77671	15.053	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	60.200%		
21) 2-Butanone-d5	7.081	46		83866	37.635	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	75.260%		
24) Chloroform-d	7.648	84		67553	3.006	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	12.040%#		
26) 1,2-Dichloroethane-d4	8.307	65		234572m	21.393	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	85.560%		
32) Benzene-d6	8.276	84		918001	19.631	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	78.520%		
36) 1,2-Dichloropropane-d6	9.276	67		282226	21.329	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	85.320%		
41) Toluene-d8	10.325	98		806069	19.368	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	77.480%		
43) trans-1,3-Dichloroprop...	10.575	79		103598	19.375	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.520%		
47) 2-Hexanone-d5	10.922	63		44747	28.065	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	56.120%		
56) 1,1,2,2-Tetrachloroeth...	12.684	84		2155m	0.203	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	0.800%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		287300	26.892	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	107.560%		
Target Compounds							
						Qvalue	
13) Acetone	4.131	43		9402	4.466	ug/L	96
14) Carbon disulfide	4.387	76		28688	0.789	ug/L	99
16) Methylene chloride	4.923	84		46757	3.286	ug/L	94
25) Chloroform	7.679	83		386581	18.132	ug/L	97
34) Trichloroethene	9.093	95		40648	3.216	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
Data File : VW027148.D
Acq On : 19 Sep 2023 15:28
Operator : SY/MD
Sample : 04472-17
Misc : 6.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYM6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:37:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 20 01:34:37 2023
Response via : Initial Calibration

