




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027154.D
 Acq On : 19 Sep 2023 17:51
 Operator : SY/MD
 Sample : 04472-15RE
 Misc : 5.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM4RE

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:38:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

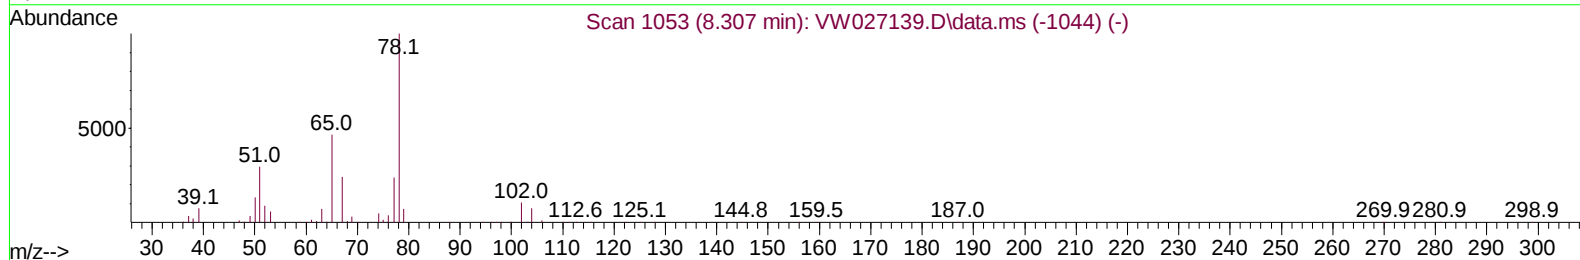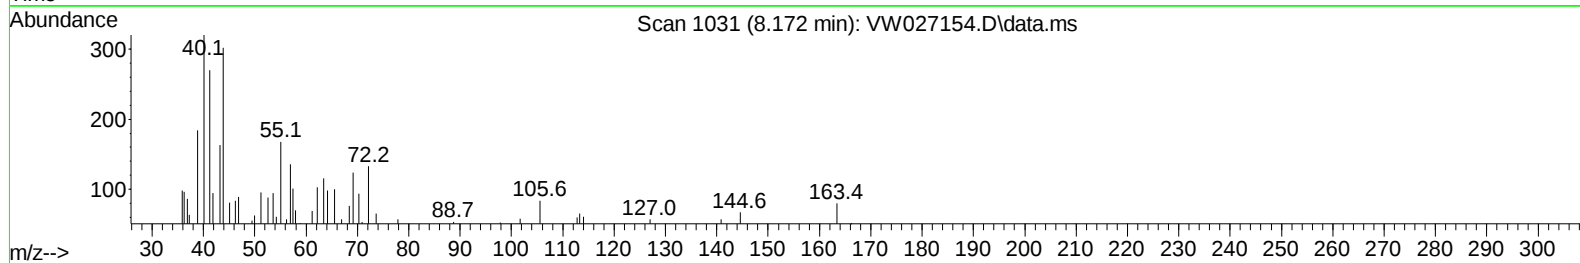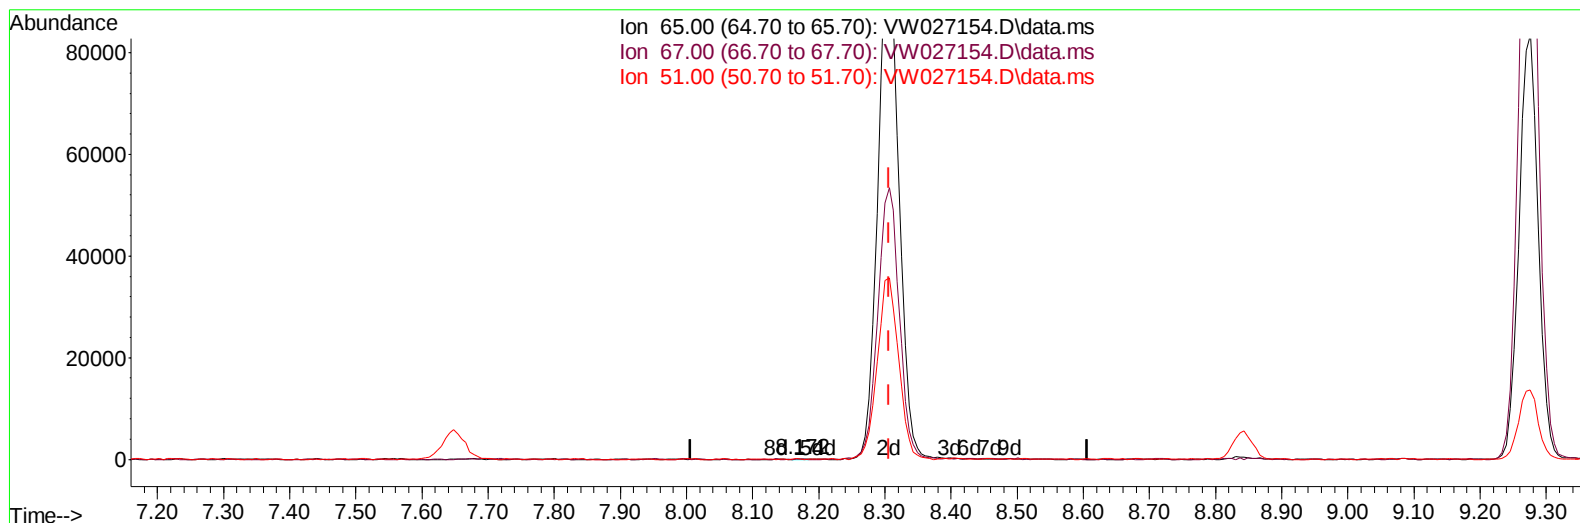

TIC: VW027154.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.172min (-0.134) 0.01 ug/L

response 110

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.30	66.36
51.00	101.20	120.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027154.D
 Acq On : 19 Sep 2023 17:51
 Operator : SY/MD
 Sample : 04472-15RE
 Misc : 5.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:38:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

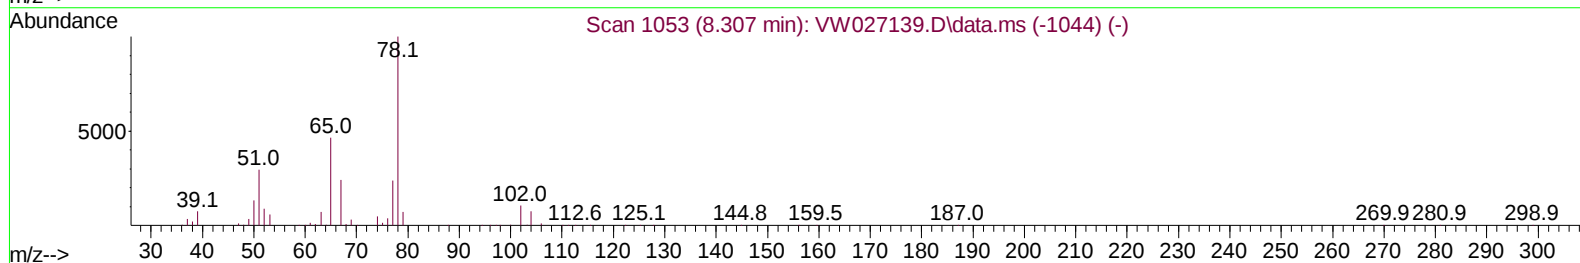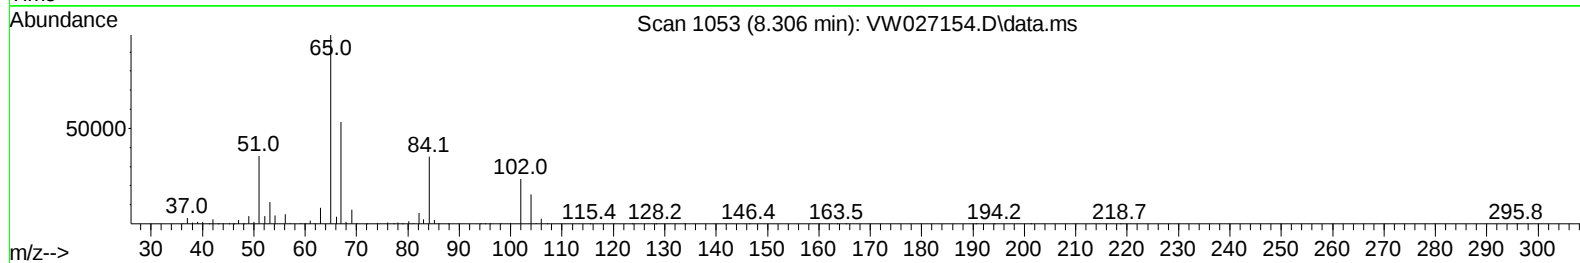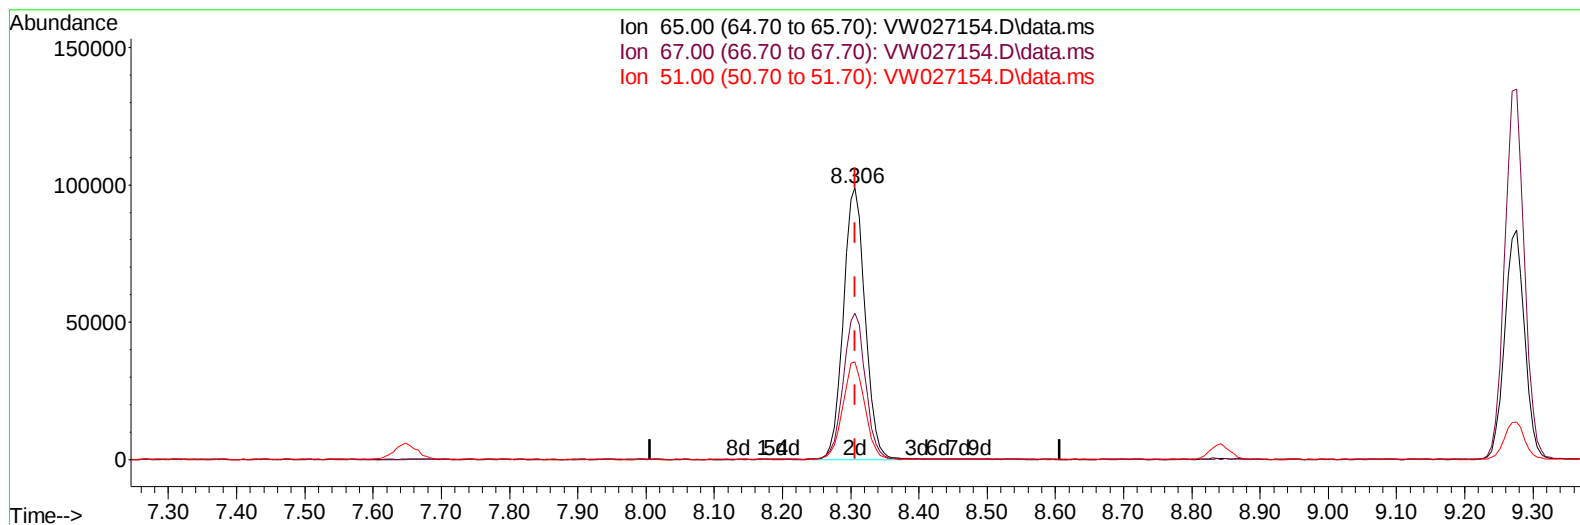

TIC: VW027154.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.306min (-0.000) 22.57 ug/L m

response 218365

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.30	0.03#
51.00	101.20	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027154.D
 Acq On : 19 Sep 2023 17:51
 Operator : SY/MD
 Sample : 04472-15RE
 Misc : 5.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM4RE

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:38:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		660114	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		540088	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152		106906	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		147381	13.876	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	55.520%		
7) Chloroethane-d5	2.893	69		222494	27.127	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	108.520%		
11) 1,1-Dichloroethene-d2	4.021	65		71850	15.779	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	63.120%		
21) 2-Butanone-d5	7.075	46		110024	55.946	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	111.900%		
24) Chloroform-d	7.648	84		429733	21.669	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	86.680%		
26) 1,2-Dichloroethane-d4	8.306	65		218365m	22.566	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	90.280%		
32) Benzene-d6	8.276	84		860171	24.661	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	98.640%		
36) 1,2-Dichloropropane-d6	9.276	67		271138	27.473	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	109.880%		
41) Toluene-d8	10.324	98		645272	20.787	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	83.160%		
43) trans-1,3-Dichloroprop...	10.580	79		72612	18.207	ug/L	0.00
Spiked Amount 25.000	Range 30						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
Data File : VW027154.D
Acq On : 19 Sep 2023 17:51
Operator : SY/MD
Sample : 04472-15RE
Misc : 5.51g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYM4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:38:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 20 01:34:37 2023
Response via : Initial Calibration

