

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027156.D
 Acq On : 19 Sep 2023 18:39
 Operator : SY/MD
 Sample : 04472-16RE
 Misc : 6.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYM5RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:39:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	634754	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	436972	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	143130	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	112399	11.006	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	44.040%
7) Chloroethane-d5	2.887	69	155731	19.746	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.000%
11) 1,1-Dichloroethene-d2	4.021	65	48916	11.172	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	44.680%#
21) 2-Butanone-d5	7.075	46	118611	62.722	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.440%
24) Chloroform-d	7.648	84	311352	16.327	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.320%
26) 1,2-Dichloroethane-d4	8.306	65	184312	19.808	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.240%
32) Benzene-d6	8.270	84	576103	20.415	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.640%
36) 1,2-Dichloropropane-d6	9.270	67	190406	23.845	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.400%
41) Toluene-d8	10.324	98	347061	13.818	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	55.280%
43) trans-1,3-Dichloroprop...	10.580	79	67356	20.874	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.480%
47) 2-Hexanone-d5	10.922	63	65236	67.800	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	135.600%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	212034	33.140	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	132.560%#
66) 1,2-Dichlorobenzene-d4	13.848	152	69488	13.595	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	54.360%#
Target Compounds					Qvalue	
13) Acetone	4.118	43	30207	16.908	ug/L	100
16) Methylene chloride	4.917	84	62805	5.201	ug/L	92
22) 2-Butanone	7.173	43	12988m	5.382	ug/L	
35) Methylcyclohexane	9.337	83	12506	0.961	ug/L	96
53) m,p-Xylene	11.830	106	23281	1.815	ug/L	84
54) o-Xylene	12.159	106	11850	0.970	ug/L	95
60) Isopropylbenzene	12.458	105	16153	0.842	ug/L #	88
62) 1,3,5-Trimethylbenzene	12.940	105	32103	2.092	ug/L	97
63) 1,2,4-Trimethylbenzene	13.245	105	64395	4.331	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
Data File : VW027156.D
Acq On : 19 Sep 2023 18:39
Operator : SY/MD
Sample : 04472-16RE
Misc : 6.95g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EZYM5RE

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 09/20/2023
Supervised By : Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:39:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 20 01:34:37 2023
Response via : Initial Calibration

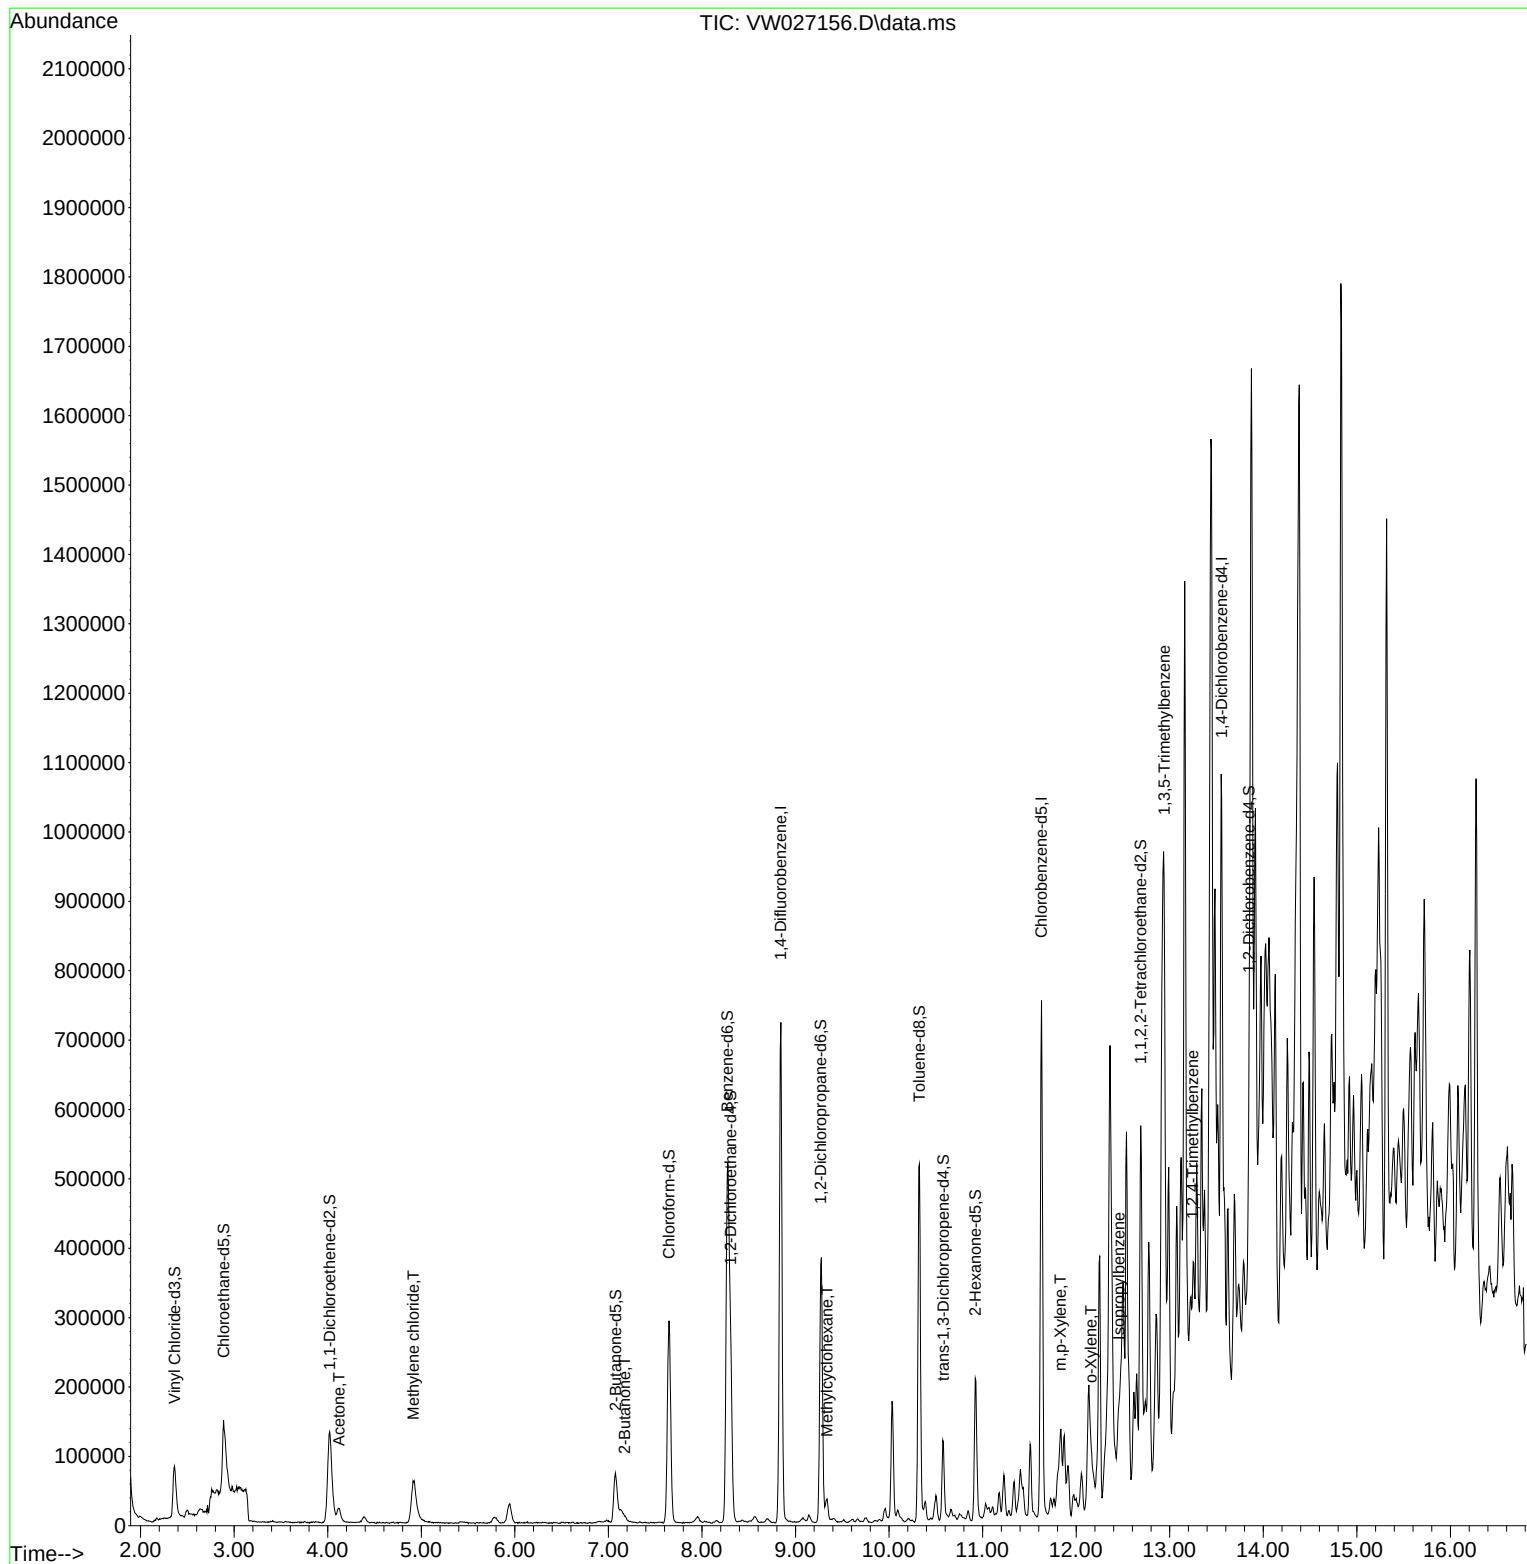

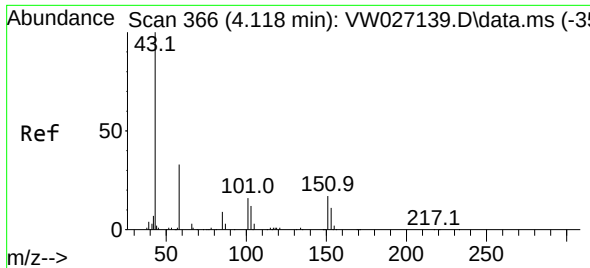

#13

Acetone

Concen: 16.908 ug/L

RT: 4.118 min Scan# 3020

Delta R.T. -0.000 min

Lab File: VW027156.D

Acq: 19 Sep 2023 18:39

Instrument :

MSVOA_W

ClientSampleId :





EZYM5RE

Tgt Ion: 43 Resp: 3020
 Ion Ratio Lower Upper
 43 100
 58 38.8 0.0 77.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

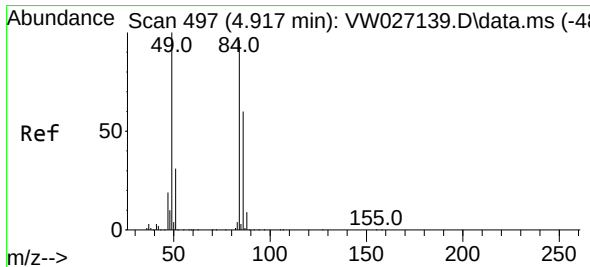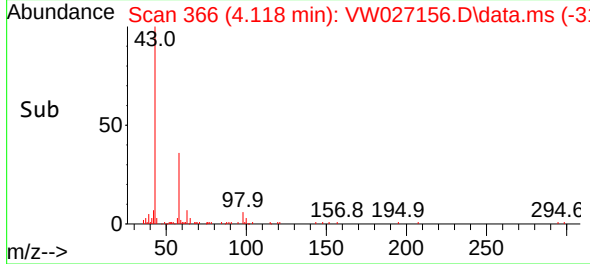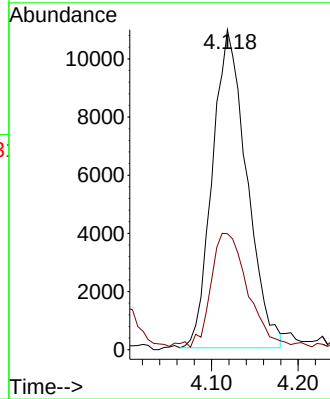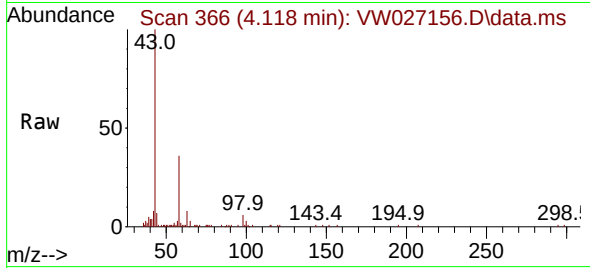

#16

Methylene chloride

Concen: 5.201 ug/L




RT: 4.917 min Scan# 497


Delta R.T. -0.000 min

Lab File: VW027156.D

Acq: 19 Sep 2023 18:39


Tgt Ion: 84 Resp: 62805
 Ion Ratio Lower Upper
 84 100
 86 57.4 46.7 86.7
 49 104.2 77.1 143.1

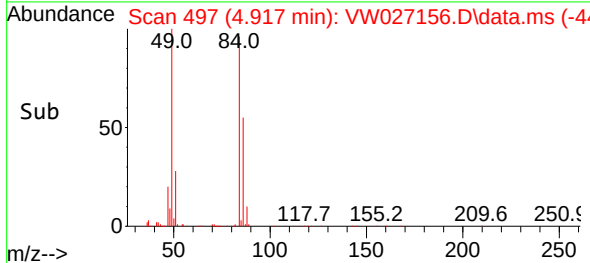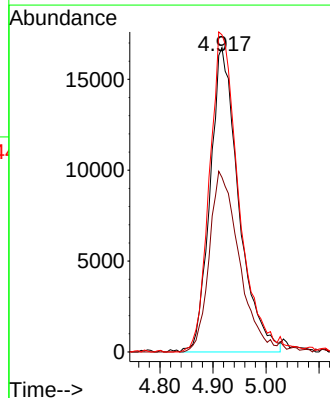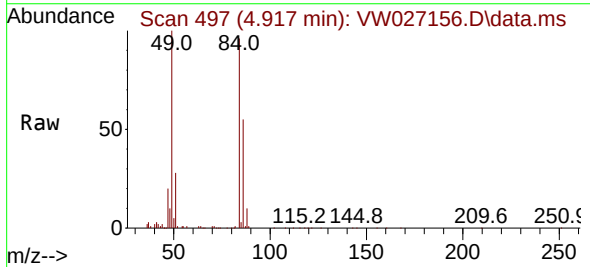

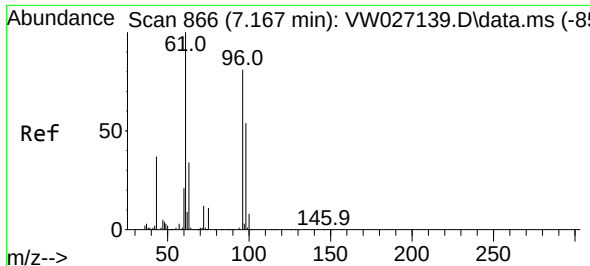

#22
2-Butanone
Concen: 5.382 ug/L m
RT: 7.173 min Scan# 867
Delta R.T. 0.006 min
Lab File: VW027156.D
Acq: 19 Sep 2023 18:39




Instrument :
MSVOA_W
ClientSampleId :
EZYM5RE

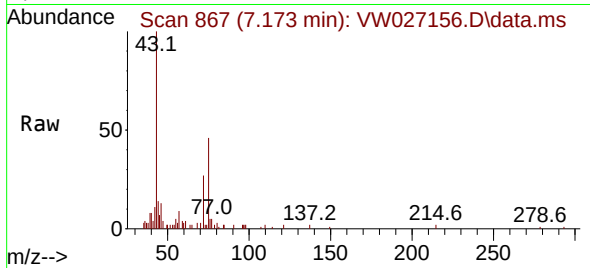

Tgt Ion: 43 Resp: 1298
Ion Ratio Lower Upper
43 100
72 0.8 16.8 50.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

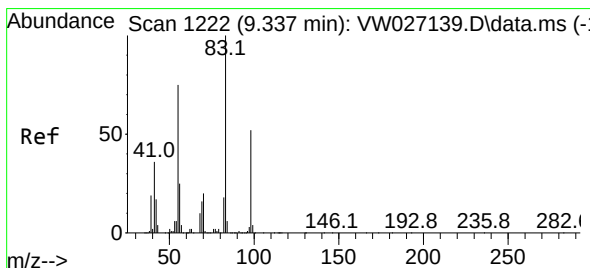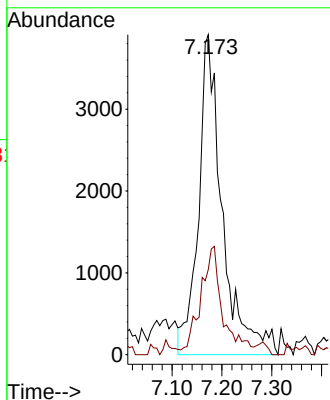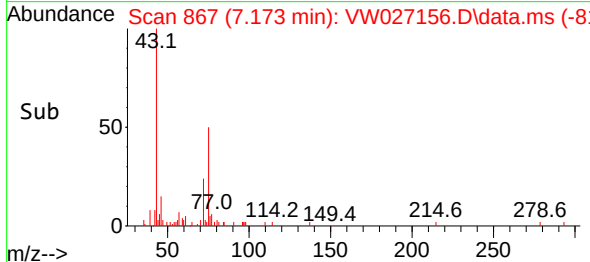

#35
Methylcyclohexane
Concen: 0.961 ug/L
RT: 9.337 min Scan# 1222
Delta R.T. -0.000 min
Lab File: VW027156.D
Acq: 19 Sep 2023 18:39

Tgt Ion: 83 Resp: 12506
Ion Ratio Lower Upper
83 100
55 76.4 58.0 87.0
98 50.2 38.5 57.7

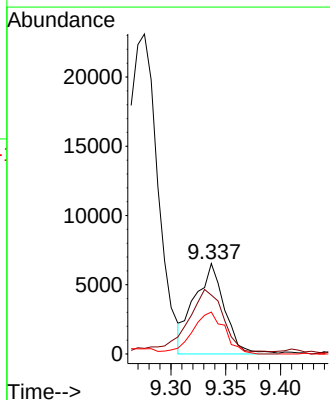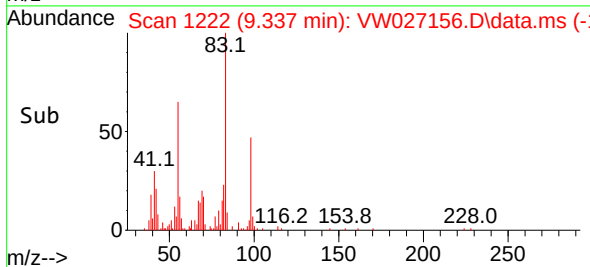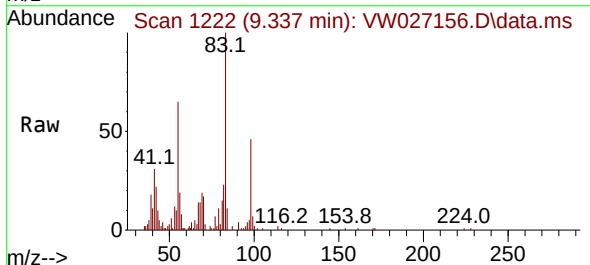

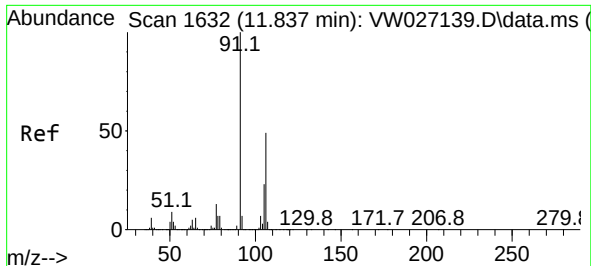





#53
m,p-Xylene
Concen: 1.815 ug/L
RT: 11.830 min Scan# 1631
Delta R.T. -0.006 min
Lab File: VW027156.D
Acq: 19 Sep 2023 18:39

Instrument :
MSVOA_W
ClientSampleId :
EZYMSRE

Tgt Ion:106 Resp: 2328
Ion Ratio Lower Upper
106 100
91 178.9 142.7 265.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

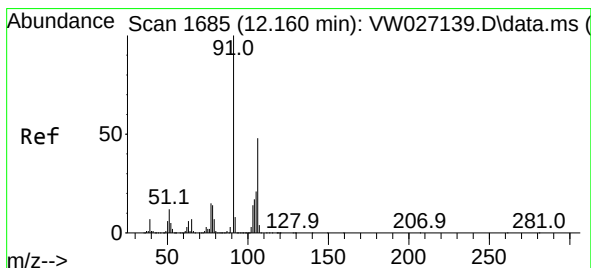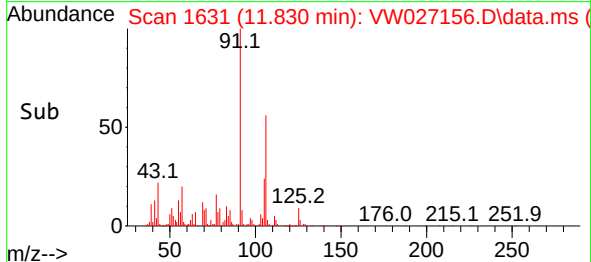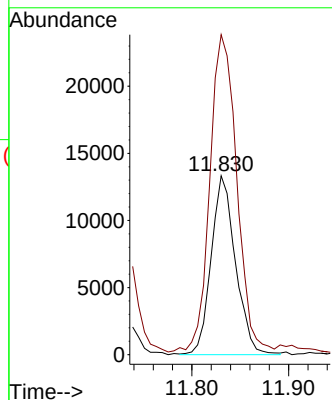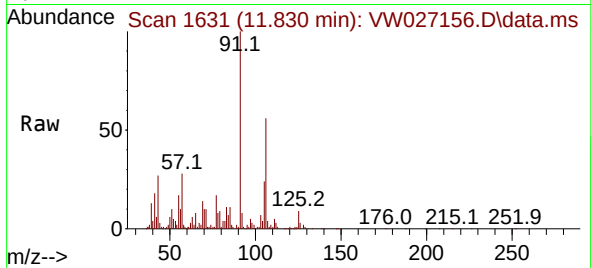

#54
o-Xylene
Concen: 0.970 ug/L
RT: 12.159 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VW027156.D
Acq: 19 Sep 2023 18:39

Tgt Ion:106 Resp: 11850
Ion Ratio Lower Upper
106 100
91 208.8 140.6 261.0

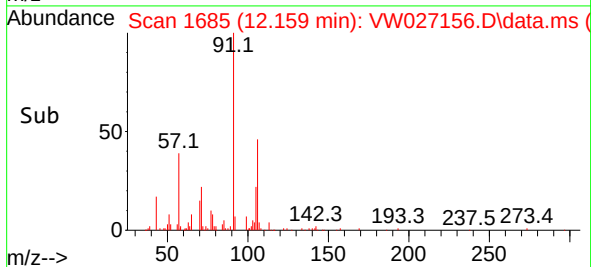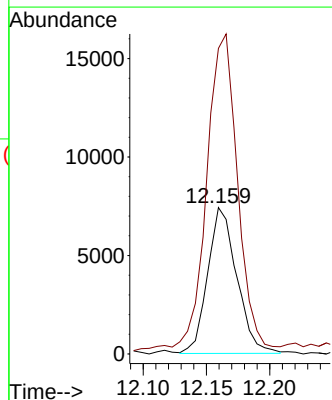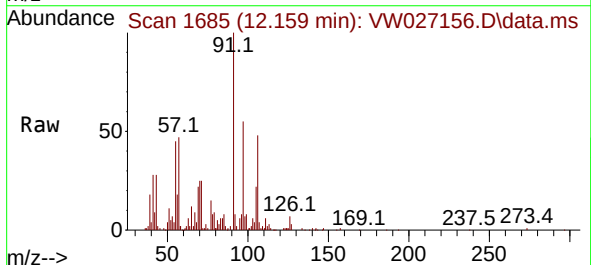

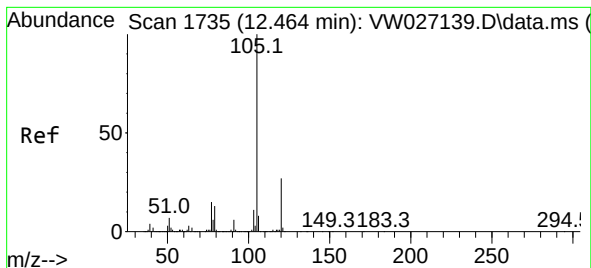

#60

Isopropylbenzene

Concen: 0.842 ug/L

RT: 12.458 min Scan# 1

Delta R.T. -0.006 min

Lab File: VW027156.D

Acq: 19 Sep 2023 18:39

Instrument :

MSVOA_W

ClientSampleId :





EZYM5RE

Tgt Ion:	105	Resp:	1615
Ion Ratio	Lower	Upper	
105	100		
120	28.2	21.0	31.4
77	26.2	12.0	18.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

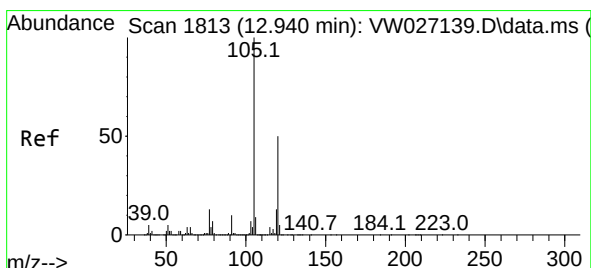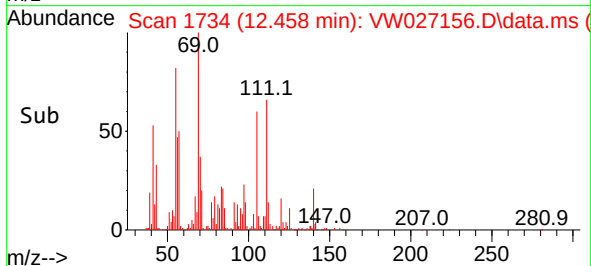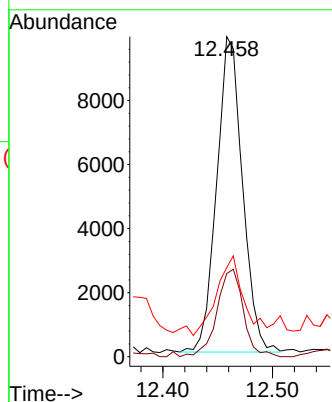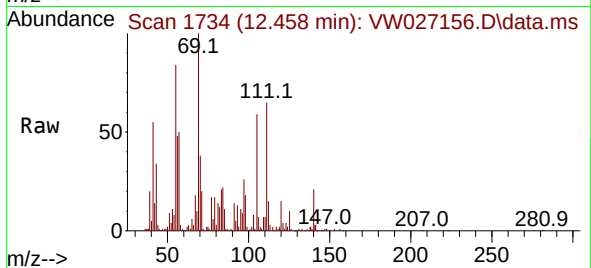

#62

1,3,5-Trimethylbenzene

Concen: 2.092 ug/L




RT: 12.940 min Scan# 1813


Delta R.T. -0.000 min

Lab File: VW027156.D

Acq: 19 Sep 2023 18:39


Tgt Ion:	105	Resp:	32103
Ion Ratio	Lower	Upper	
105	100		
120	48.7	40.5	60.7

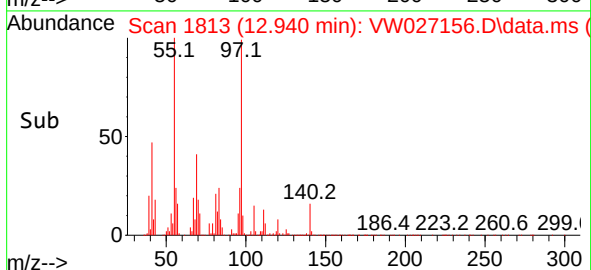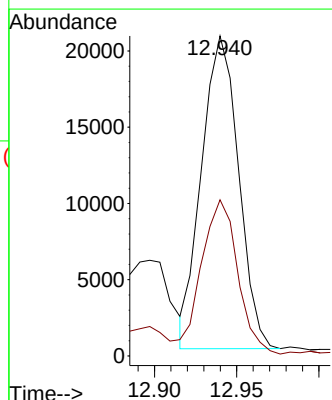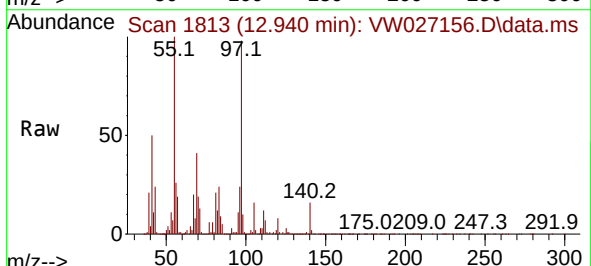

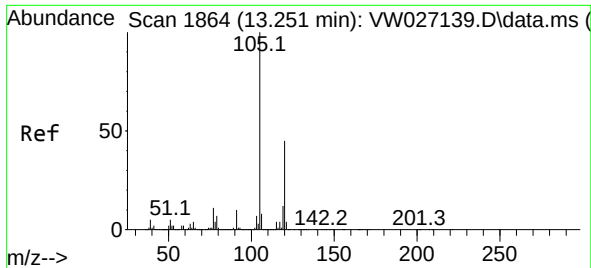

#63
1,2,4-Trimethylbenzene
Concen: 4.331 ug/L
RT: 13.245 min Scan# 1863
Delta R.T. -0.006 min
Lab File: VW027156.D
Acq: 19 Sep 2023 18:39

Instrument :
MSVOA_W
ClientSampleId :
EZYM5RE

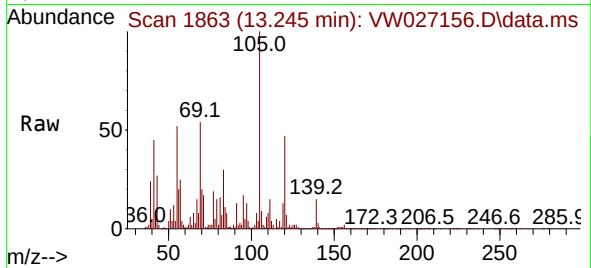

Tgt Ion:105 Resp: 6439
Ion Ratio Lower Upper
105 100
120 43.2 36.2 54.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

