

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091924\
 Data File : VW030145.D
 Acq On : 19 Sep 2024 13:58
 Operator : SY/MD
 Sample : P4083-08
 Misc : 5.73g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 20 01:30:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 20 01:21:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	385964	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	274468	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	67434	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	75067	15.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.240%
7) Chloroethane-d5	2.893	69	57434	16.322	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.280%
11) 1,1-Dichloroethene-d2	4.021	65	38957	15.643	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.560%
21) 2-Butanone-d5	7.075	46	36681	30.392	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.780%
24) Chloroform-d	7.648	84	184235	17.360	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.440%
26) 1,2-Dichloroethane-d4	8.307	65	97067	18.214	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.840%
32) Benzene-d6	8.270	84	352653	22.303	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	9.270	67	112126	22.968	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.880%
41) Toluene-d8	10.319	98	286136	20.194	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.760%
43) trans-1,3-Dichloroprop...	10.575	79	39986	20.444	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.760%
47) 2-Hexanone-d5	10.922	63	30704	41.101	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66293	18.240	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.960%
66) 1,2-Dichlorobenzene-d4	13.849	152	43863	19.161	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	76.640%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2765	0.416	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091924\
Data File : VW030145.D
Acq On : 19 Sep 2024 13:58
Operator : SY/MD
Sample : P4083-08
Misc : 5.73g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 20 01:30:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 20 01:21:33 2024
Response via : Initial Calibration

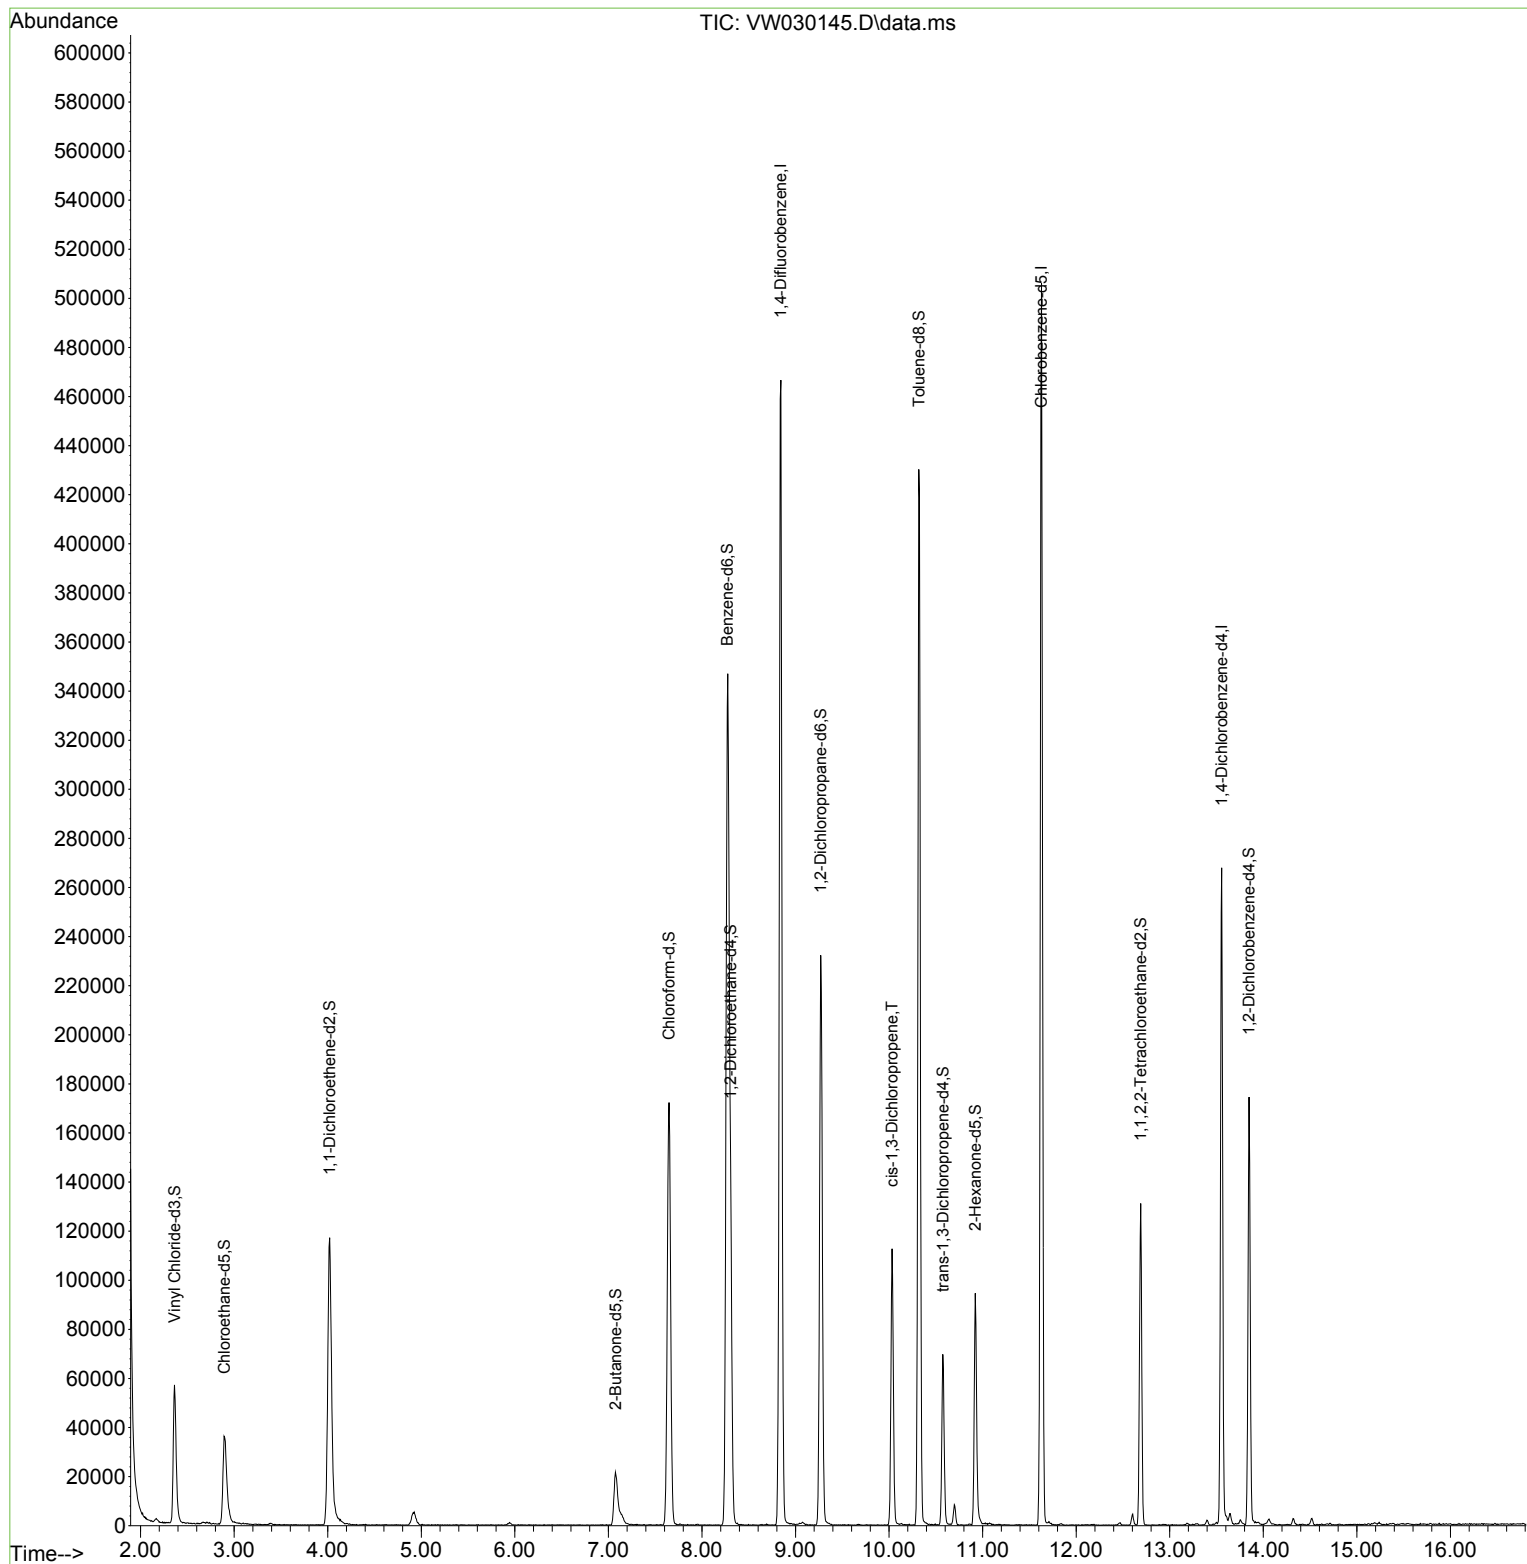

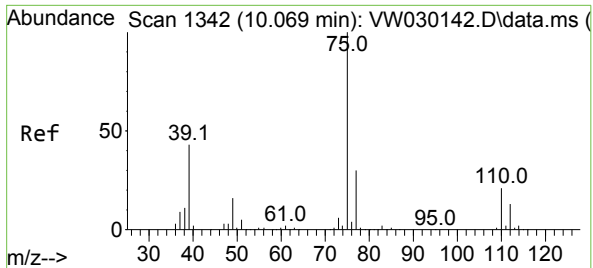

#39
cis-1,3-Dichloropropene
Concen: 0.416 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.036 min
Lab File: VW030145.D
Acq: 19 Sep 2024 13:58

Instrument :
MSVOA_W
ClientSampleId :

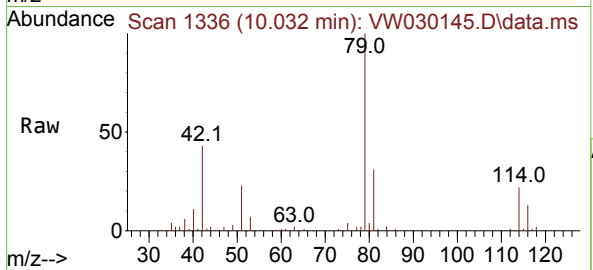

Tgt Ion: 75 Resp: 2765
Ion Ratio Lower Upper
75 100
77 46.8 20.7 38.5#

