


Data File : VW005536.D
Acq On : 20 Sep 2018 15:51
Operator : SY/AP
Sample : J4970-06
Misc : 5.71G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 03:20:42 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091918S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 21 01:00:52 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
E5FD8

Manual Integrations
APPROVED

MMDadoda
9/24/2018 10:40:37 AM

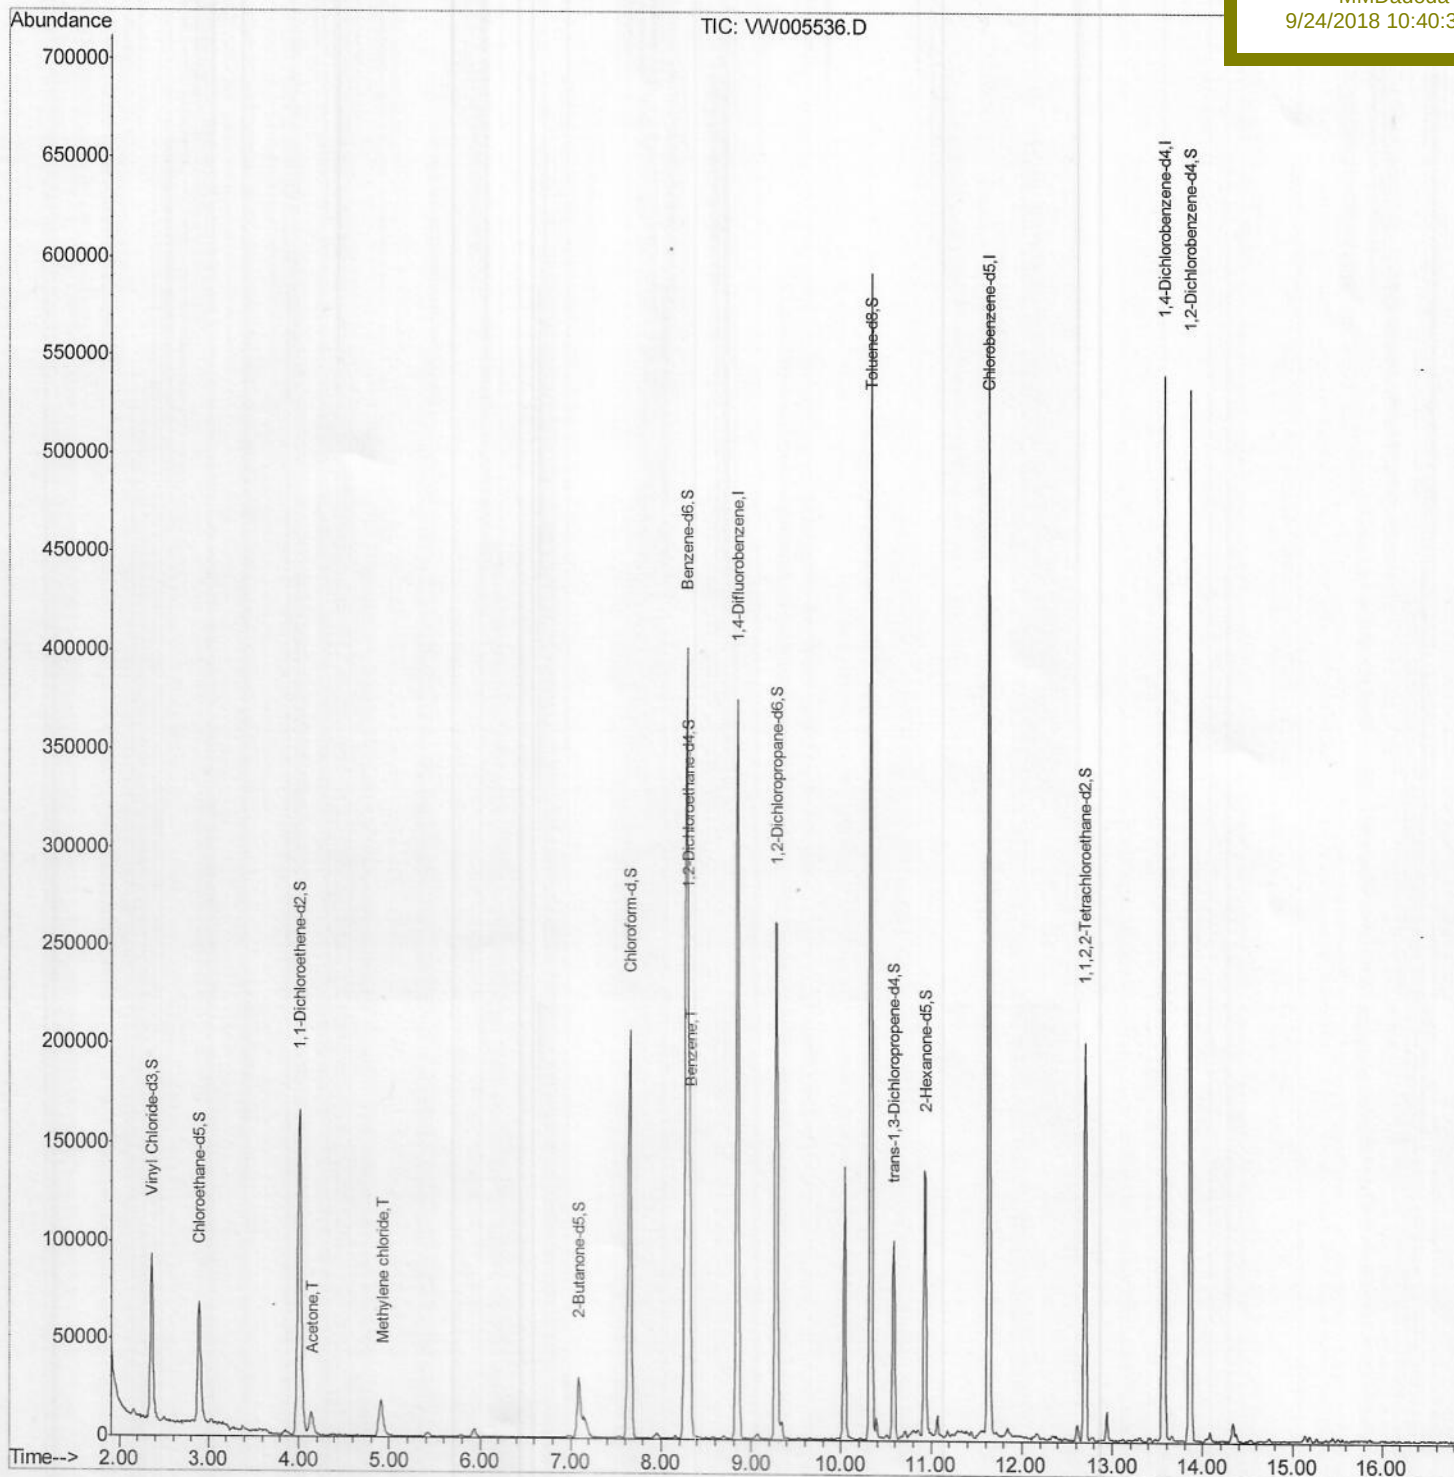

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092018\

Data File : VW005536.D

Acq On : 20 Sep 2018 15:51

Operator : SY/AP

Sample : J4970-06

Misc : 5.71G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 01:01:56 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091918S.M

Quant Title : VOC Analysis

QLast Update : Fri Sep 21 01:00:52 2018

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :




E5FD8

Manual Integrations

APPROVED

MMDadoda

9/24/2018 10:40:37 AM

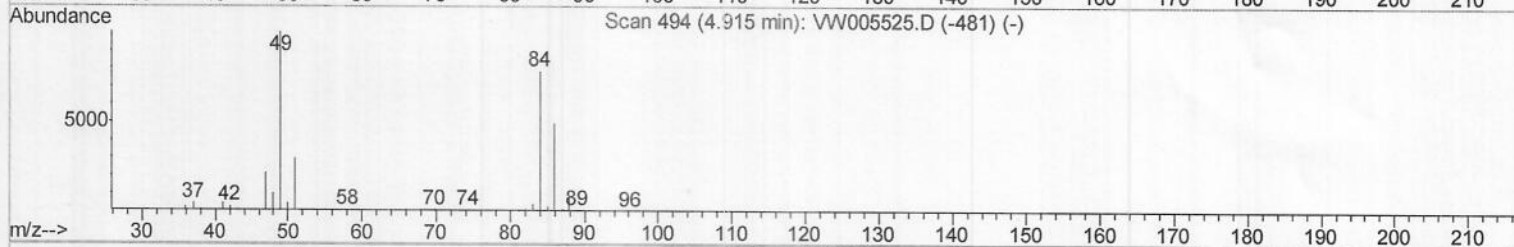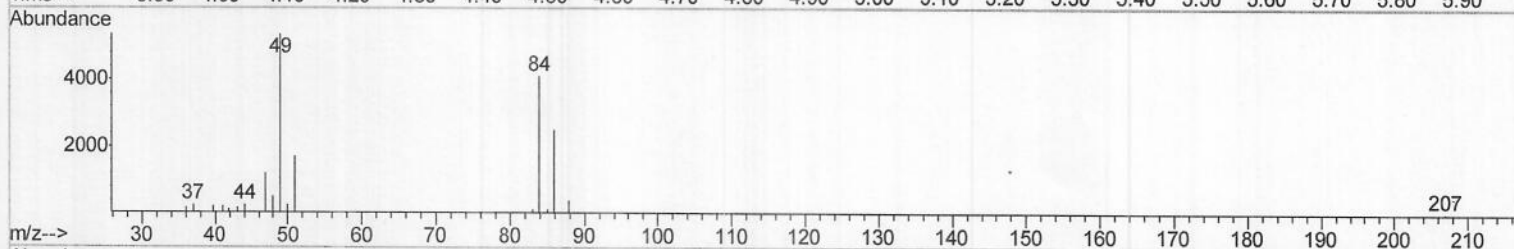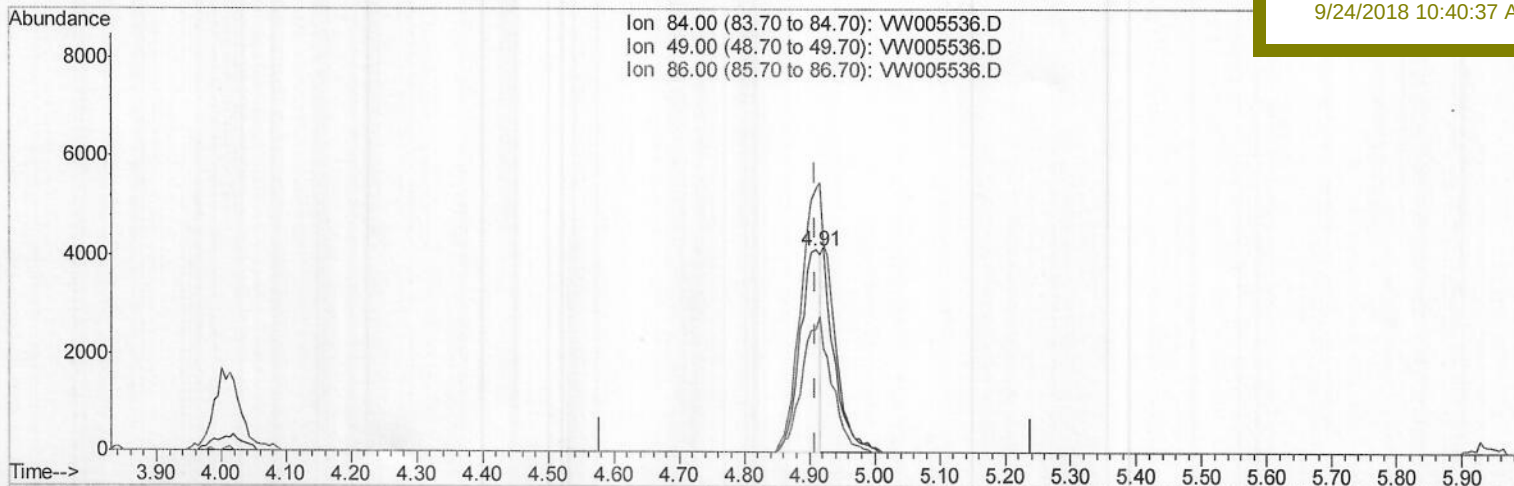

(16) Methylene chloride (T)

4.909min (-0.000) 1.73ug/L

response 8802

Ion	Exp%	Act%
84.00	100	100
49.00	130.70	129.77
86.00	64.00	60.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092018\
Data File : VW005536.D
Acq On : 20 Sep 2018 15:51
Operator : SY/AP
Sample : J4970-06
Misc : 5.71G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 01:01:56 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091918S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 21 01:00:52 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
E5FD8

Manual Integrations
APPROVED

MMDadoda
9/24/2018 10:40:37 AM

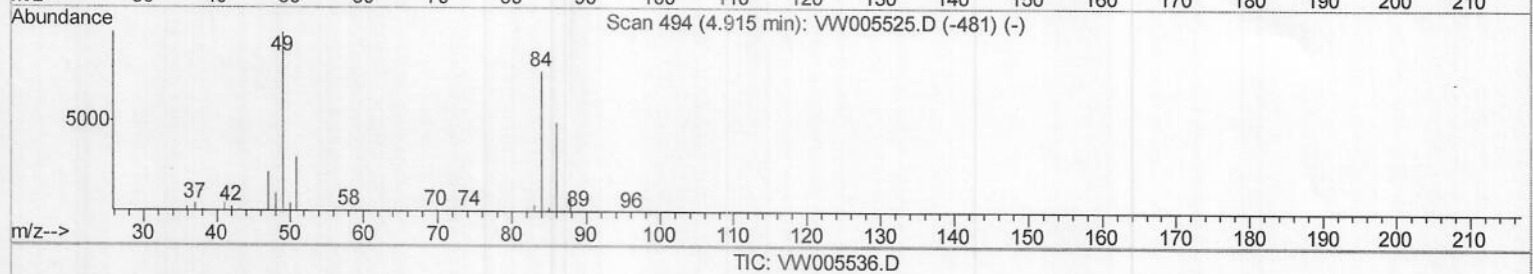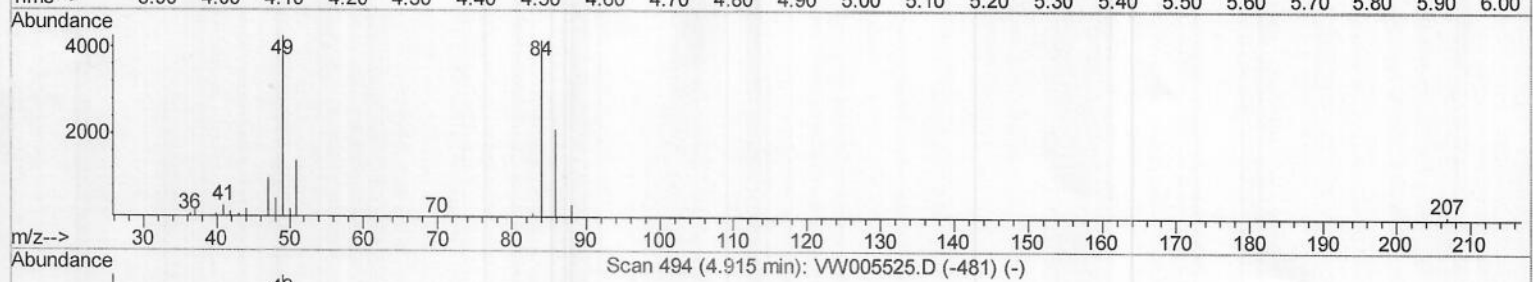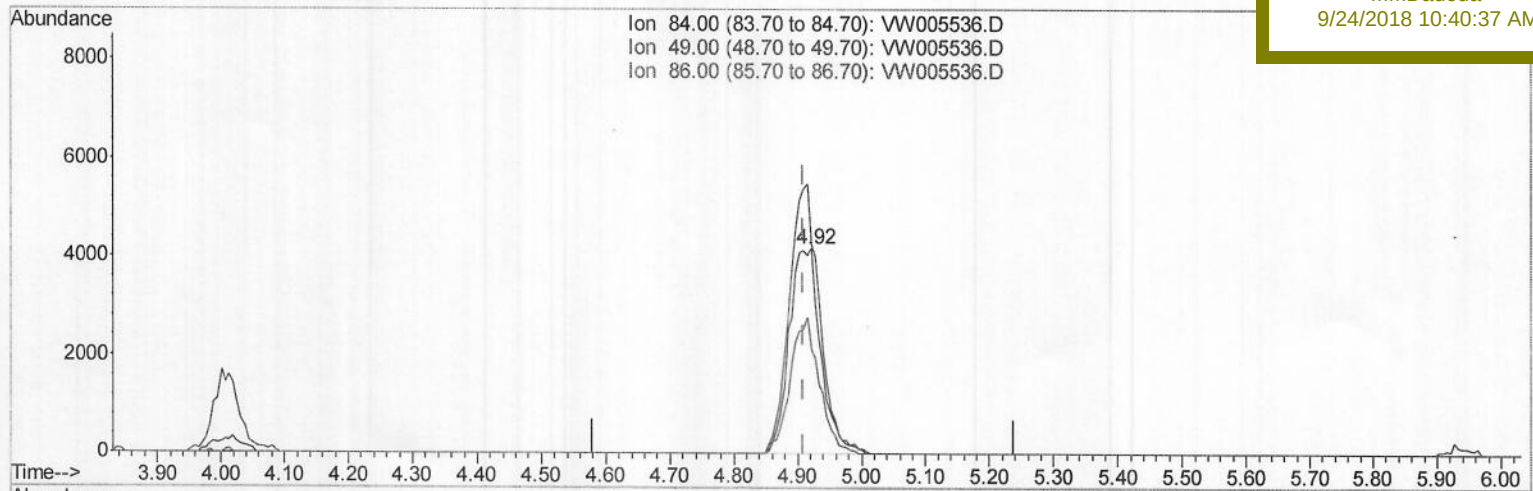

(16) Methylene chloride (T)

4.921min (+0.012) 2.82ug/L m) MD10/04/18

response 14348

Ion	Exp%	Act%
84.00	100	100
49.00	130.70	102.30
86.00	64.00	50.59
0.00	0.00	0.00

Data File : VW005536.D
Acq On : 20 Sep 2018 15:51
Operator : SY/AP
Sample : J4970-06
Misc : 5.71G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
E5FD8

Quant Time: Oct 04 03:20:42 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091918S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 21 01:00:52 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/24/2018 10:40:37 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.85	114	307196	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	300580	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	140911	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	109196	26.40	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	105.60%		
7) Chloroethane-d5	2.89	69	85445	25.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	103.68%		
10) 1,1-Dichloroethene-d2	4.01	63	177062	19.45	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	77.80%		
20) 2-Butanone-d5	7.09	46	52463	32.50	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	65.00%		
24) Chloroform-d	7.65	84	211490	25.36	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	101.44%		
26) 1,2-Dichloroethane-d4	8.31	65	125588	25.02	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.08%		
29) Benzene-d6	8.28	84	399887	22.50	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.00%		
33) 1,2-Dichloropropane-d6	9.27	67	117321	21.67	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.68%		
37) Toluene-d8	10.33	98	383200	23.43	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.72%		
38) trans-1,3-Dichloropropene-	10.58	79	54958	22.13	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.52%		
39) 2-Hexanone-d5	10.93	63	41559	32.86	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	65.72%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	96535	19.74	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	78.96%		
61) 1,2-Dichlorobenzene-d4	13.86	152	139860	25.62	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.48%		

Target Compounds

					Qvalue
13) Acetone	4.14	43	19394	14.033 ug/L	100
16) Methylene chloride	4.92	84	14348m)	2.824 ug/L	
34) Benzene	8.32	78	15455	0.852 ug/L	100

JMD10/04/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed