



2,2-Dichloropropane

Response Ratio

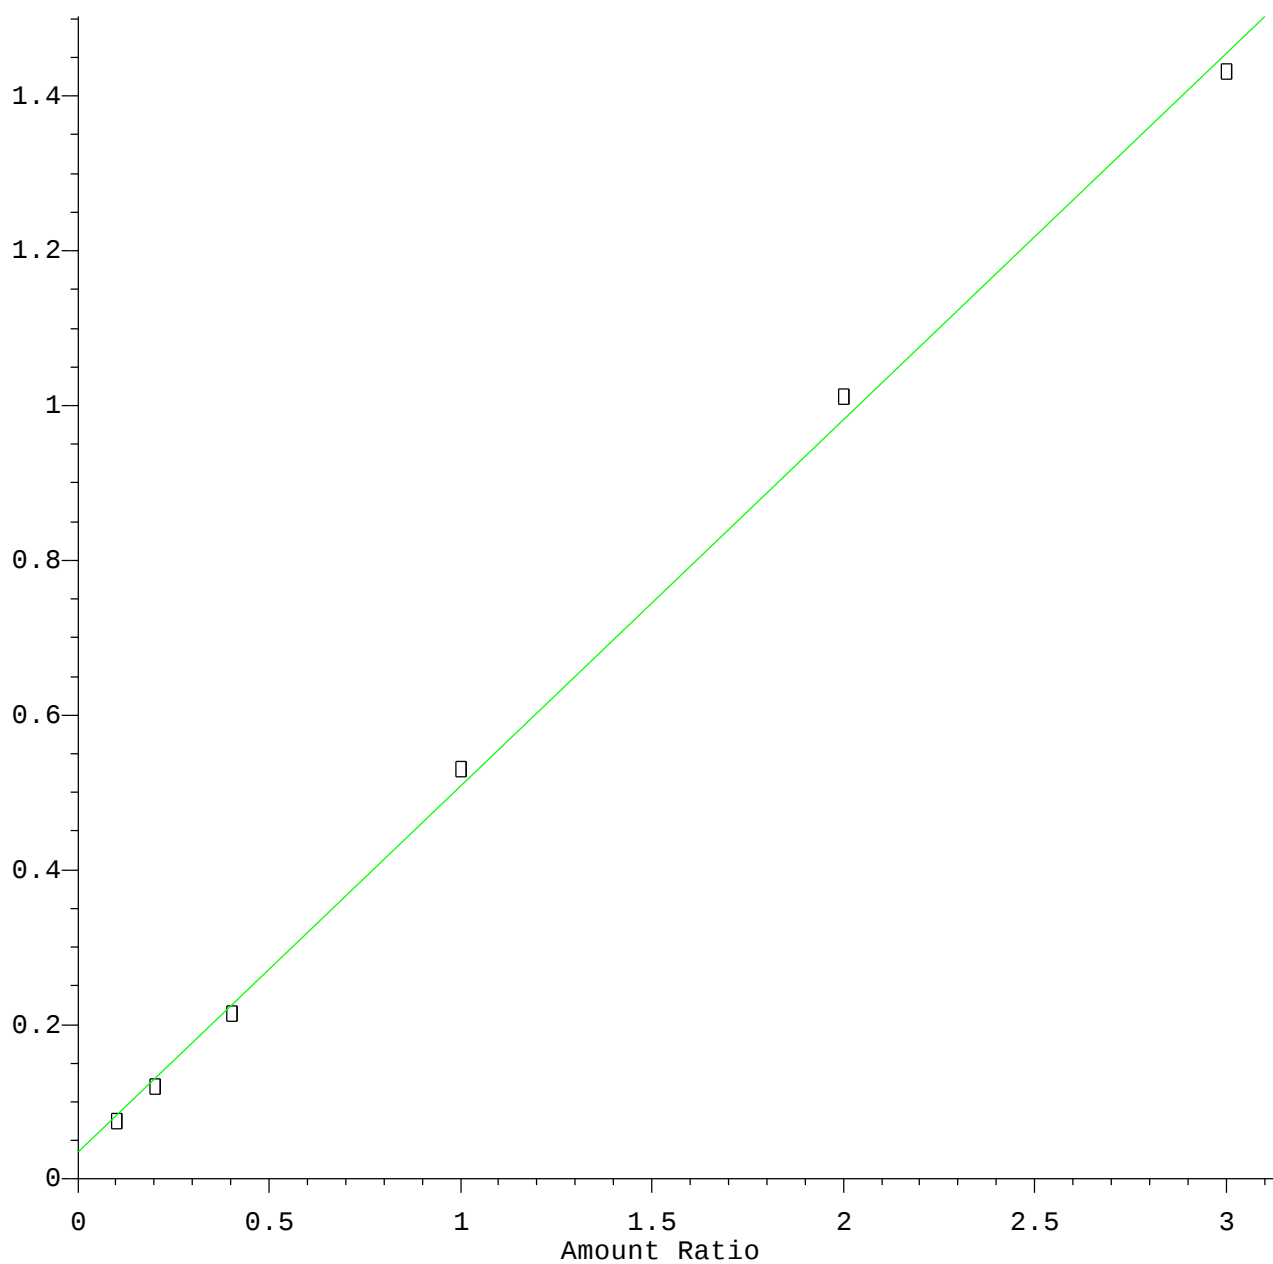

Resp Ratio = $4.74 \times 10^{-1} \times \text{Amt} + 3.38 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092019S.M
Calibration Table Last Updated: Fri Sep 20 15:58:08 2019

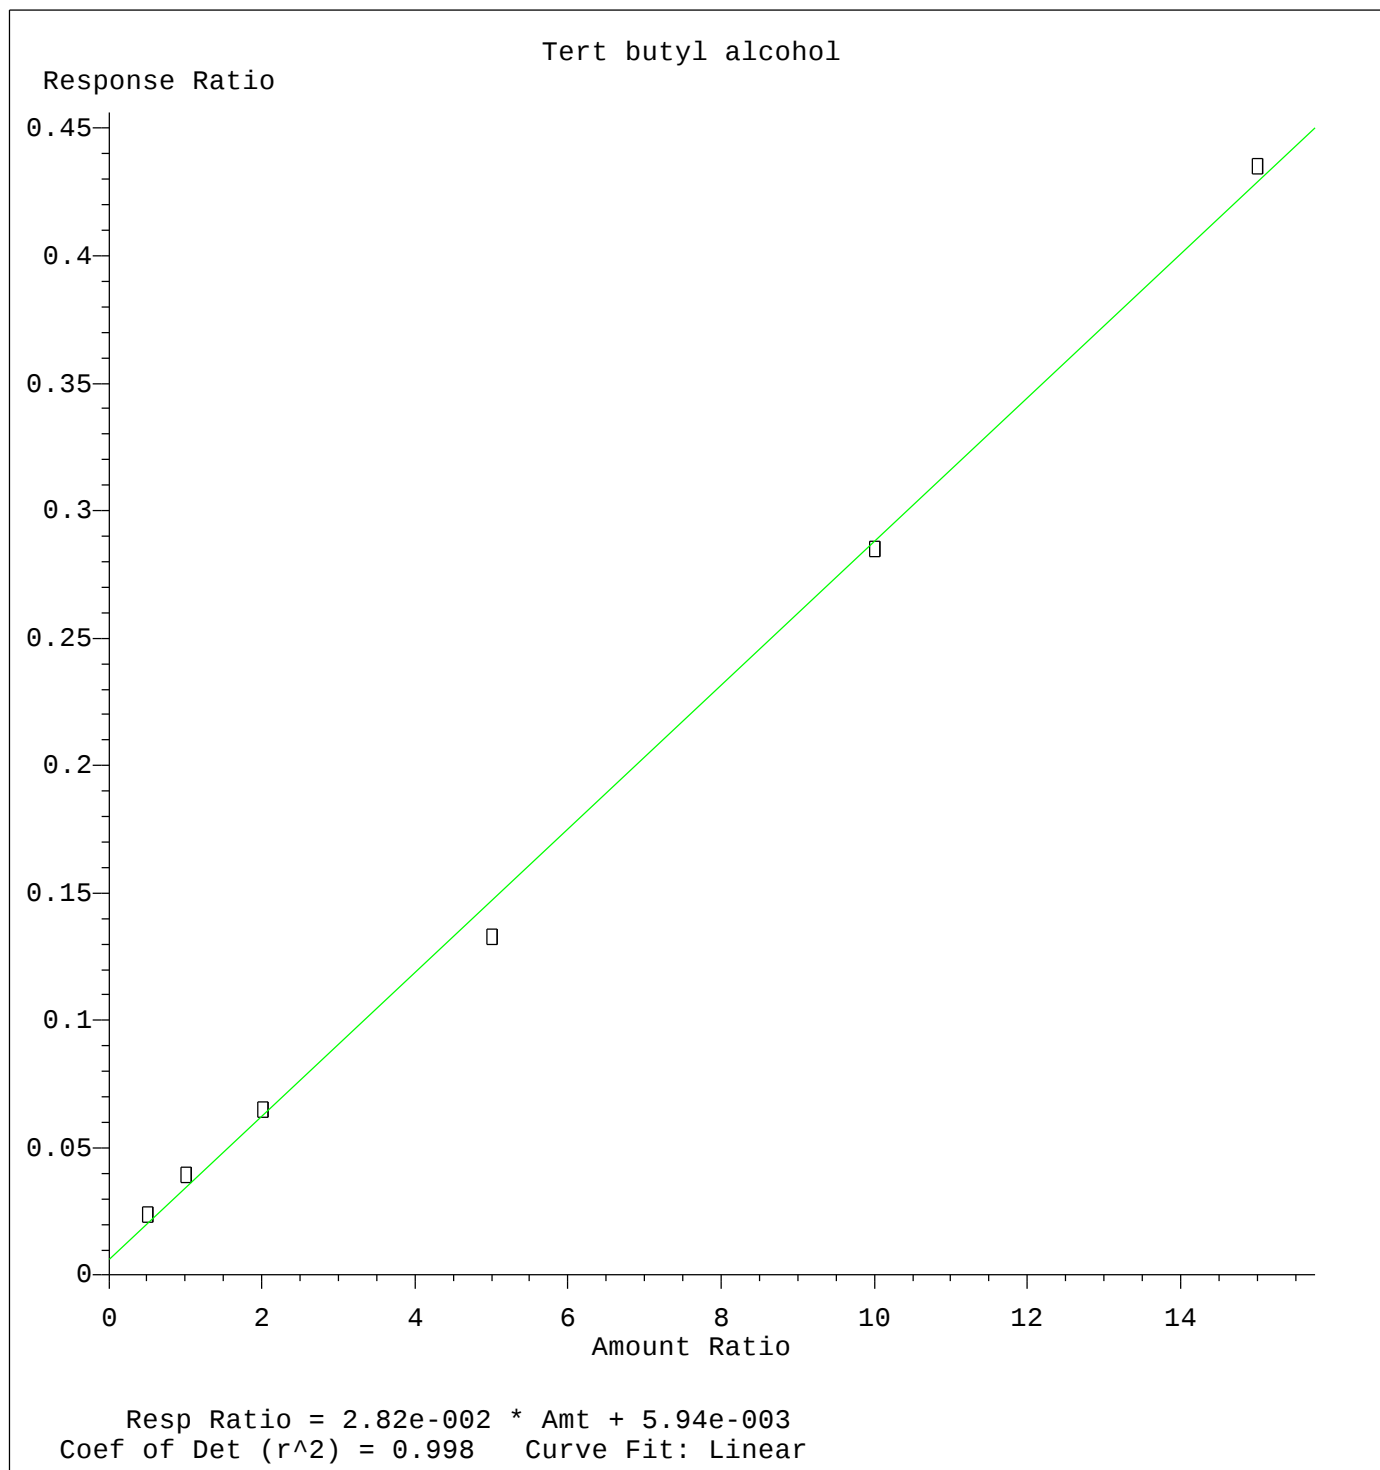

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092019S.M
Calibration Table Last Updated: Fri Sep 20 15:58:08 2019

Methylene Chloride

Response Ratio

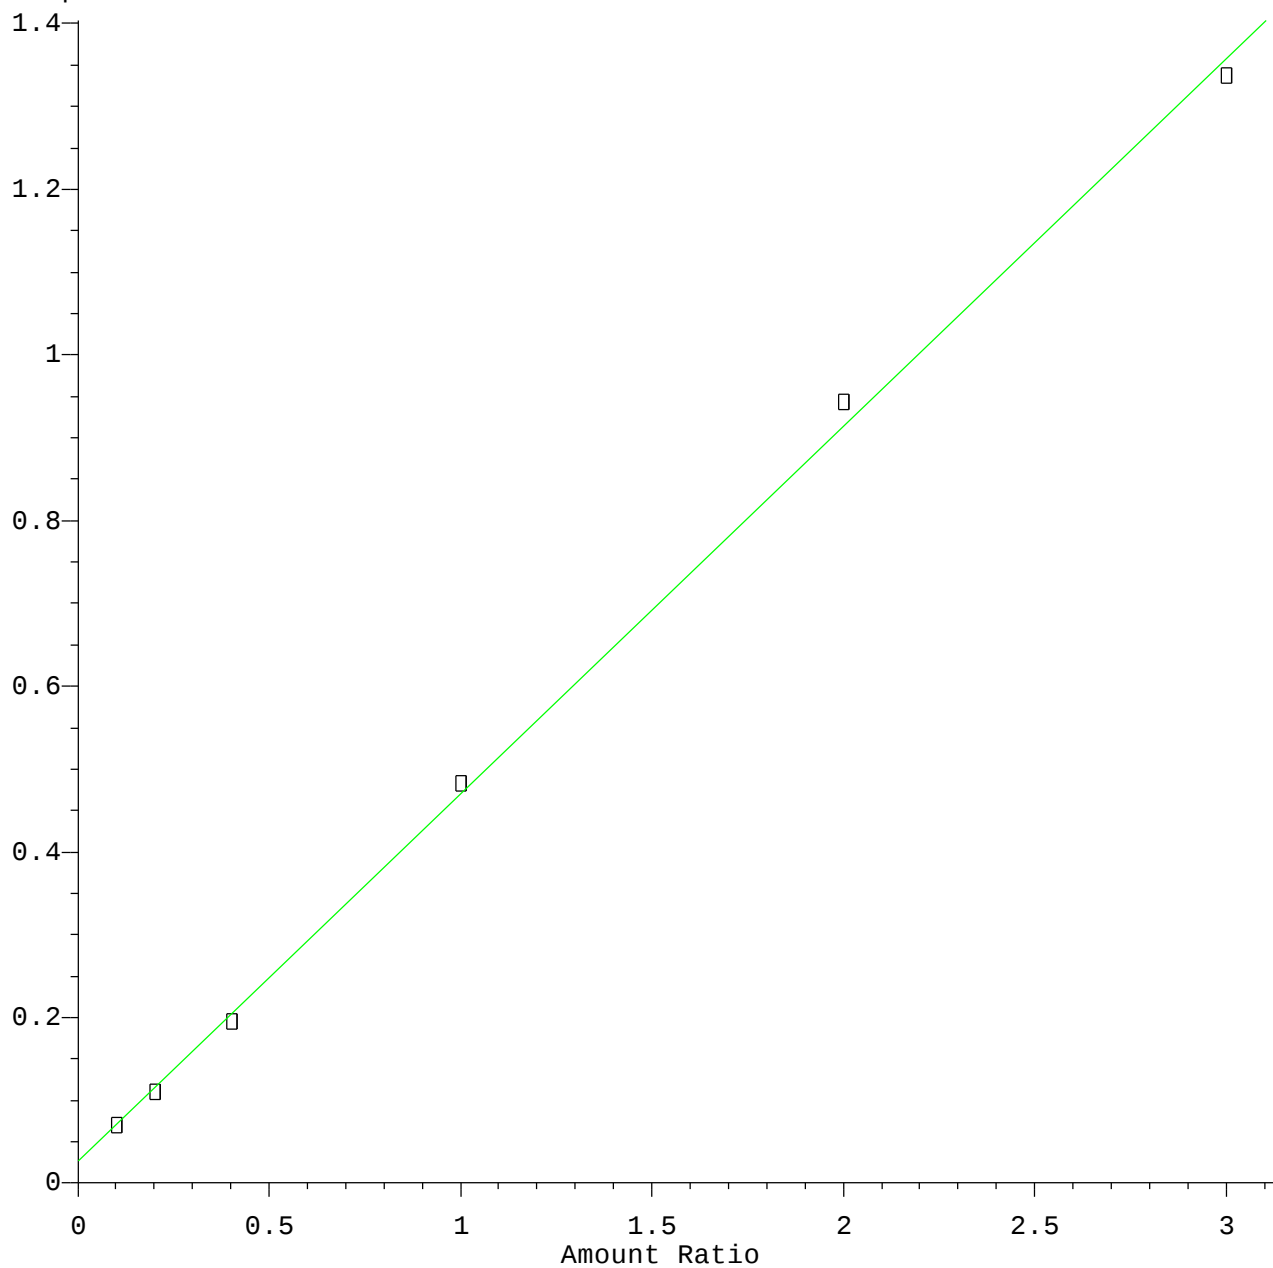

Resp Ratio = $4.43 \times 10^{-1} \times \text{Amt} + 2.73 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092019S.M
Calibration Table Last Updated: Fri Sep 20 15:58:08 2019