

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020070.D
Acq On : 20 Sep 2021 09:26
Operator : SY/VA
Sample : VW0920SBL03
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK441

Manual Integrations
APPROVED

MMDadoda
9/21/2021 6:59:59 PM

Quant Time: Sep 21 01:32:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

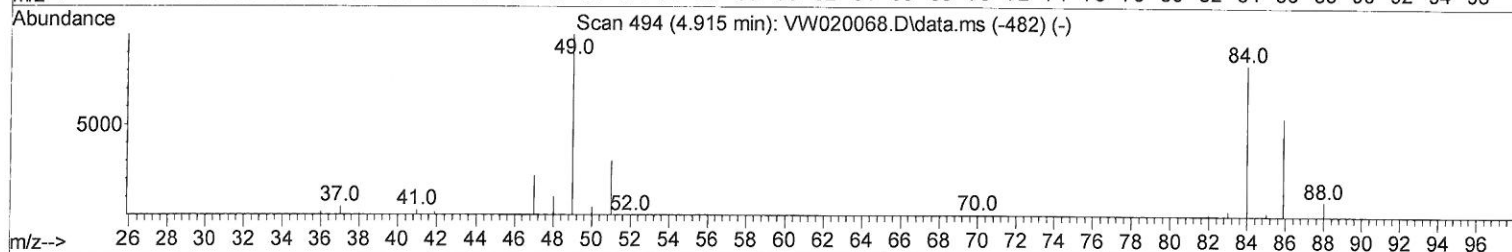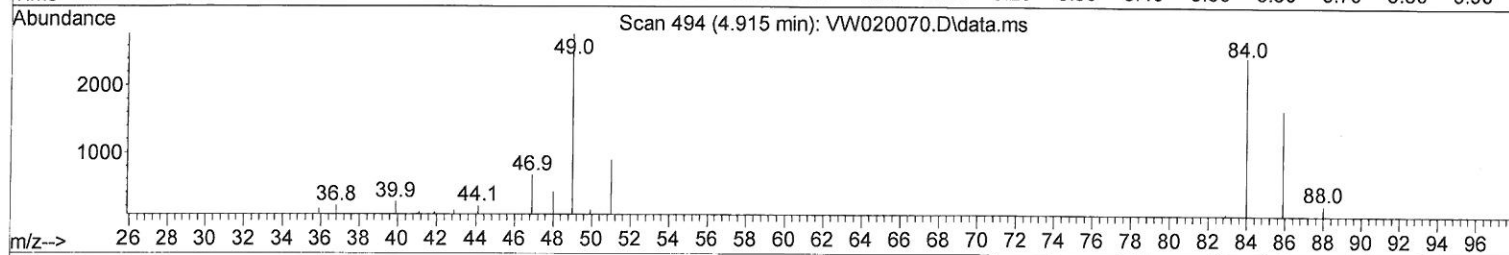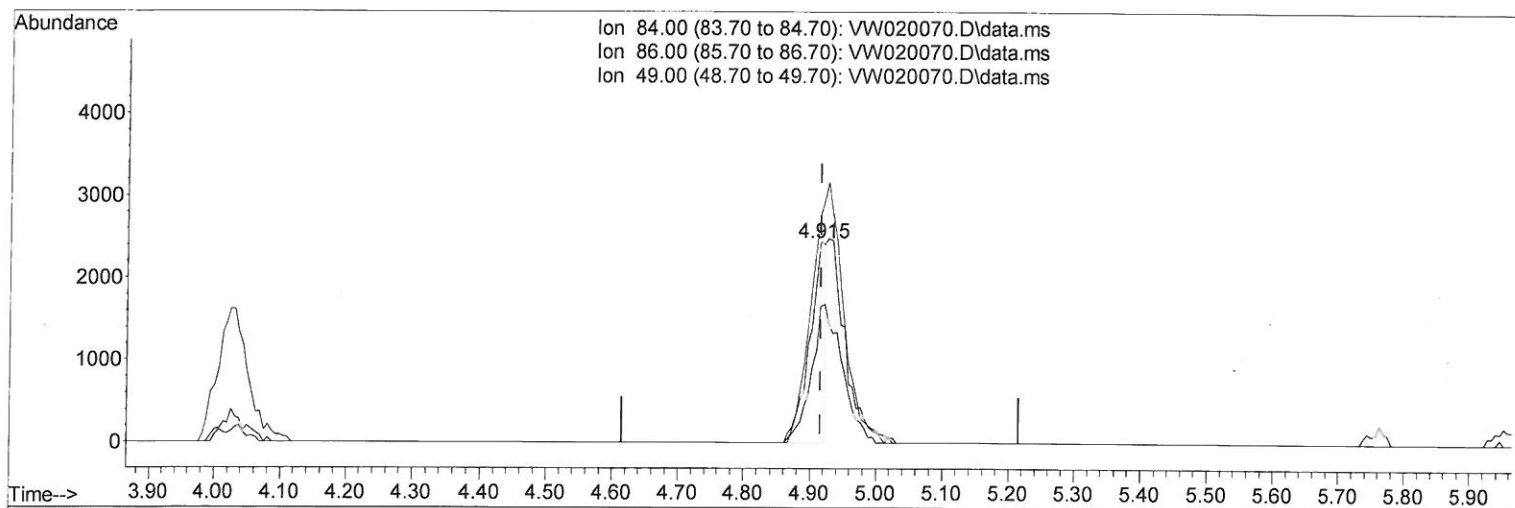

TIC: VW020070.D\data.ms

(16) Methylene chloride (T)

4.915min (+ 0.000) 0.71 ug/L

response 4057

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	67.91
49.00	123.70	113.48
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020070.D
 Acq On : 20 Sep 2021 09:26
 Operator : SY/VA
 Sample : VW0920SBL03
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK441

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 6:59:59 PM

Quant Time: Sep 21 01:32:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

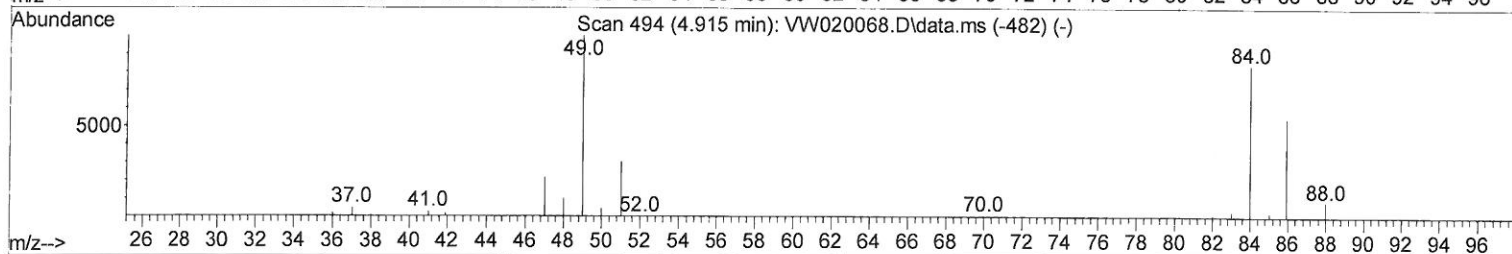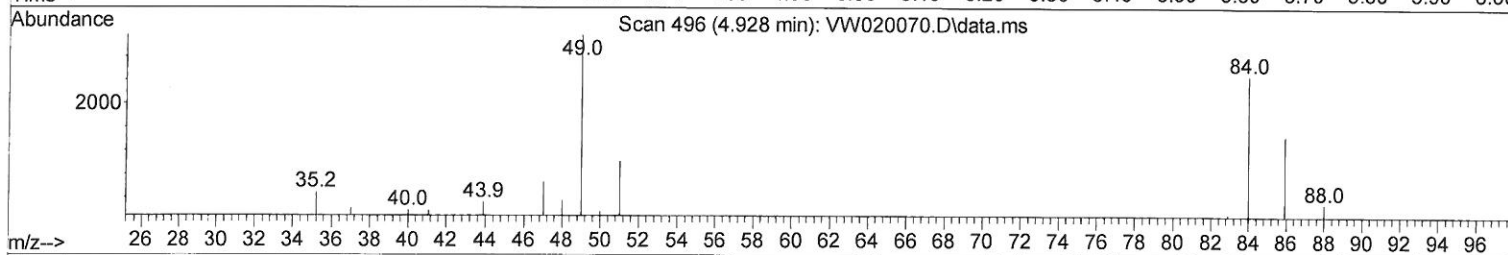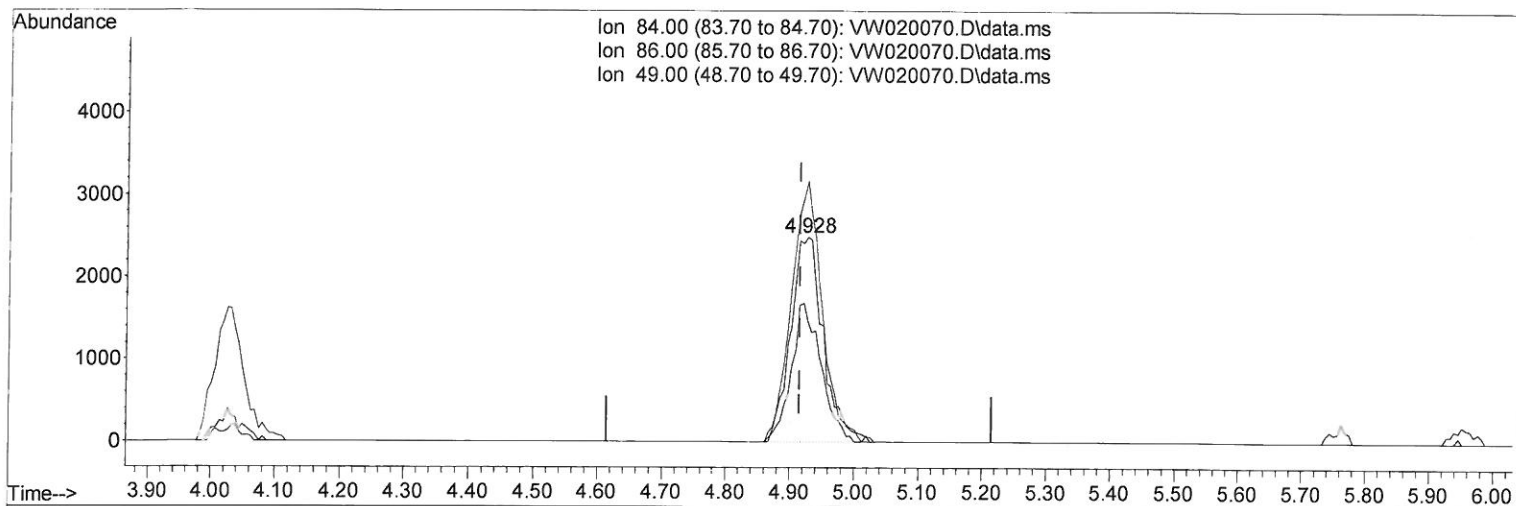

TIC: VW020070.D\data.ms

(16) Methylene chloride (T)

4.928min (+ 0.012) 1.55 ug/L m

709/24/21 SY

response 8796

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	58.96
49.00	123.70	127.09
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020070.D
 Acq On : 20 Sep 2021 09:26
 Operator : SY/VA
 Sample : VW0920SBL03
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK441

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 6:59:59 PM

Quant Time: Sep 21 01:32:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	322671	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	311813	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	138867	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	128204	24.123	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.480%		
7) Chloroethane-d5	2.898	69	103189	22.558	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.240%		
11) 1,1-Dichloroethene-d2	4.025	63	158557	18.252	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.000%		
21) 2-Butanone-d5	7.080	46	50587	34.795	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	69.580%		
24) Chloroform-d	7.653	84	229829	25.850	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	103.400%		
26) 1,2-Dichloroethane-d4	8.311	65	133282	25.447	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.800%		
32) Benzene-d6	8.281	84	429902	25.270	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	101.080%		
36) 1,2-Dichloropropane-d6	9.281	67	132264	26.211	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	104.840%		
41) Toluene-d8	10.329	98	387891	24.324	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	97.280%		
43) trans-1,3-Dichloroprop...	10.579	79	54503	23.481	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	93.920%		
47) 2-Hexanone-d5	10.927	63	35824	34.751	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	69.500%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	106215	21.396	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.600%		
66) 1,2-Dichlorobenzene-d4	13.853	152	130108	27.492	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	109.960%		
Target Compounds						
16) Methylene chloride	4.928	84	8796m	1.547	ug/L	Qvalue 95
42) Toluene	10.390	91	6607	0.330	ug/L	09/29/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020070.D
Acq On : 20 Sep 2021 09:26
Operator : SY/VA
Sample : VW0920SBL03
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK441

Manual Integrations
APPROVED

MMDadoda
9/21/2021 6:59:59 PM

Quant Time: Sep 21 01:32:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

