

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020071.D
Acq On : 20 Sep 2021 09:50
Operator : SY/VA
Sample : MDL
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

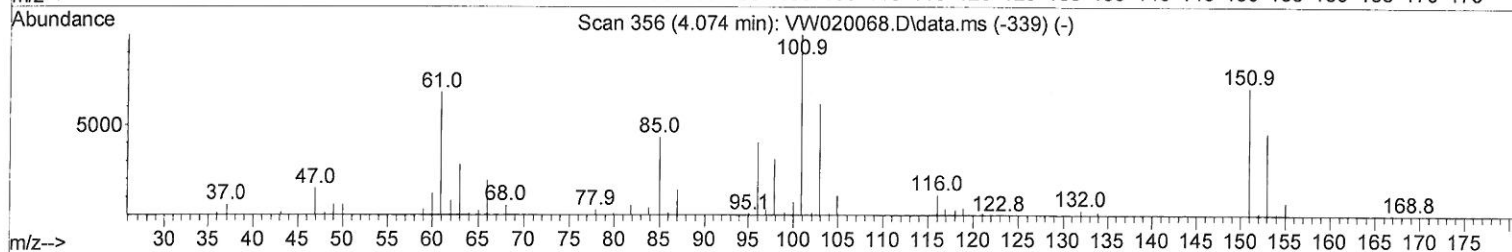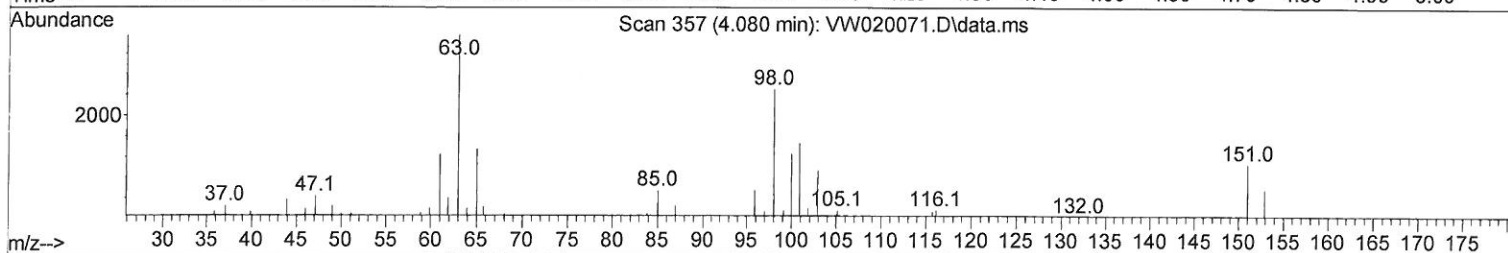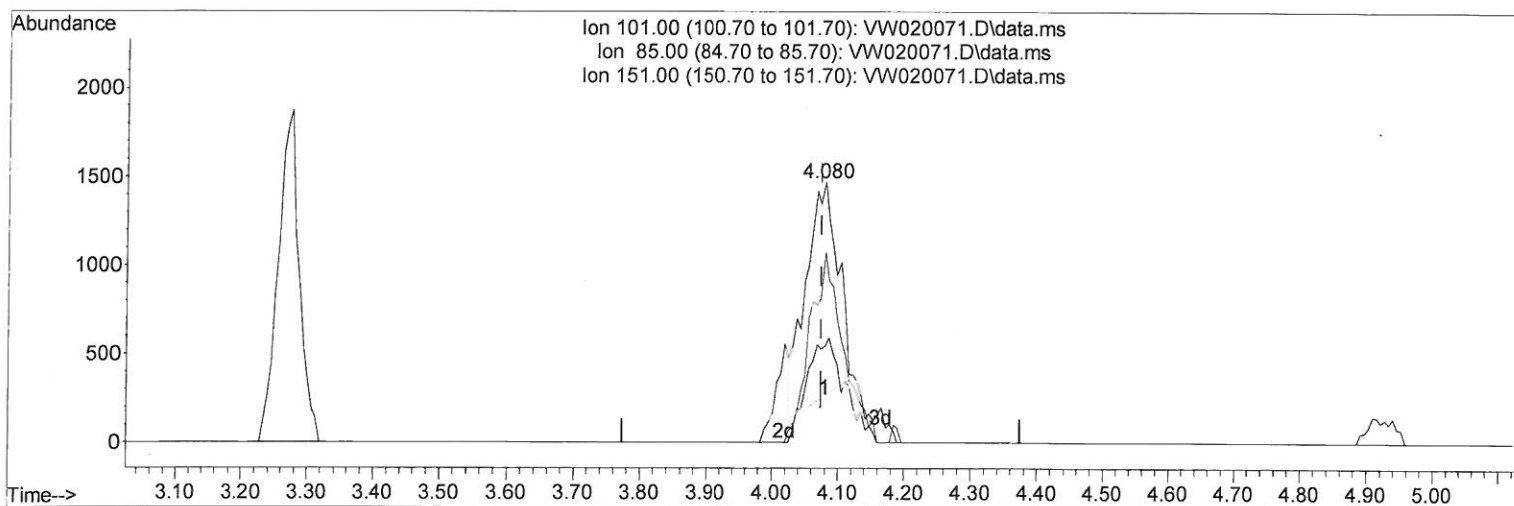

TIC: VW020071.D\data.ms

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.080min (+ 0.006) 0.90 ug/L

response 4069

Ion	Exp%	Act%
101.00	100.00	100.00
85.00	47.70	4.87#
151.00	70.80	62.82
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

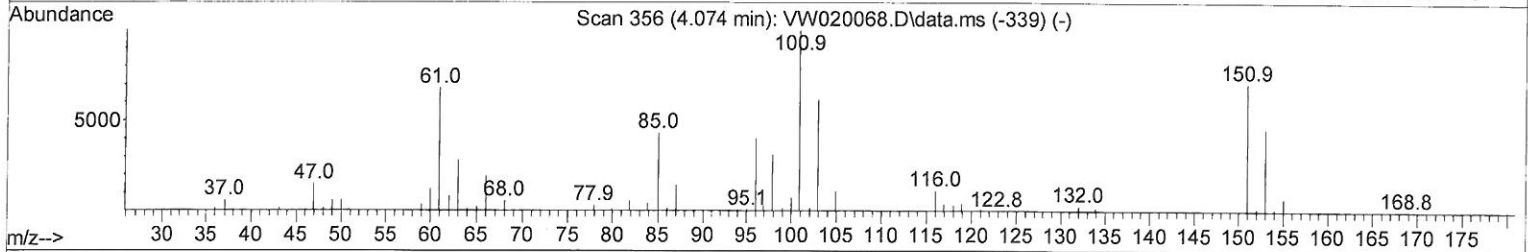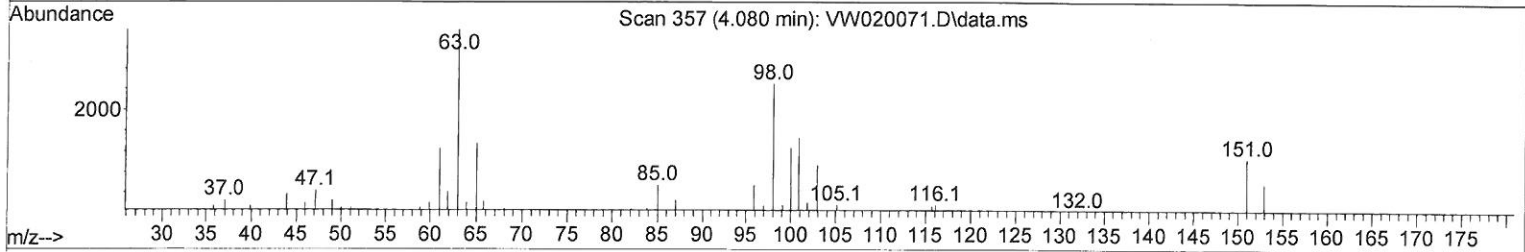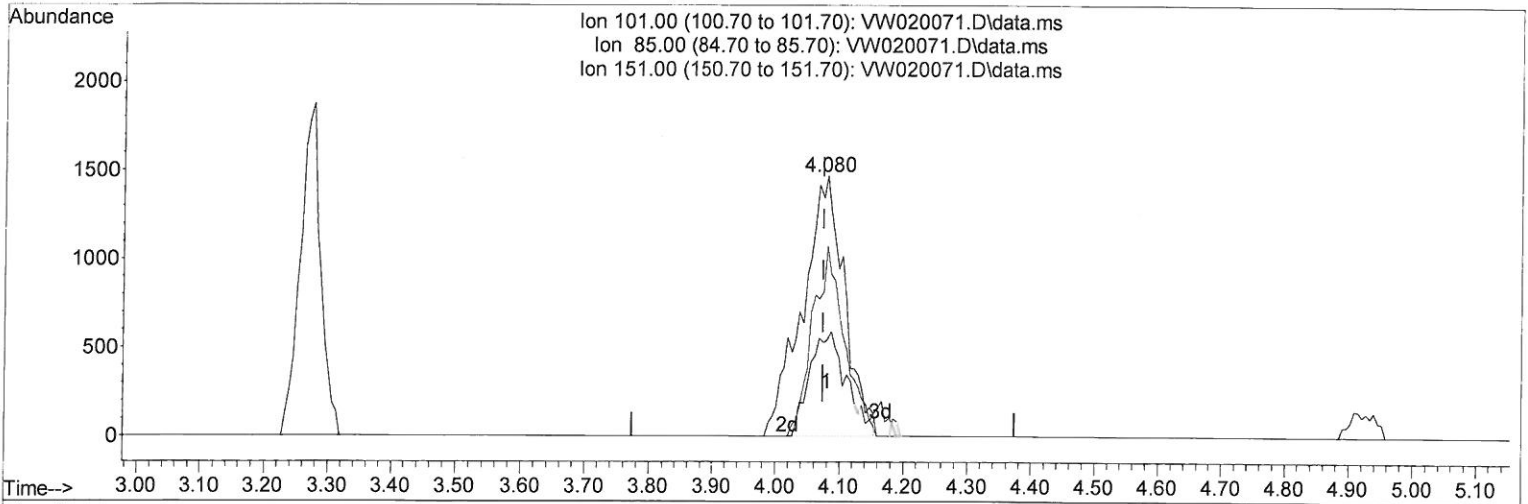

TIC: VW020071.D\data.ms

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.080min (+ 0.006) 1.47 ug/L m

09/24/21 Sy

response 6659

Ion	Exp%	Act%
101.00	100.00	100.00
85.00	47.70	2.97#
151.00	70.80	38.38#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

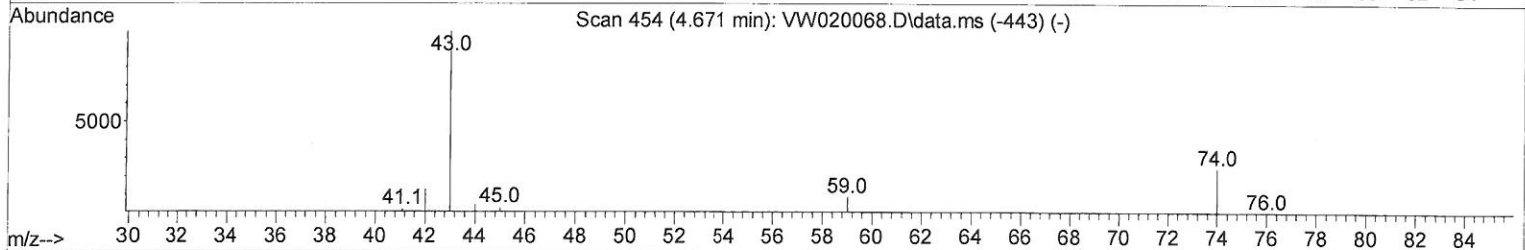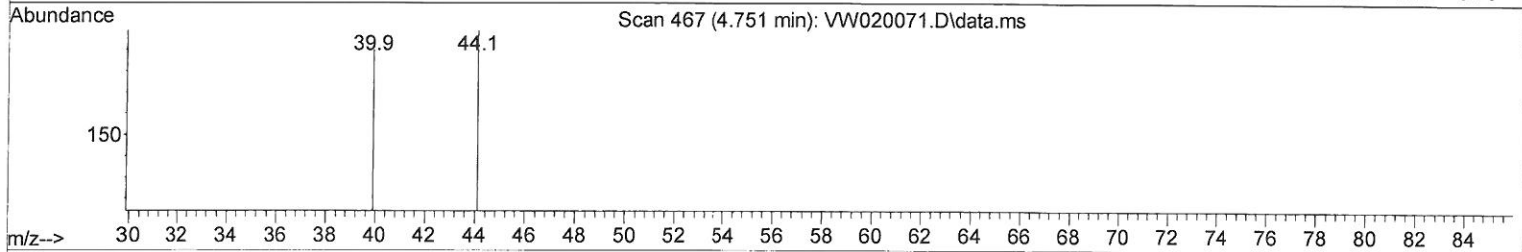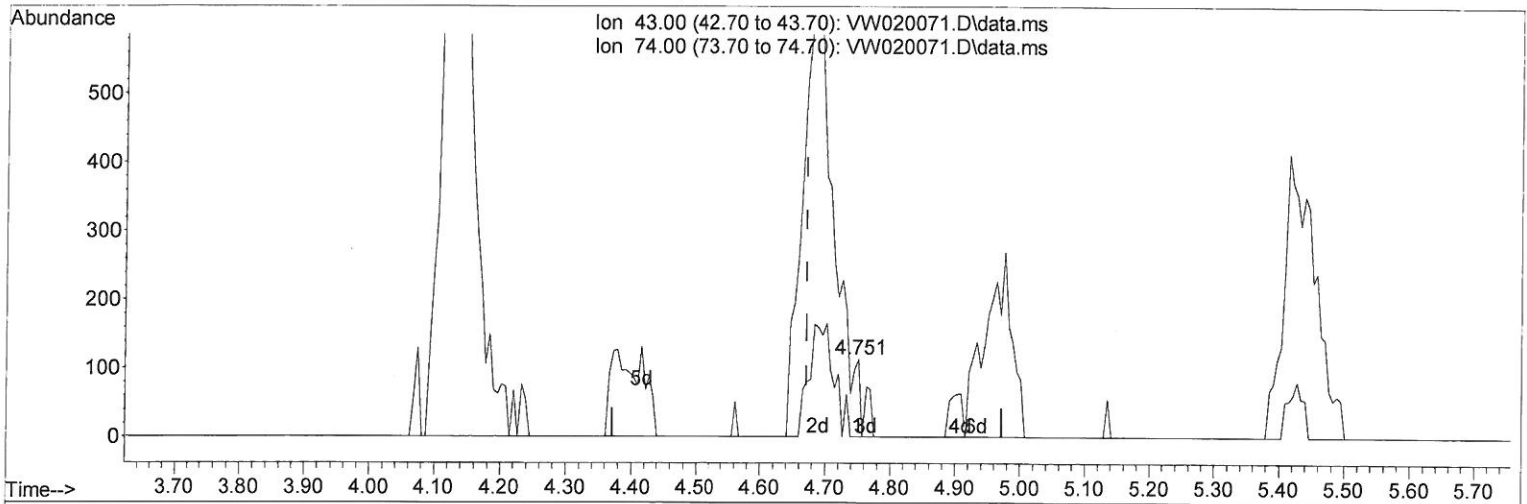

TIC: VW020071.D\data.ms

(15) Methyl Acetate (T)

4.751min (+ 0.079) 0.03 ug/L

response 78

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.00	29.49
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

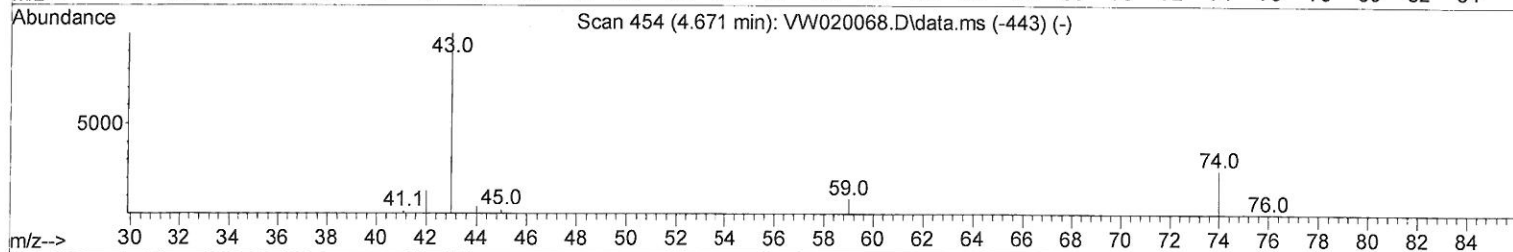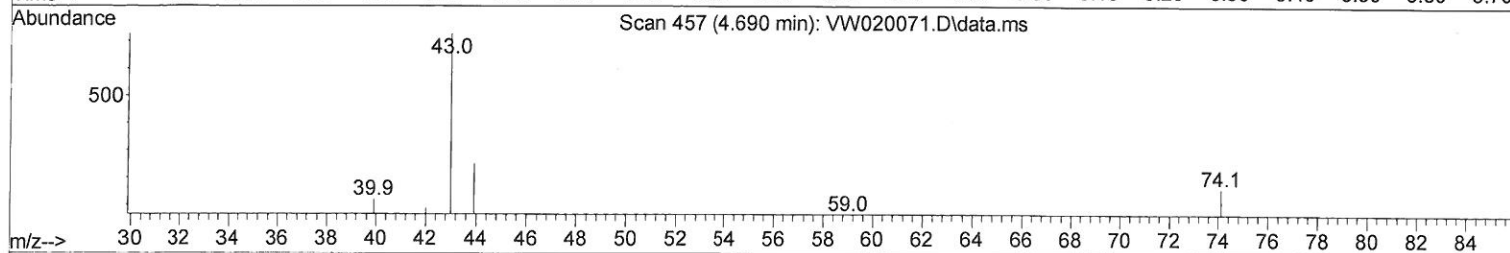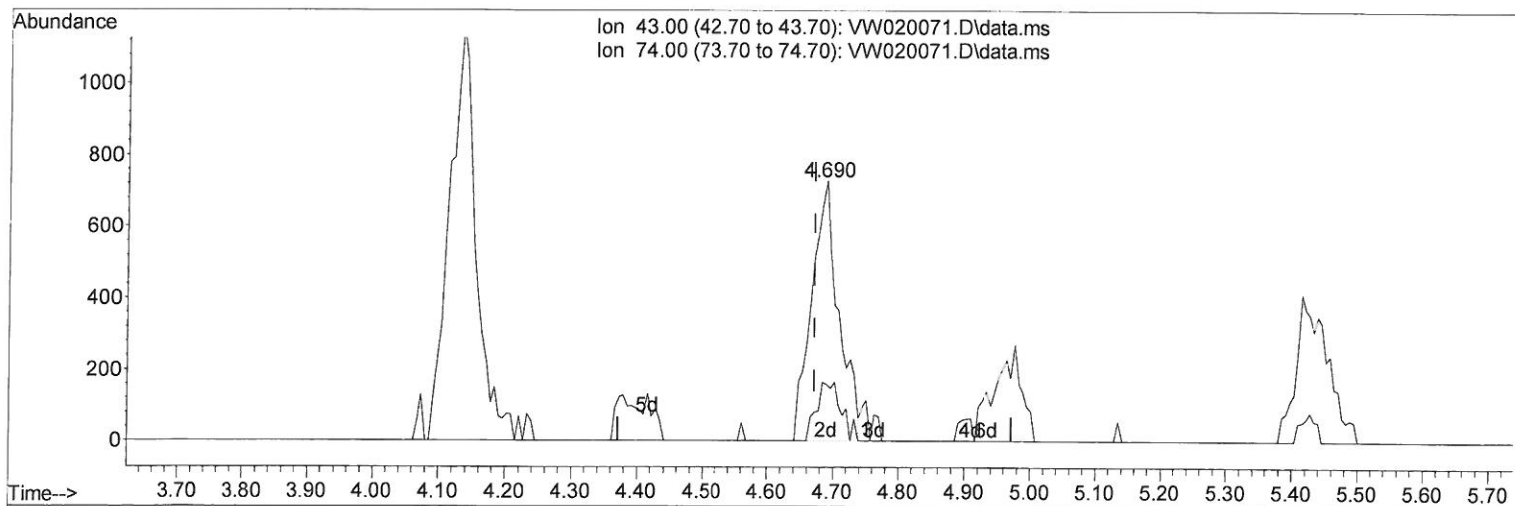

TIC: VW020071.D\data.ms

(15) Methyl Acetate (T)

4.690min (+ 0.018) 0.89 ug/L m

509/24/21 Sy

response 2091

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.00	1.10#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

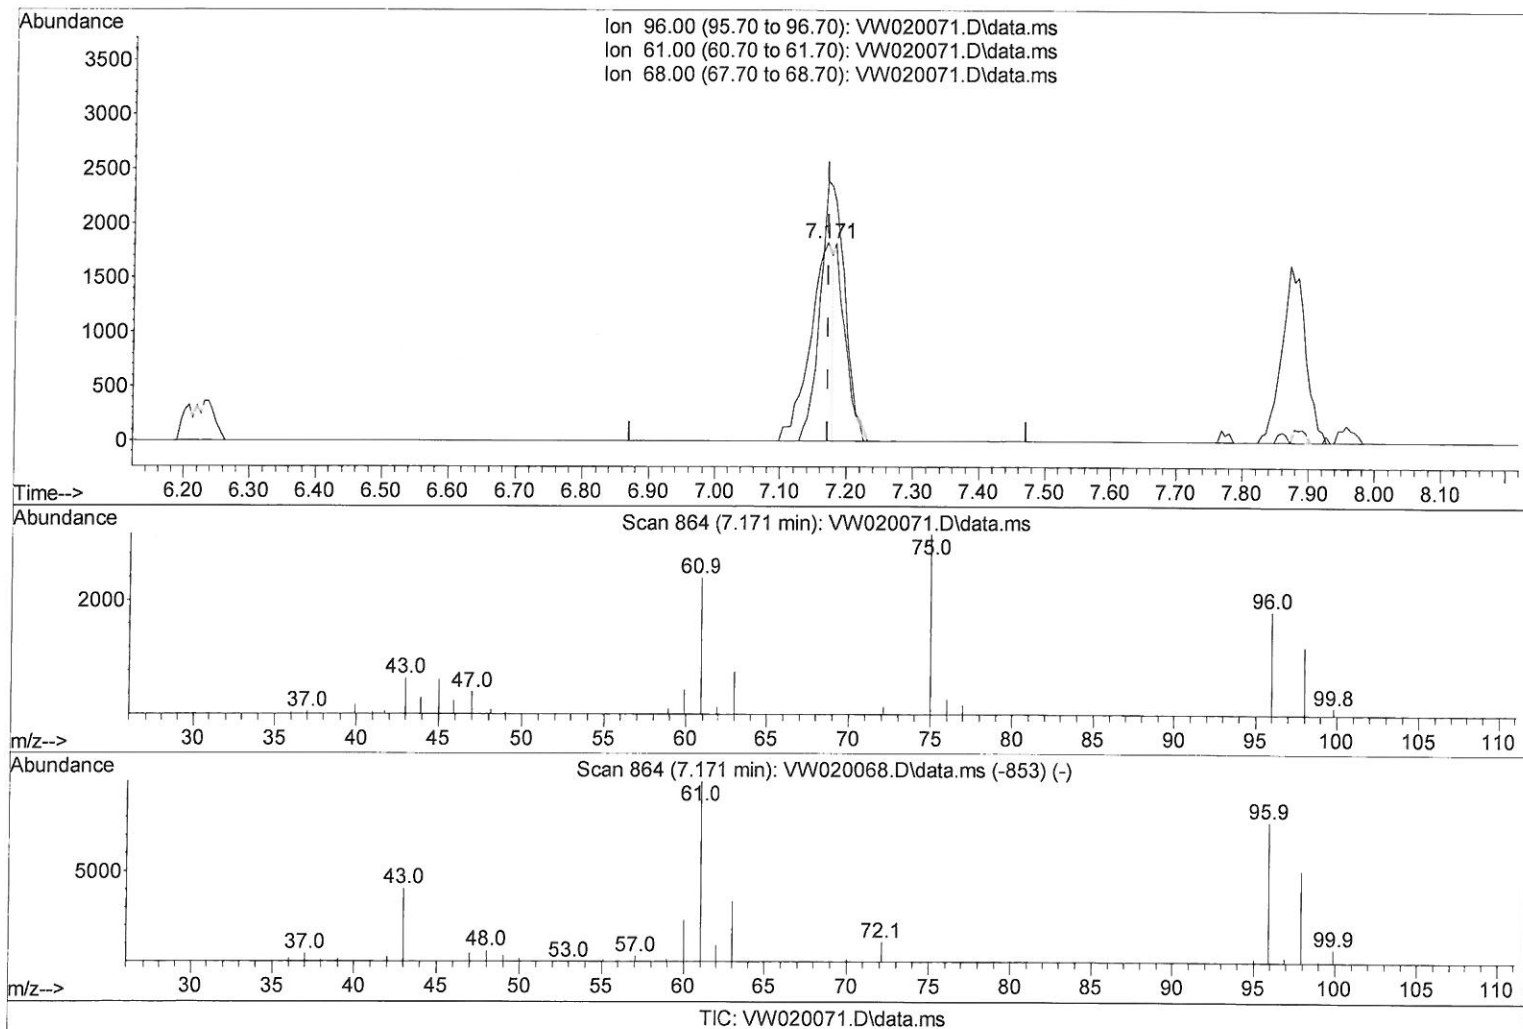

(20) cis-1,2-Dichloroethene (T)

7.171min (+ 0.000) 0.63 ug/L

response 2922

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	126.40	131.01
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

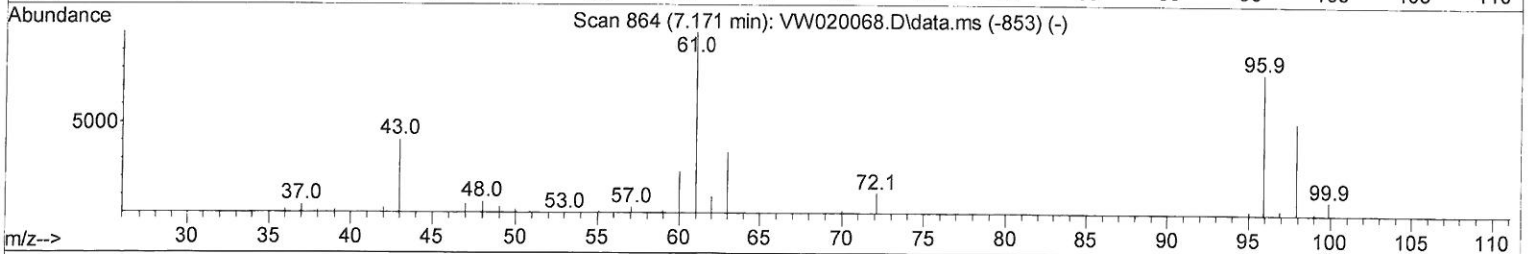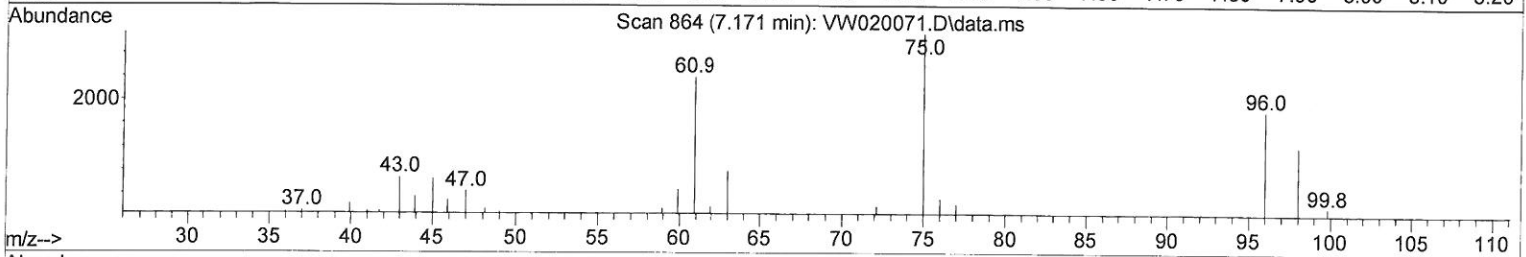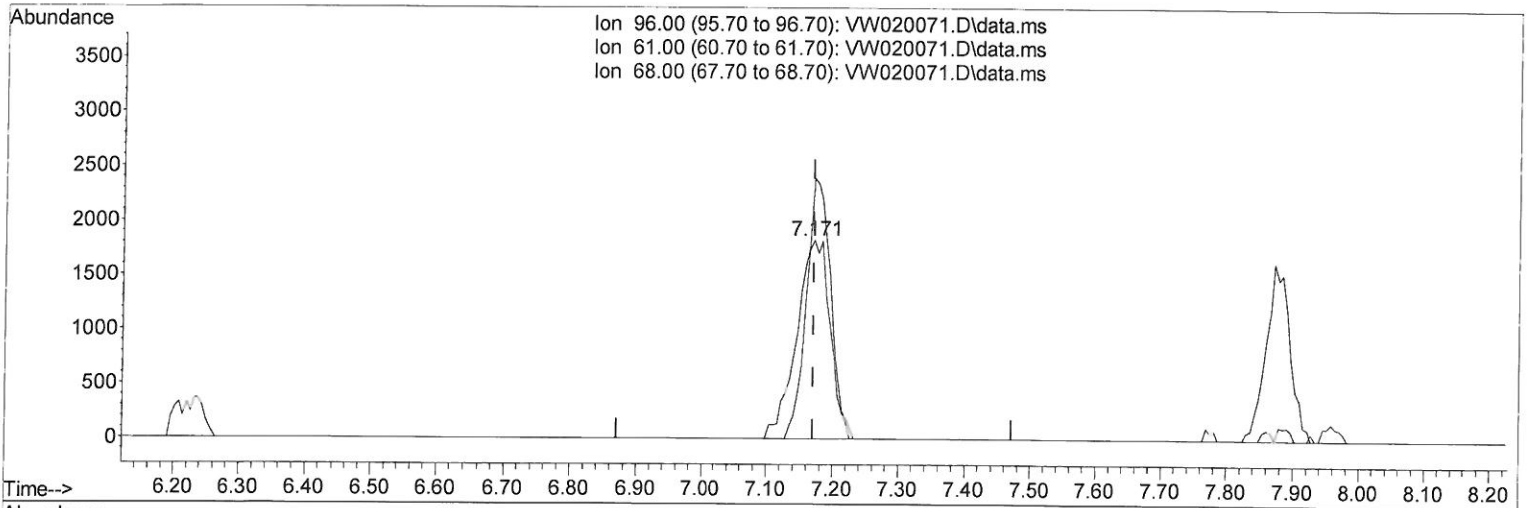

TIC: VW020071.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.171min (+ 0.000) 1.08 ug/L m) 09/24/21 Sy

response 5005

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	126.40	131.01
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

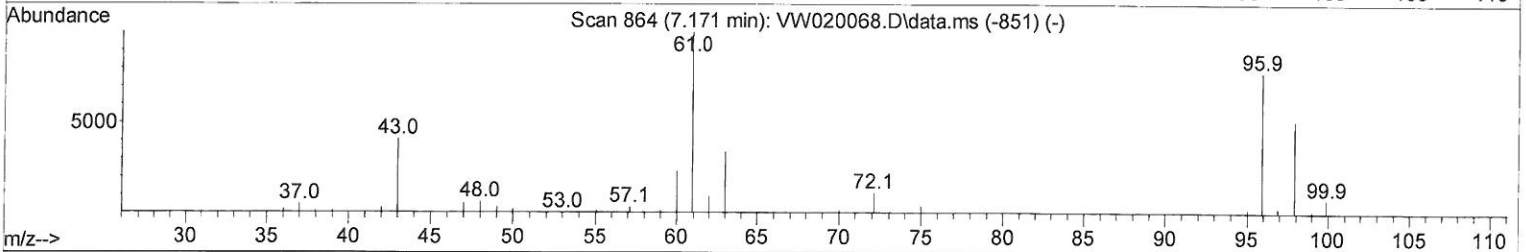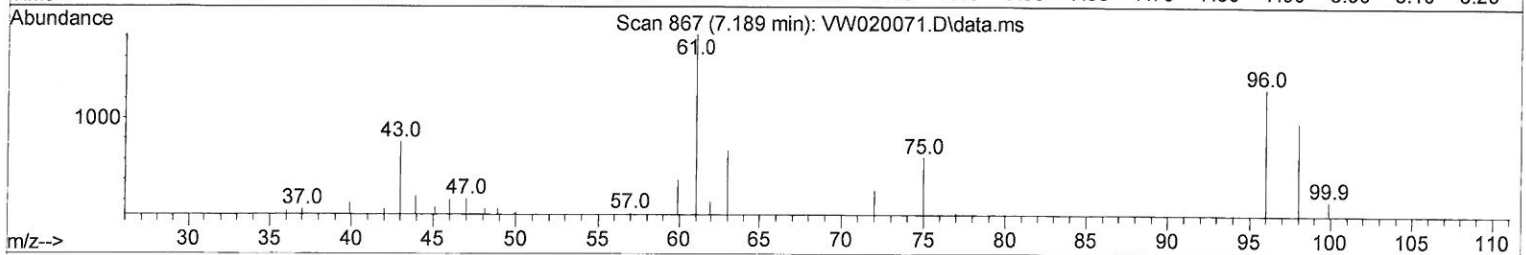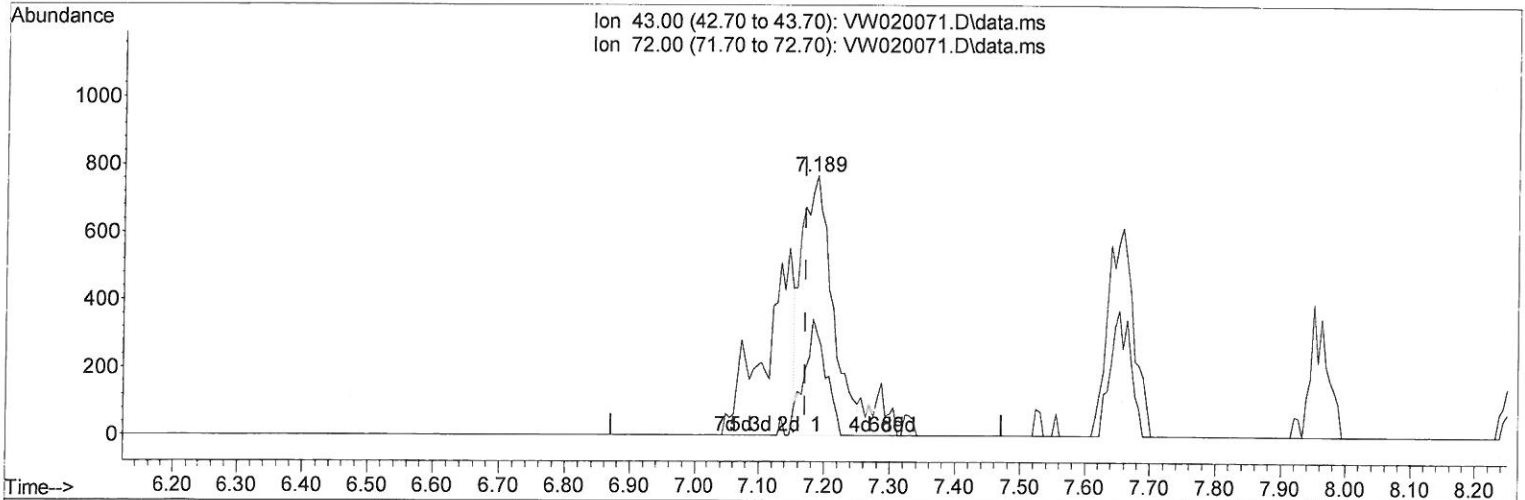

TIC: VW020071.D\data.ms

(22) 2-Butanone (T)

7.189min (+ 0.018) 1.49 ug/L

response 2515

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	31.97
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

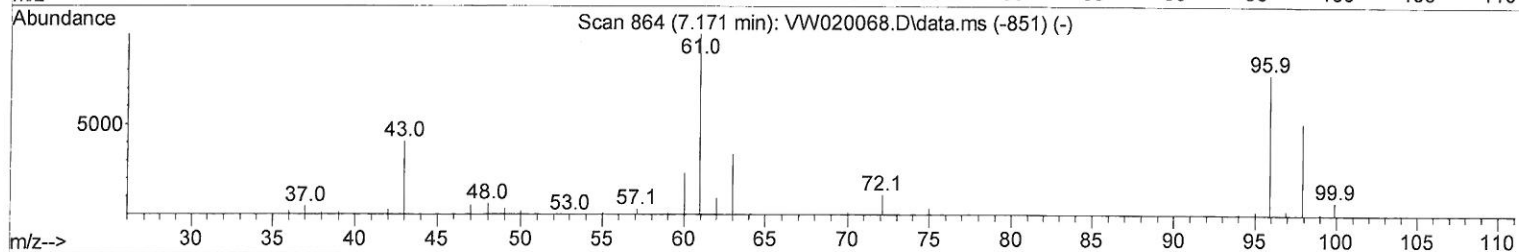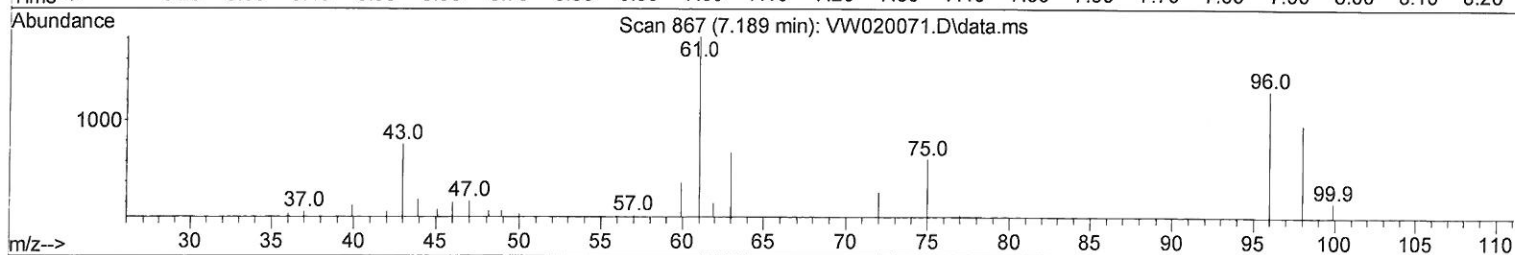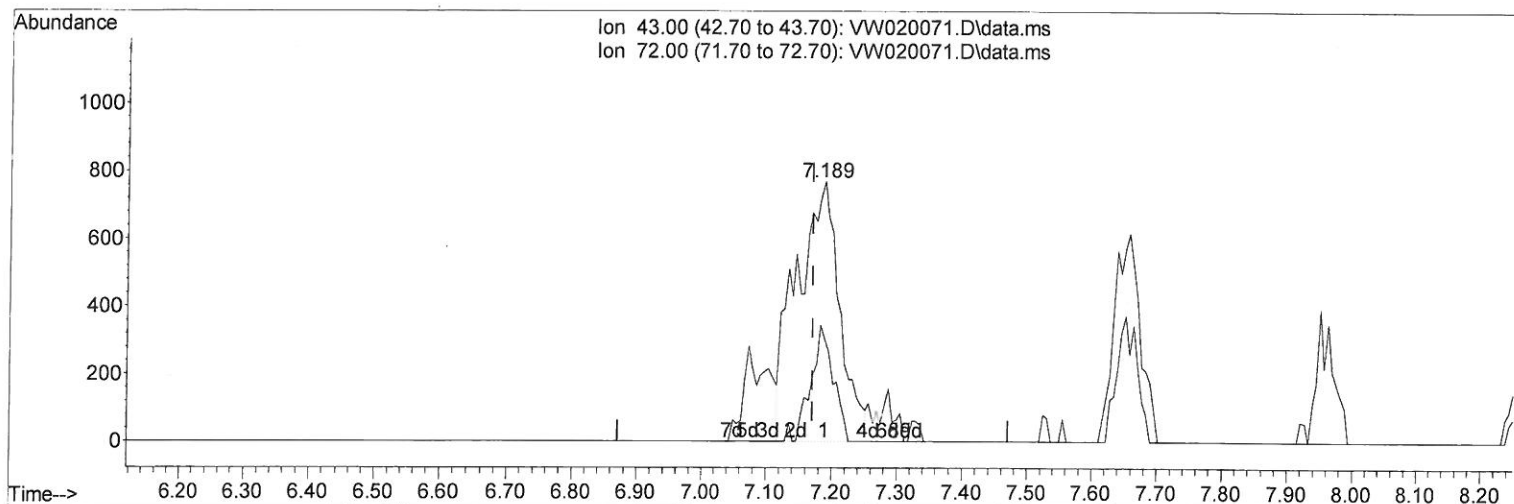

TIC: VW020071.D\data.ms

(22) 2-Butanone (T)

7.189min (+ 0.018) 2.07 ug/L m

509/24/21 Sy

response 3507

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	22.93
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020071.D
Acq On : 20 Sep 2021 09:50
Operator : SY/VA
Sample : MDL
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

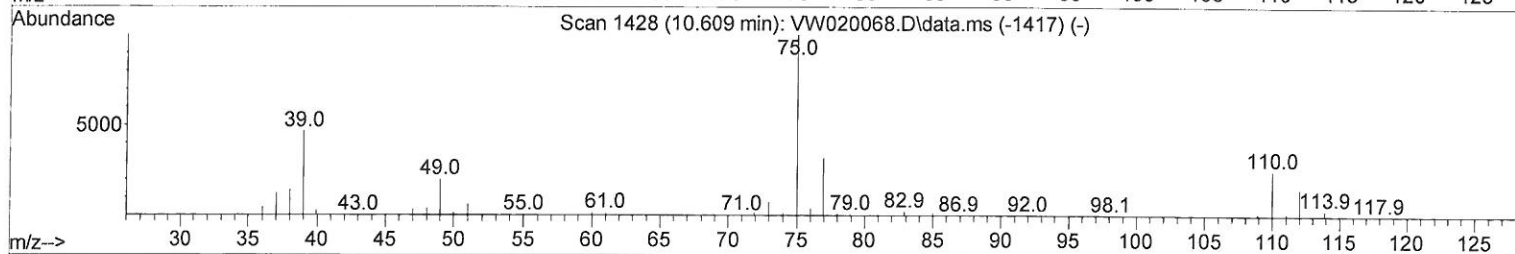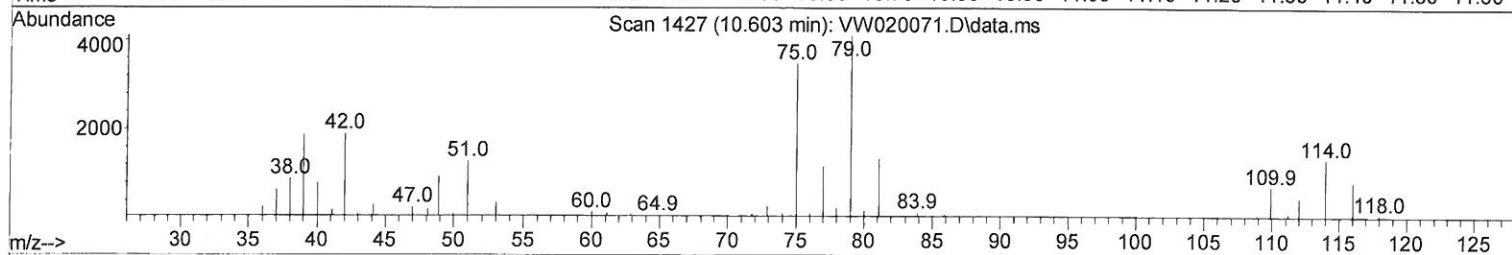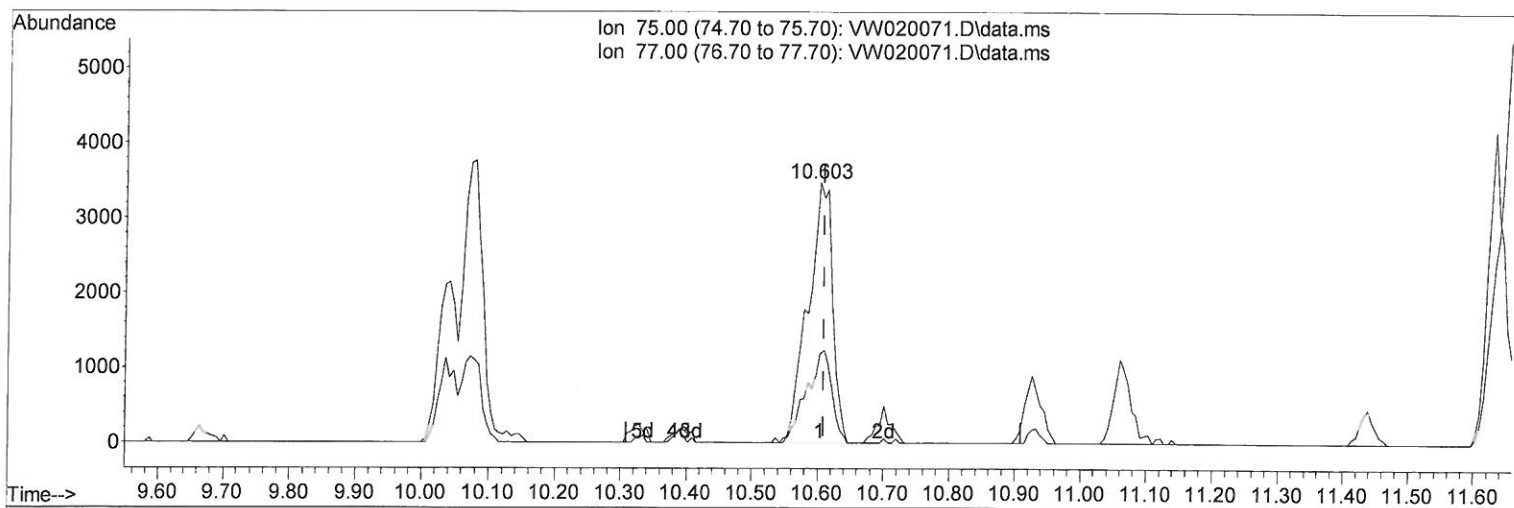

TIC: VW020071.D\data.ms

(44) trans-1,3-Dichloropropene (T)

10.603min (-0.006) 1.36 ug/L

response 8971

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	30.10	34.03
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020071.D
Acq On : 20 Sep 2021 09:50
Operator : SY/VA
Sample : MDL
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

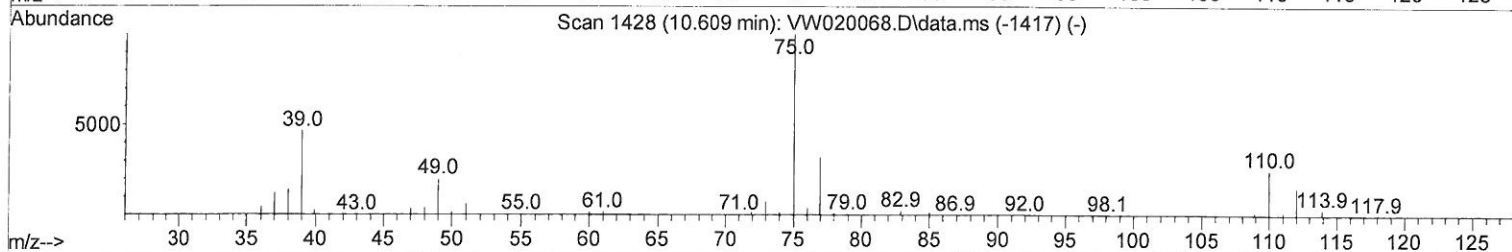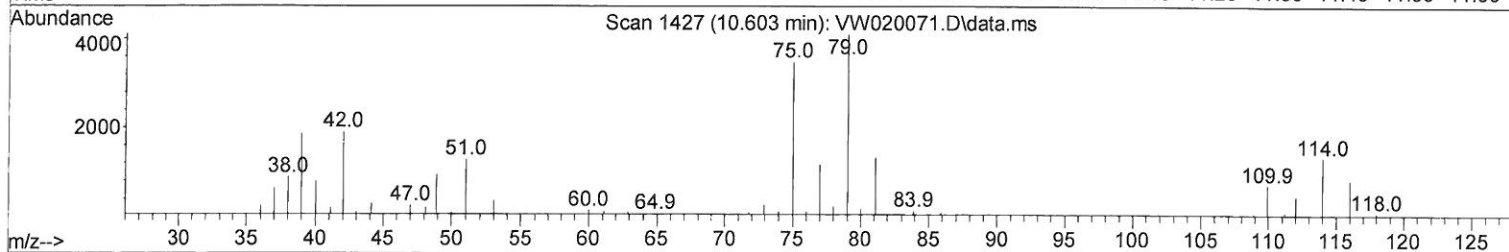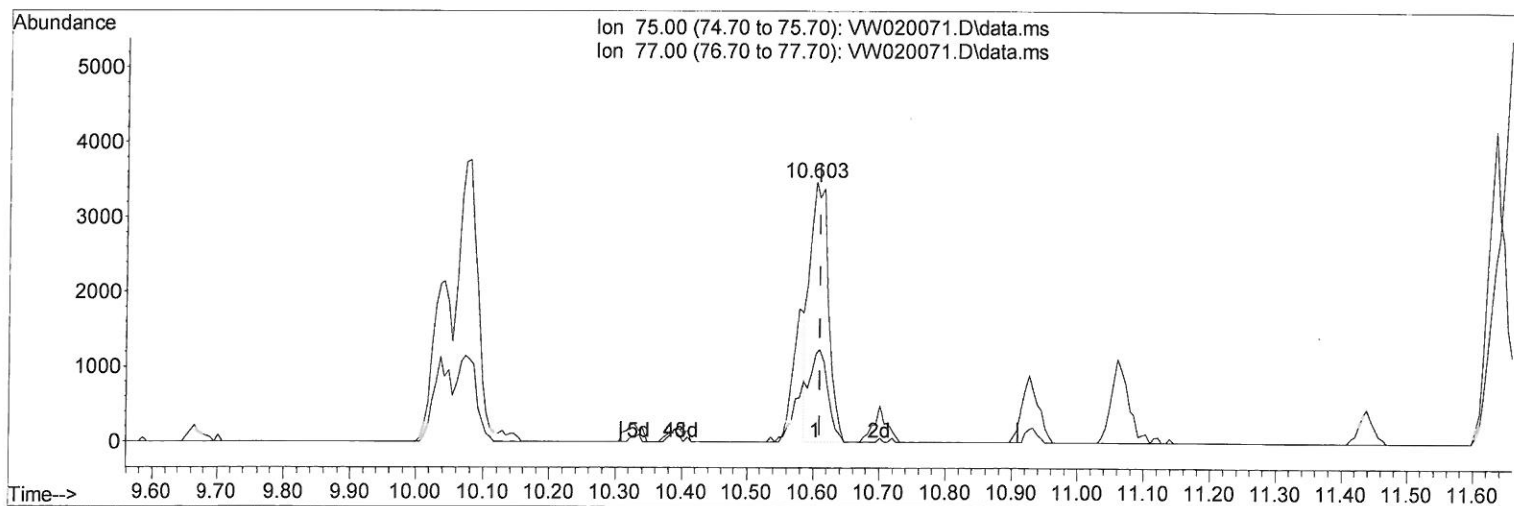

TIC: VW020071.D\data.ms

(44) trans-1,3-Dichloropropene (T)

10.603min (-0.006) 1.03 ug/L m

response 6760

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	30.10	34.03
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020071.D
Acq On : 20 Sep 2021 09:50
Operator : SY/VA
Sample : MDL
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

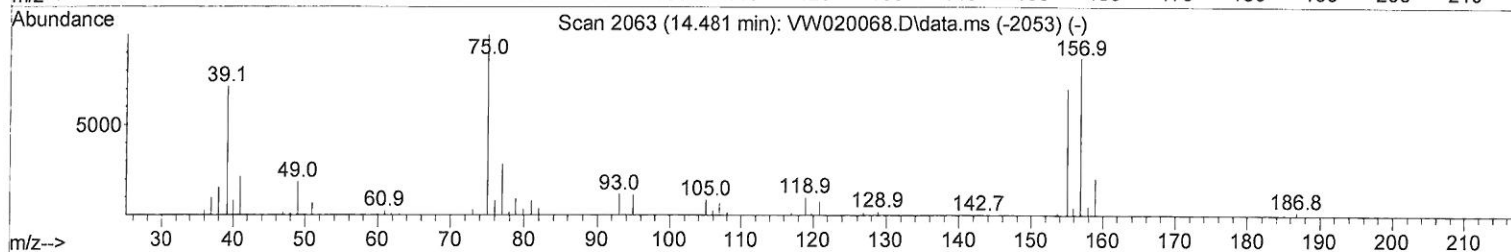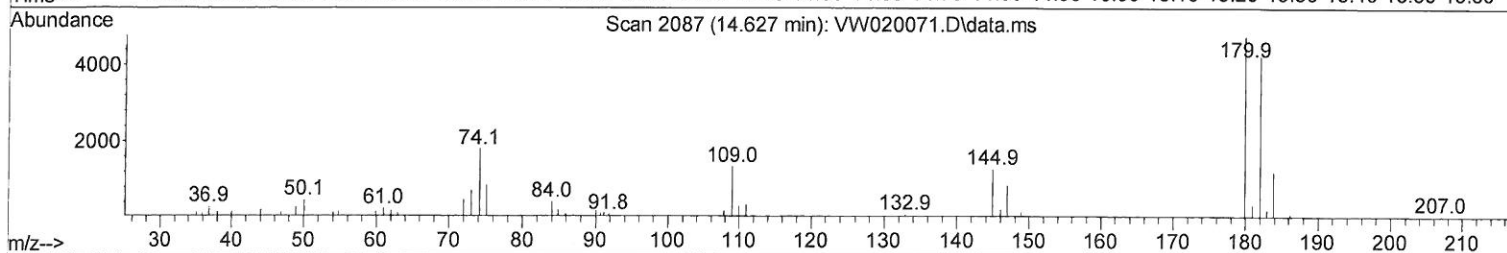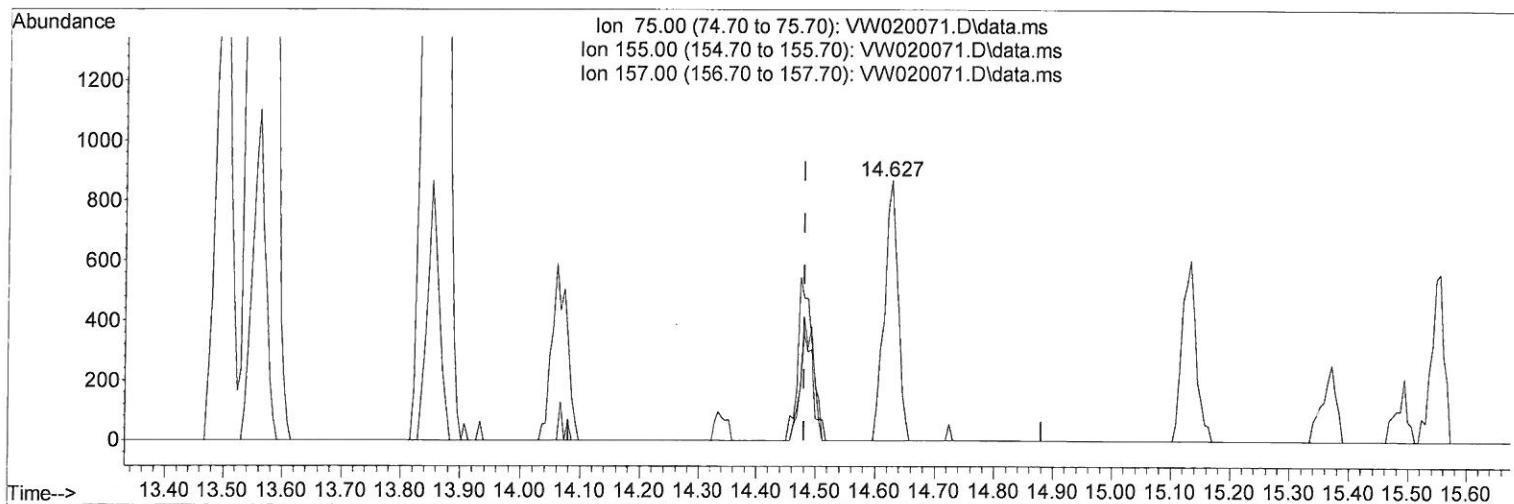

TIC: VW020071.D\data.ms

(68) 1,2-Dibromo-3-chloropropane (T)

14.627min (+ 0.146) 1.66 ug/L

response 1356

Ion	Exp%	Act%
75.00	100.00	100.00
155.00	74.20	0.00#
157.00	90.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020071.D
Acq On : 20 Sep 2021 09:50
Operator : SY/VA
Sample : MDL
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

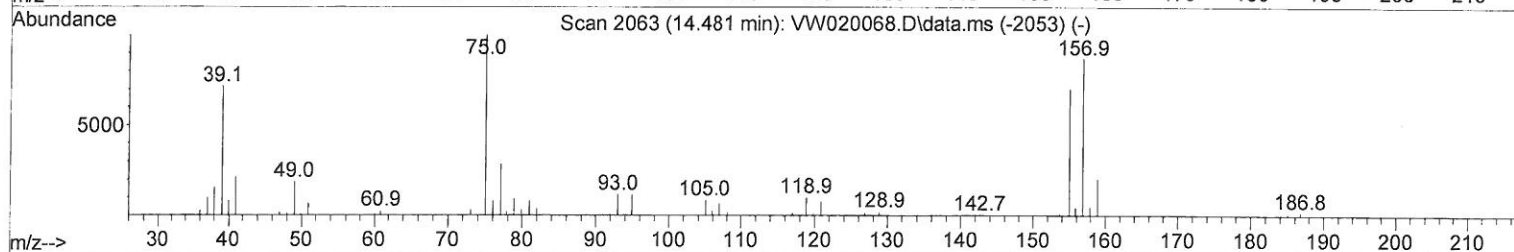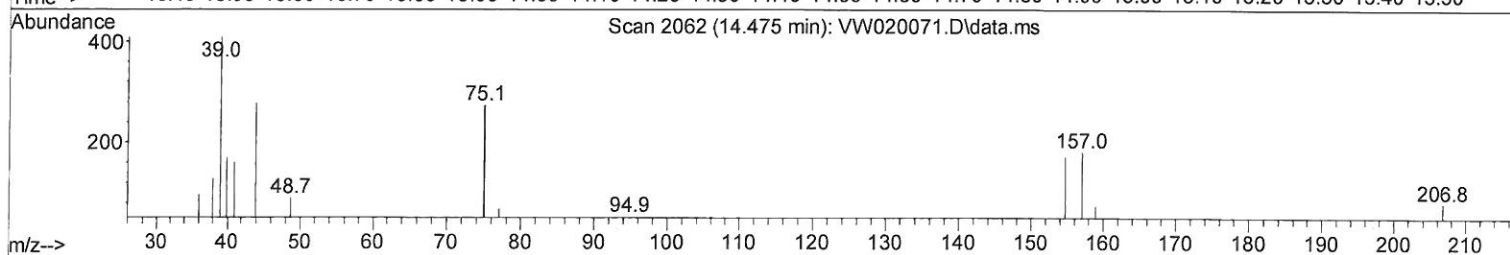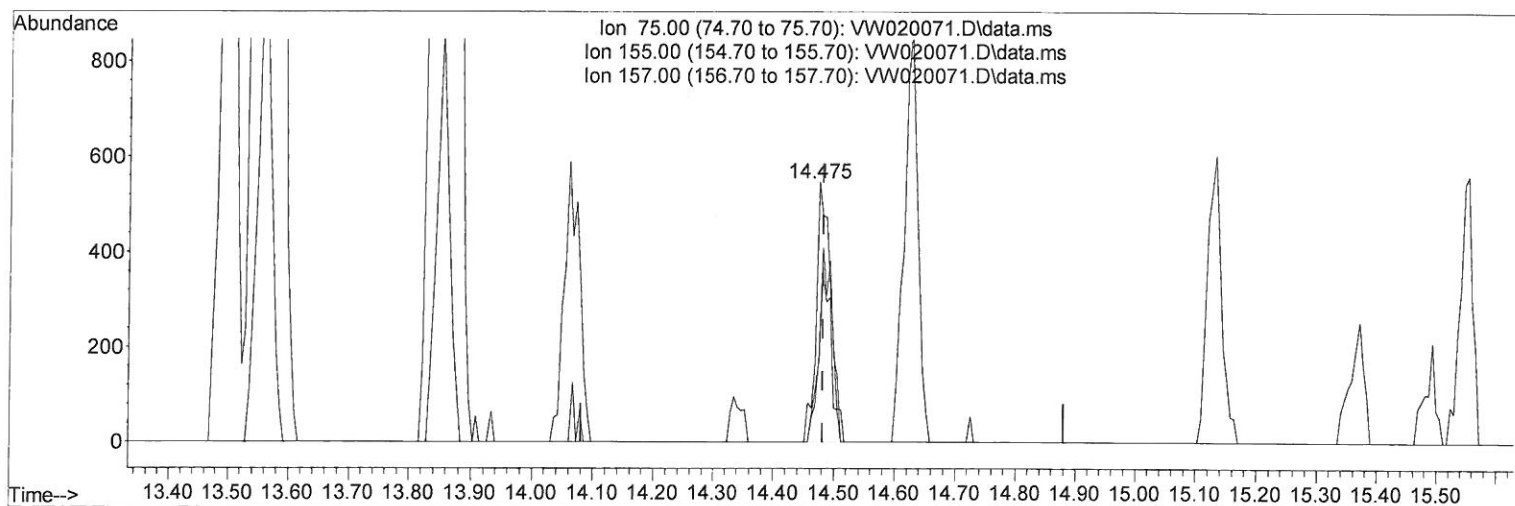

TIC: VW020071.D\data.ms

(68) 1,2-Dibromo-3-chloropropane (T)

14.475min (-0.006) 1.11 ug/L m

response 908

Ion	Exp%	Act%
75.00	100.00	100.00
155.00	74.20	63.14
157.00	90.20	66.42#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	315195	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	315979	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	144893	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	125910	24.253	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.000%		
7) Chloroethane-d5	2.897	69	101081	22.621	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.480%		
11) 1,1-Dichloroethene-d2	4.025	63	158636	18.695	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.760%		
21) 2-Butanone-d5	7.086	46	50733	35.723	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	71.440%		
24) Chloroform-d	7.659	84	229404	26.414	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	105.640%		
26) 1,2-Dichloroethane-d4	8.311	65	131986	25.798	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.200%		
32) Benzene-d6	8.281	84	430325	24.961	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.840%		
36) 1,2-Dichloropropane-d6	9.280	67	131276	25.672	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.680%		
41) Toluene-d8	10.329	98	390583	24.170	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.680%		
43) trans-1,3-Dichloroprop...	10.579	79	54040	22.974	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.880%		
47) 2-Hexanone-d5	10.926	63	36554	34.992	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	69.980%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	107011	21.272	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152	131970	26.726	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	106.920%		
Target Compounds						
2) Dichlorodifluoromethane	2.013	85	2963	0.907	ug/L	96
3) Chloromethane	2.221	50	4945	1.124	ug/L	87
5) Vinyl chloride	2.373	62	7622	1.107	ug/L #	62
6) Bromomethane	2.788	94	4576	0.948	ug/L	95
8) Chloroethane	2.940	64	4491	1.069	ug/L	95
9) Trichlorofluoromethane	3.275	101	4166	1.037	ug/L	95
10) 1,1,2-Trichloro-1,2,2-...	4.080	101	6659m	1.474	ug/L	
12) 1,1-Dichloroethene	4.050	96	5803	1.357	ug/L #	1
13) Acetone	4.135	43	3180	2.358	ug/L	66
14) Carbon disulfide	4.397	76	13937	0.998	ug/L	95
15) Methyl Acetate	4.690	43	2091m	0.889	ug/L	
16) Methylene chloride	4.921	84	12276	2.210	ug/L	88
17) trans-1,2-Dichloroethene	5.440	96	4786	1.062	ug/L	82
18) Methyl tert-butyl Ether	5.446	73	5617	0.998	ug/L #	80
19) 1,1-Dichloroethane	6.226	63	9527	1.182	ug/L #	86
20) cis-1,2-Dichloroethene	7.171	96	5005m	1.076	ug/L	
22) 2-Butanone	7.189	43	3507m	2.075	ug/L	
23) Bromochloromethane	7.525	128	2488	1.155	ug/L	91

09/24/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
 Data File : VW020071.D
 Acq On : 20 Sep 2021 09:50
 Operator : SY/VA
 Sample : MDL
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 MDL

Manual Integrations
 APPROVED

MMDadoda
 9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 01:31:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
25) Chloroform	7.683	83	11235	1.327	ug/L	99
27) 1,2-Dichloroethane	8.409	62	6872	1.160	ug/L #	93
29) Cyclohexane	7.957	56	5531	0.777	ug/L	99
30) 1,1,1-Trichloroethane	7.878	97	8482	1.145	ug/L	100
31) Carbon tetrachloride	8.073	117	7772	1.125	ug/L	95
33) Benzene	8.329	78	20559	1.081	ug/L	100
34) Trichloroethene	9.098	95	5261	1.045	ug/L	92
35) Methylcyclohexane	9.341	83	7640	0.900	ug/L	93
37) 1,2-Dichloropropane	9.372	63	5012	1.088	ug/L	99
38) Bromodichloromethane	9.646	83	6903	1.111	ug/L	96
39) cis-1,3-Dichloropropene	10.079	75	7014	1.009	ug/L	94
40) 4-Methyl-2-pentanone	10.213	43	5564	1.694	ug/L	99
42) Toluene	10.390	91	27323	1.346	ug/L	95
44) trans-1,3-Dichloropropene	10.603	75	6760m	1.027	ug/L	94
45) 1,1,2-Trichloroethane	10.786	97	3843	1.044	ug/L	94
46) Tetrachloroethene	10.866	164	4310	1.106	ug/L	94
48) 2-Hexanone	10.969	43	3892	1.653	ug/L	94
49) Dibromochloromethane	11.134	129	4312	1.019	ug/L	98
50) 1,2-Dibromoethane	11.237	107	3525	0.973	ug/L	92
51) Chlorobenzene	11.658	112	14352	1.091	ug/L	93
52) Ethylbenzene	11.731	91	20748	0.936	ug/L	99
53) m,p-Xylene	11.841	106	7232	0.858	ug/L	99
54) o-Xylene	12.170	106	6359	0.799	ug/L	93
55) Styrene	12.182	104	10234	0.748	ug/L	97
57) 1,1,2,2-Tetrachloroethane	12.713	83	5288	1.096	ug/L #	89
59) Bromoform	12.353	173	2223	1.014	ug/L	98
60) Isopropylbenzene	12.463	105	16290	0.848	ug/L	98
61) 1,2,3-Trichloropropane	12.768	75	3341	0.986	ug/L	94
62) 1,3,5-Trimethylbenzene	12.944	105	13166	0.842	ug/L	97
63) 1,2,4-Trimethylbenzene	13.249	105	13058	0.851	ug/L	97
64) 1,3-Dichlorobenzene	13.499	146	9480	1.073	ug/L	94
65) 1,4-Dichlorobenzene	13.578	146	10439	1.159	ug/L	96
67) 1,2-Dichlorobenzene	13.871	146	9705	1.205	ug/L	92
68) 1,2-Dibromo-3-chloropr...	14.475	75	908m	1.111	ug/L	92
69) 1,3,5-Trichlorobenzene	14.627	180	6603	1.080	ug/L	95
70) 1,2,4-trichlorobenzene	15.133	180	4881	1.020	ug/L	99
71) Naphthalene	15.359	128	7556	0.739	ug/L	99
72) 1,2,3-Trichlorobenzene	15.554	180	4367	0.972	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092021\
Data File : VW020071.D
Acq On : 20 Sep 2021 09:50
Operator : SY/VA
Sample : MDL
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
9/21/2021 7:00:01 PM

Quant Time: Sep 21 02:11:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 01:31:02 2021
Response via : Initial Calibration

