

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\Not Reviewed Data\
 Data File : VW020084.D
 Acq On : 21 Sep 2021 10:29
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 21 12:01:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 21 11:40:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	364384	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	346384	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	154152	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	172922	23.197	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	92.800%	
7) Chloroethane-d5	2.897	69	132709	23.632	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	94.520%	
11) 1,1-Dichloroethene-d2	4.196	63	80	0.007	ug/L	0.16
Spiked Amount	25.000	Range 45 - 110	Recovery	=	0.040%#	
21) 2-Butanone-d5	7.080	46	54595	47.460	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	94.920%	
24) Chloroform-d	7.653	84	272705	23.797	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	95.200%	
26) 1,2-Dichloroethane-d4	8.311	65	156591	25.389	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	101.560%	
32) Benzene-d6	8.281	84	544117	24.622	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	98.480%	
36) 1,2-Dichloropropane-d6	9.274	67	158952	24.854	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	99.400%	
41) Toluene-d8	10.329	98	495326	24.634	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	98.520%	
43) trans-1,3-Dichloroprop...	10.579	79	65989	24.140	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	96.560%	
47) 2-Hexanone-d5	10.927	63	40076	45.281	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	90.560%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	112417	22.787	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	91.160%	
66) 1,2-Dichlorobenzene-d4	13.853	152	156181	27.020	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	108.080%	
Target Compounds						Qvalue
34) Trichloroethene	8.848	95	11566	2.067	ug/L #	5
42) Toluene	10.390	91	8244	0.371	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\Not Reviewed Data\
Data File : VW020084.D
Acq On : 21 Sep 2021 10:29
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 21 12:01:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 21 11:40:17 2021
Response via : Initial Calibration

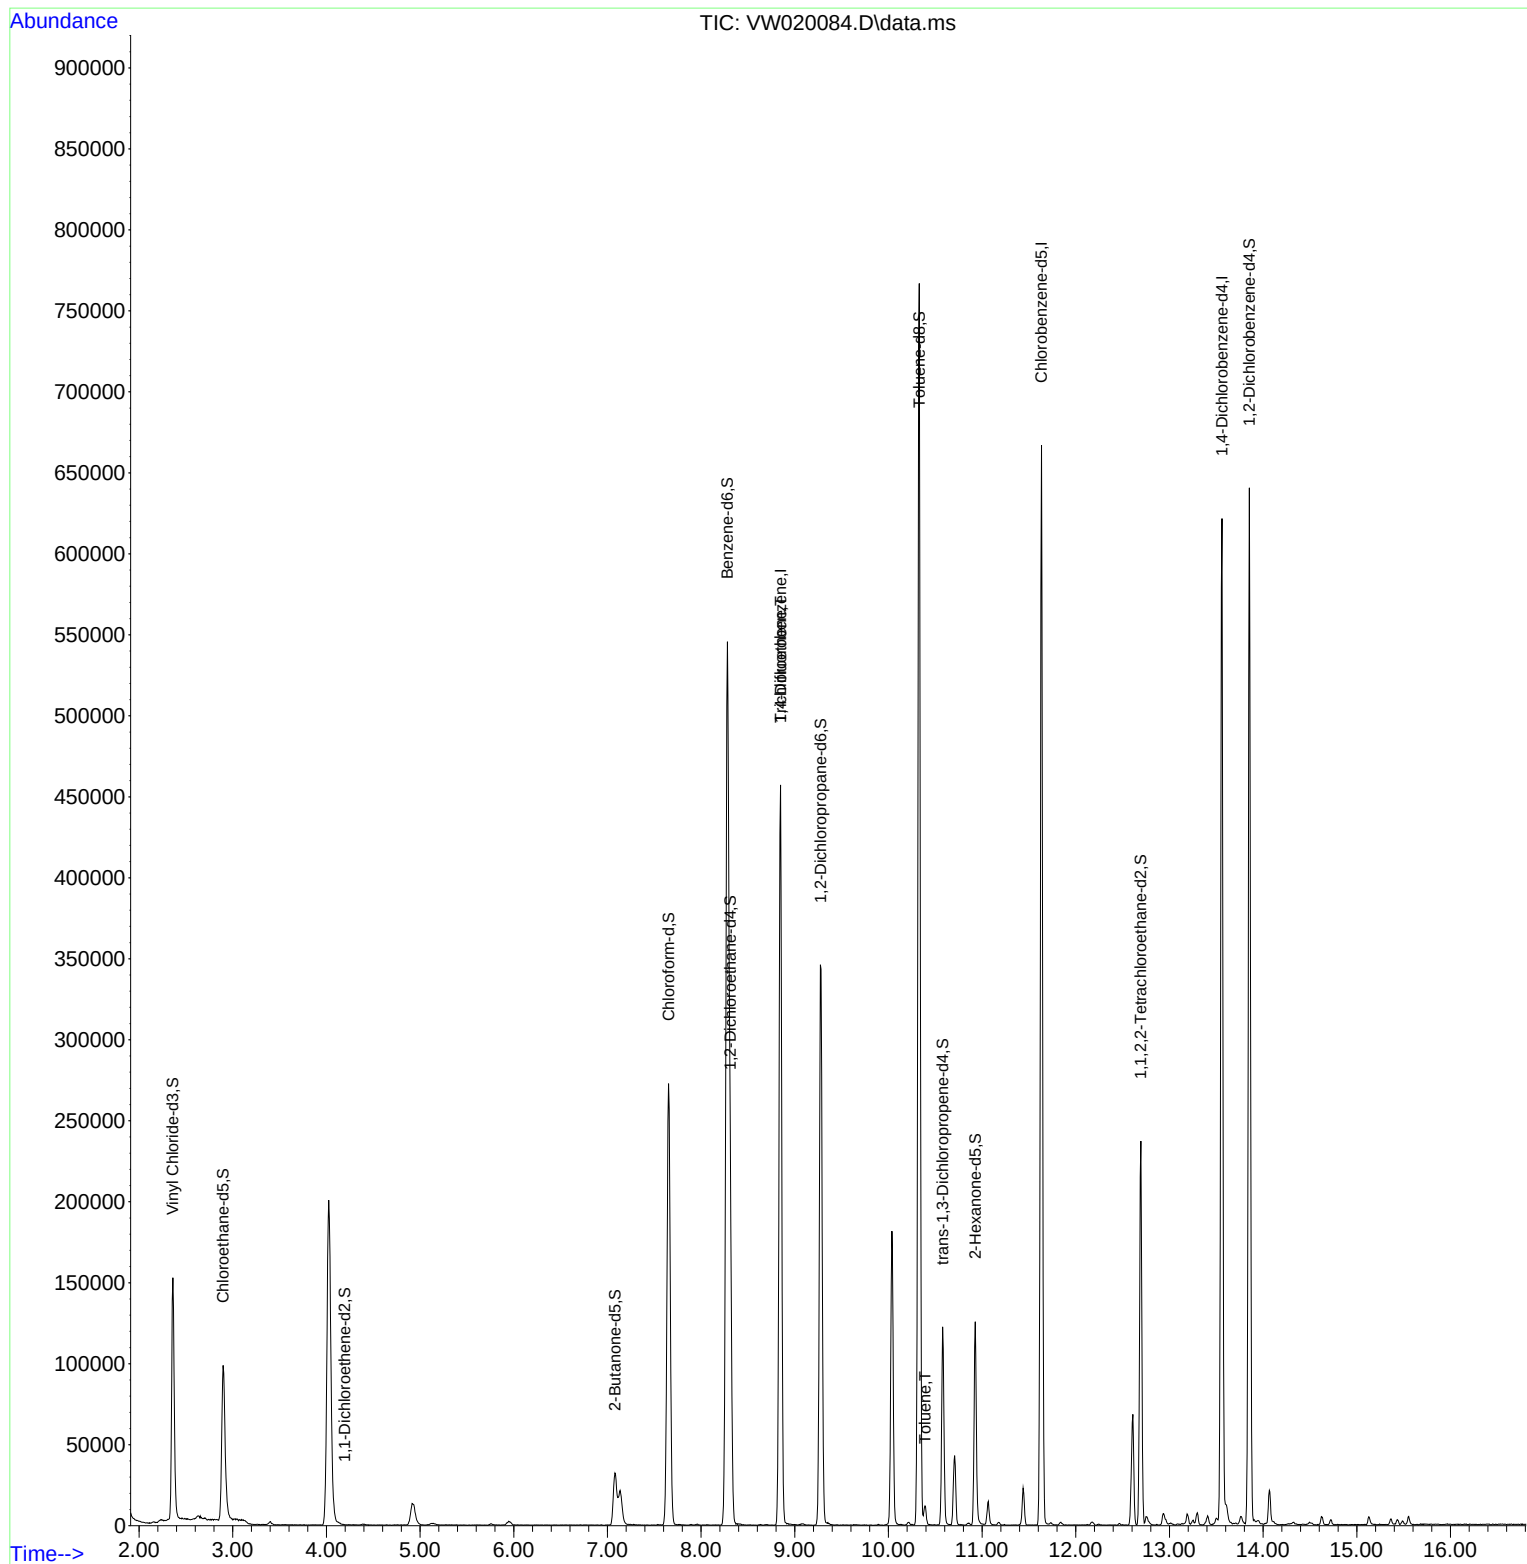




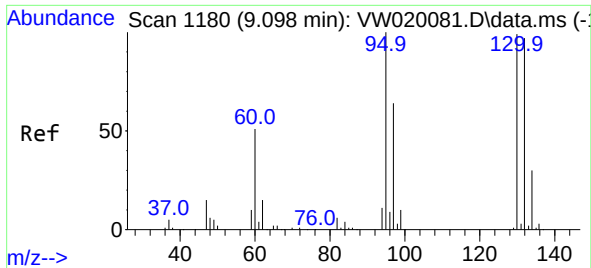


#34
 Trichloroethene
 Concen: 2.067 ug/L
 RT: 8.848 min Scan# 1139
 Delta R.T. -0.250 min
 Lab File: VW020084.D
 Acq: 21 Sep 2021 10:29

Instrument :
 MSVOA_W
 ClientSampled :

Tgt Ion: 95 Resp: 11566

Ion	Ratio	Lower	Upper
95	100		
97	0.0	47.3	87.8#
132	0.0	71.0	131.8#
130	0.0	65.1	120.9#

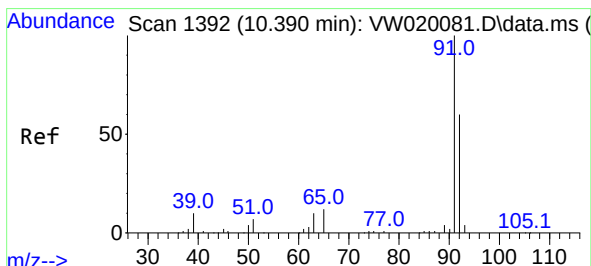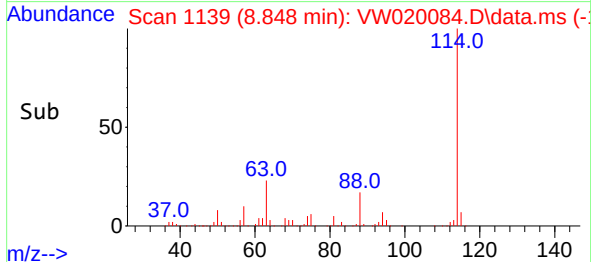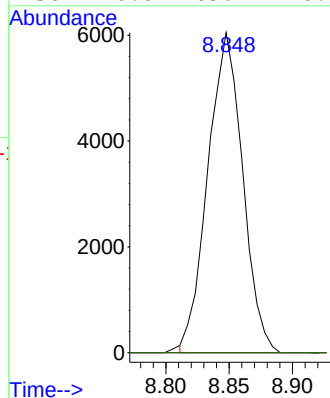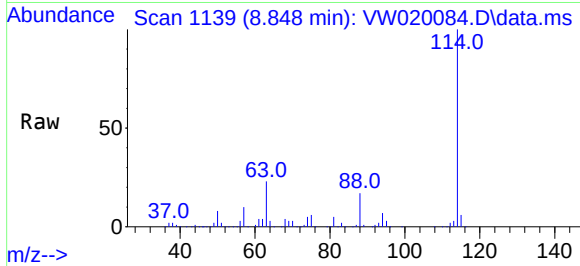

#42
 Toluene
 Concen: 0.371 ug/L
 RT: 10.390 min Scan# 1392
 Delta R.T. -0.000 min
 Lab File: VW020084.D
 Acq: 21 Sep 2021 10:29

Tgt Ion: 91 Resp: 8244

Ion	Ratio	Lower	Upper
91	100		
92	57.4	39.5	73.3

