

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
 Data File : VW020092.D
 Acq On : 21 Sep 2021 15:05
 Operator : SY/VA
 Sample : M3813-04
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB6T0

Manual Integrations
 APPROVED

MMDadoda
 9/23/2021 11:04:44 AM

Quant Time: Sep 22 05:08:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 22 05:02:48 2021
 Response via : Initial Calibration

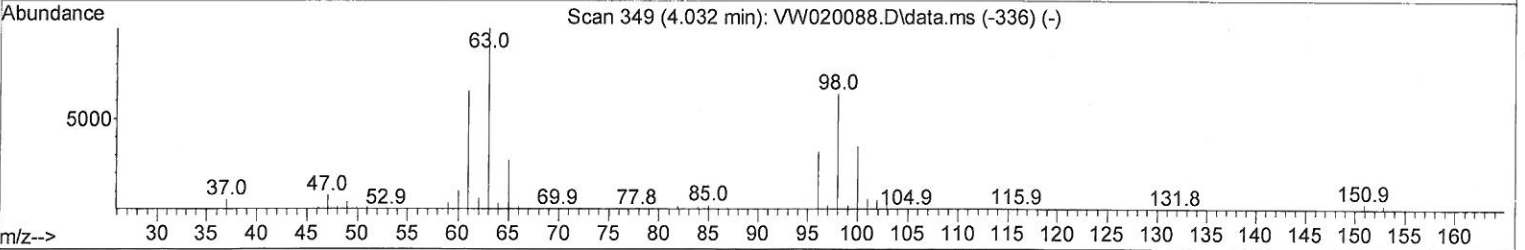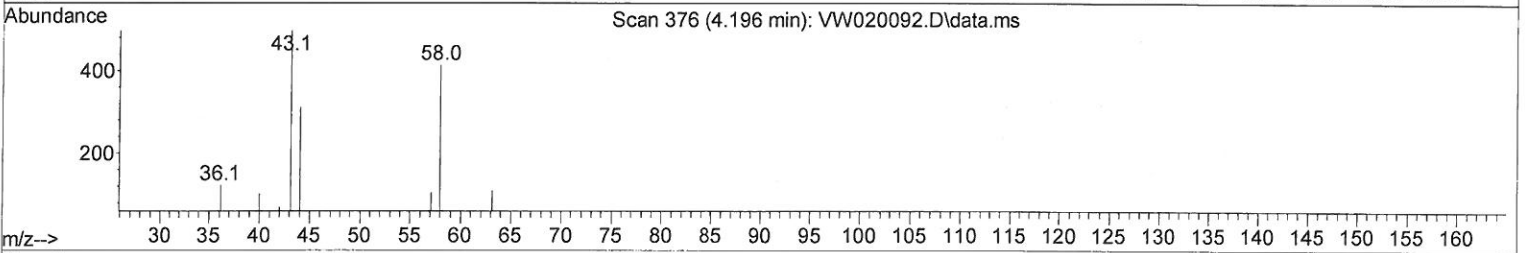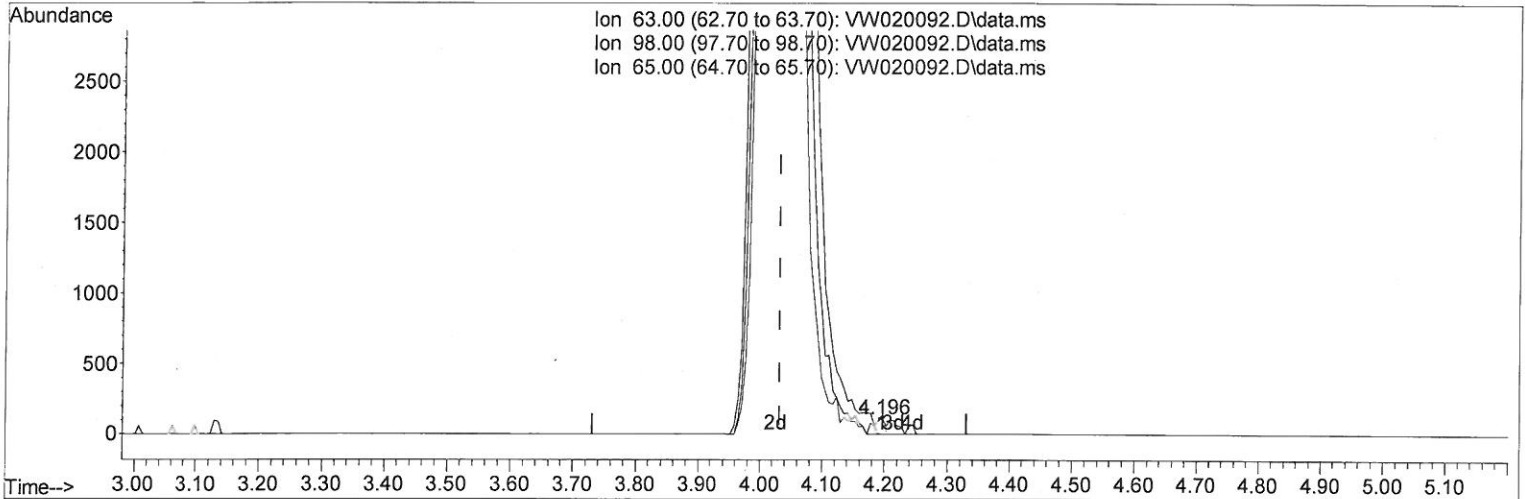

TIC: VW020092.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.196min (+ 0.165) 0.01 ug/L

response 93

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.60	52.69
65.00	23.90	24.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
 Data File : VW020092.D
 Acq On : 21 Sep 2021 15:05
 Operator : SY/VA
 Sample : M3813-04
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB6T0

Manual Integrations
 APPROVED

MMDadoda
 9/23/2021 11:04:44 AM

Quant Time: Sep 22 05:08:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 22 05:02:48 2021
 Response via : Initial Calibration

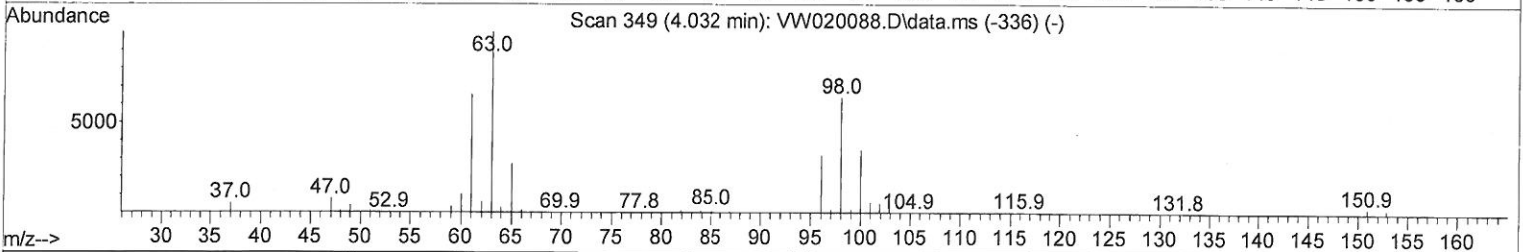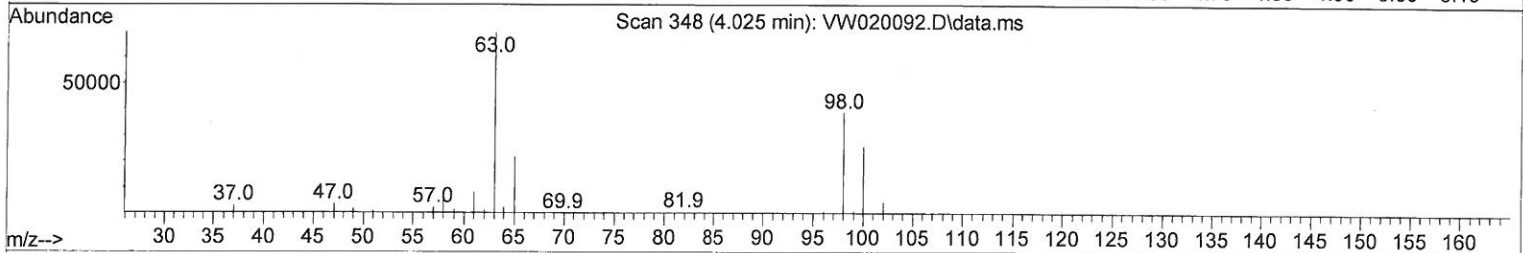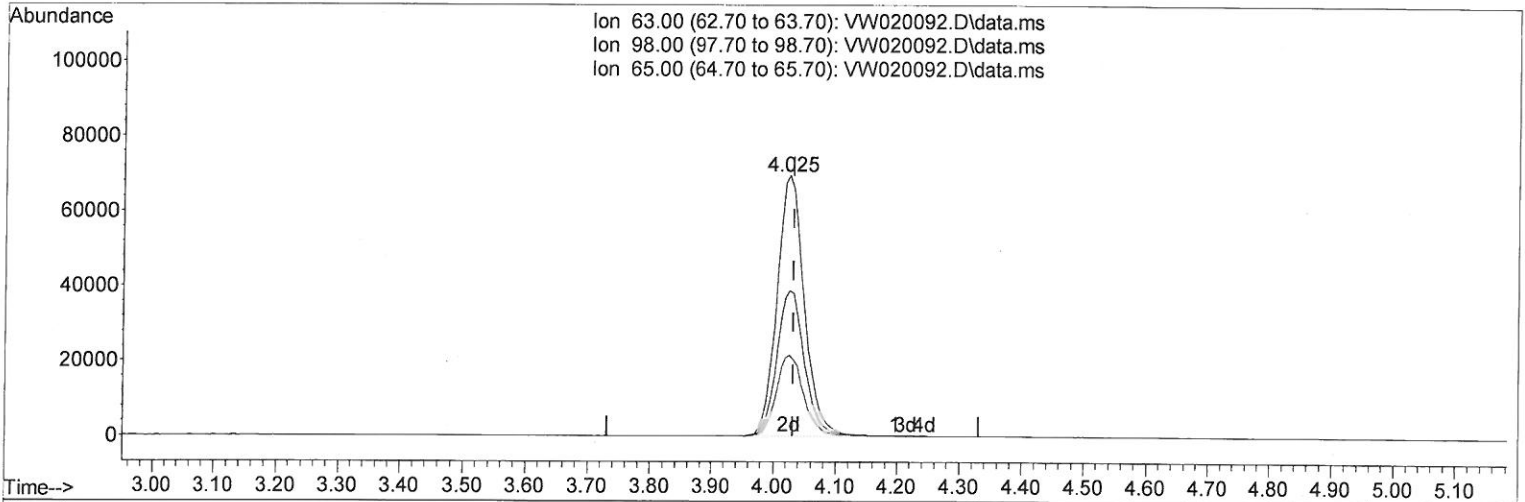

TIC: VW020092.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.025min (-0.006) 15.23 ug/L m

response 210210

Ion	Exp%	Act%
-----	------	------

63.00	100.00	100.00
-------	--------	--------

98.00	70.60	0.02#
-------	-------	-------

65.00	23.90	0.01#
-------	-------	-------

0.00	0.00	0.00
------	------	------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
 Data File : VW020092.D
 Acq On : 21 Sep 2021 15:05
 Operator : SY/VA
 Sample : M3813-04
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB6T0

Manual Integrations
 APPROVED

MMDadoda
 9/23/2021 11:04:44 AM

Quant Time: Sep 22 05:08:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 22 05:02:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	431003	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	399513	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	190151	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	165770	18.800	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	75.200%		
7) Chloroethane-d5	2.898	69	129853	19.549	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	78.200%		
11) 1,1-Dichloroethene-d2	4.025	63	210210m	15.226	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	60.920%		
21) 2-Butanone-d5	7.080	46	71460	52.519	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	105.040%		
24) Chloroform-d	7.653	84	273300	20.163	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	80.640%		
26) 1,2-Dichloroethane-d4	8.311	65	162818	22.318	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	89.280%		
32) Benzene-d6	8.281	84	527295	20.688	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	82.760%		
36) 1,2-Dichloropropane-d6	9.281	67	156898	21.270	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	85.080%		
41) Toluene-d8	10.329	98	480096	20.701	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	82.800%		
43) trans-1,3-Dichloroprop...	10.579	79	71664	22.730	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	90.920%		
47) 2-Hexanone-d5	10.927	63	58260	57.072	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	114.140%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	139262	24.475	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	97.920%		
66) 1,2-Dichlorobenzene-d4	13.853	152	155859	21.859	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	87.440%		
Target Compounds						
13) Acetone	4.135	43	30579	26.241	ug/L	92
16) Methylene chloride	4.922	84	16067	2.113	ug/L	96
22) 2-Butanone	7.183	43	4628	3.061	ug/L	95
42) Toluene	10.390	91	14927	0.583	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

09/24/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
Data File : VW020092.D
Acq On : 21 Sep 2021 15:05
Operator : SY/VA
Sample : M3813-04
Misc : 5.22g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GB6T0

Manual Integrations
APPROVED

MMDadoda
9/23/2021 11:04:44 AM

Quant Time: Sep 22 05:08:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 22 05:02:48 2021
Response via : Initial Calibration

