

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
 Data File : VW020108.D
 Acq On : 21 Sep 2021 21:51
 Operator : SY/VA
 Sample : M3837-03
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7T3

Manual Integrations
 APPROVED

MMDadoda
 9/23/2021 11:04:59 AM

Quant Time: Sep 22 05:11:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 22 05:02:48 2021
 Response via : Initial Calibration

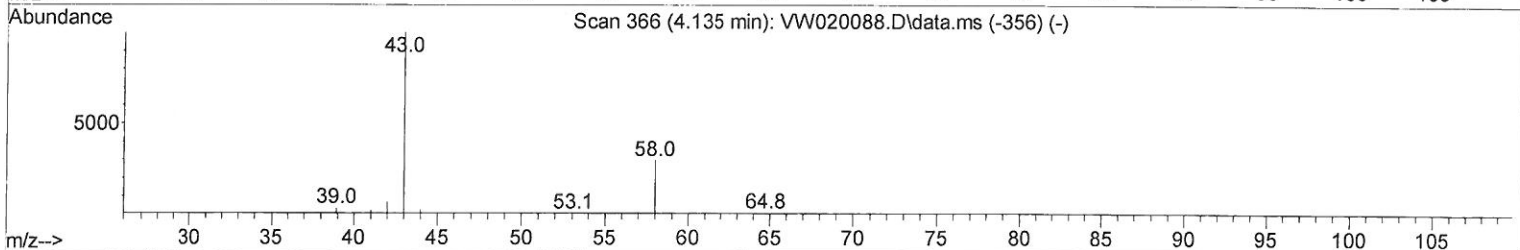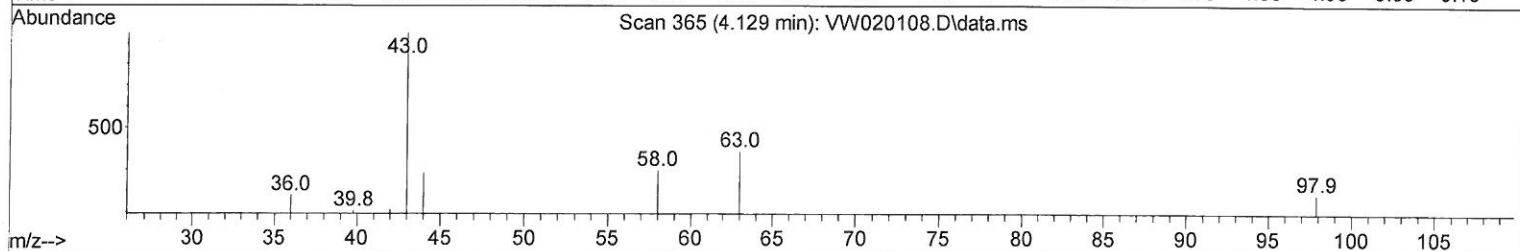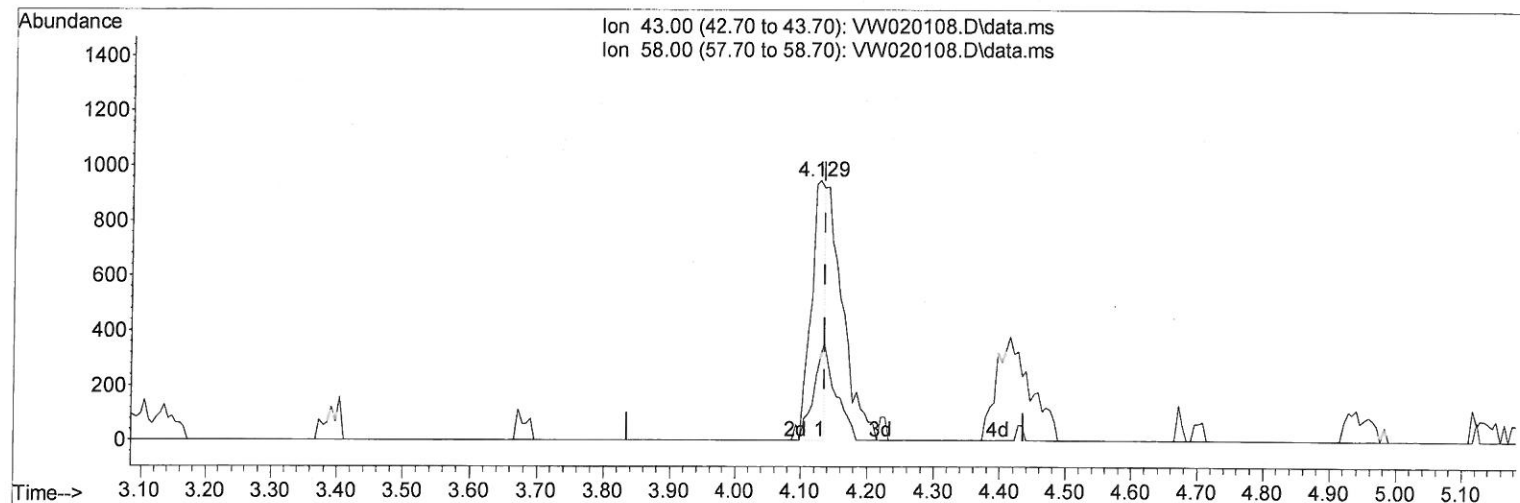

TIC: VW020108.D\data.ms

(13) Acetone (T)

4.129min (-0.006) 1.56 ug/L

response 1441

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.80	56.35
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
 Data File : VW020108.D
 Acq On : 21 Sep 2021 21:51
 Operator : SY/VA
 Sample : M3837-03
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7T3

Manual Integrations
 APPROVED

MMDadoda
 9/23/2021 11:04:59 AM

Quant Time: Sep 22 05:11:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 22 05:02:48 2021
 Response via : Initial Calibration

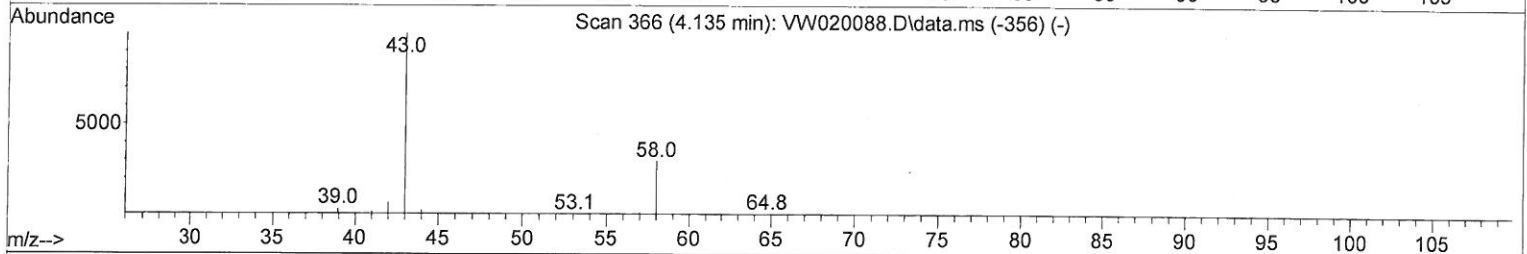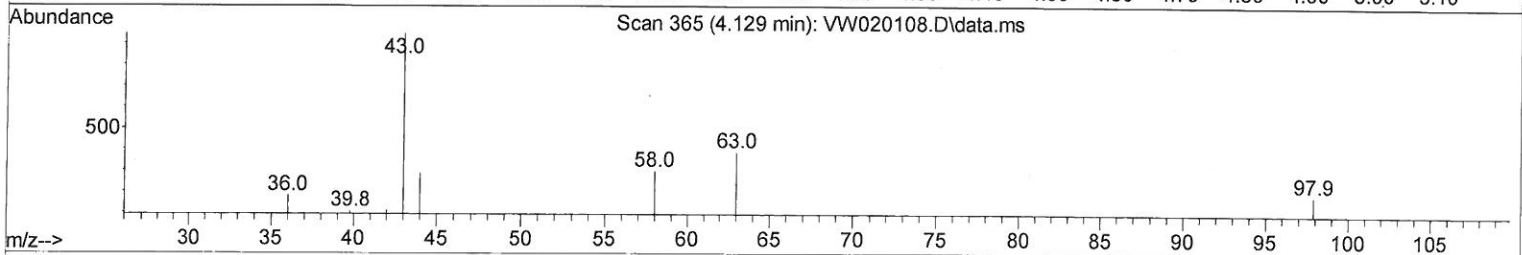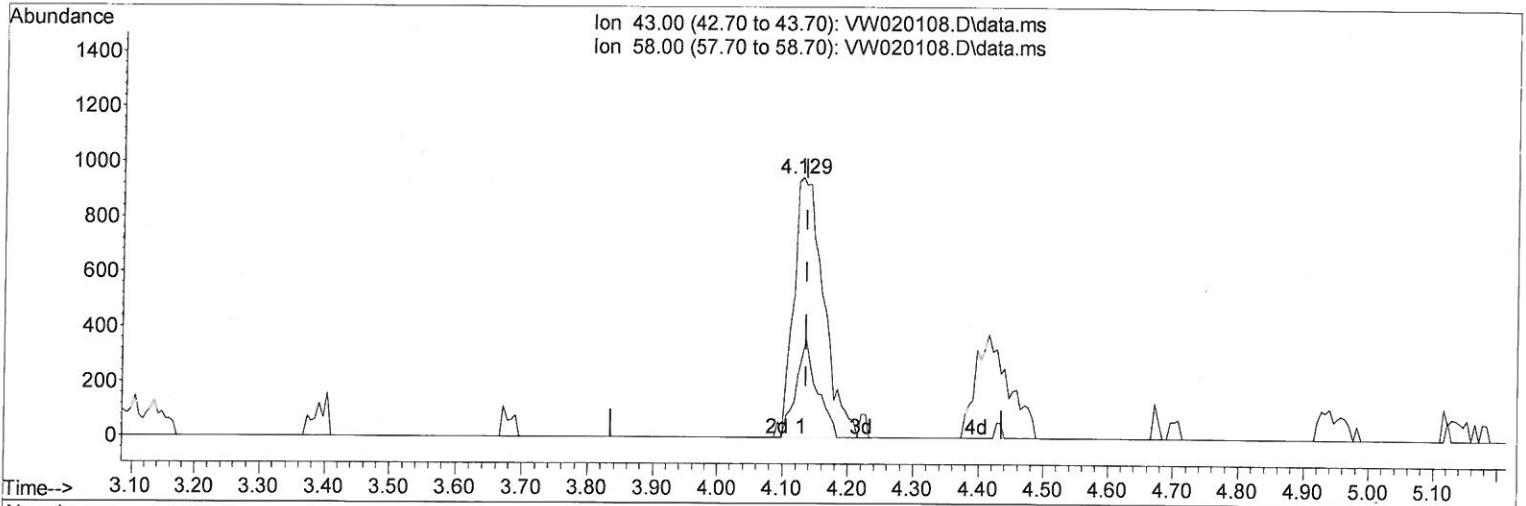

TIC: VW020108.D\data.ms

(13) Acetone (T)

4.129min (-0.006) 3.27 ug/L m

response 3011

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.80	26.97
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
 Data File : VW020108.D
 Acq On : 21 Sep 2021 21:51
 Operator : SY/VA
 Sample : M3837-03
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7T3

Manual Integrations
 APPROVED

MMDadoda
 9/23/2021 11:04:59 AM

Quant Time: Sep 22 05:11:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 22 05:02:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	340975	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	314228	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	127249	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	144794	20.757	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	83.040%	
7) Chloroethane-d5	2.897	69	116190	22.111	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	88.440%	
11) 1,1-Dichloroethene-d2	4.025	63	168791	15.454	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	61.800%	
21) 2-Butanone-d5	7.080	46	43307	40.232	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	80.460%	
24) Chloroform-d	7.653	84	238531	22.244	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	88.960%	
26) 1,2-Dichloroethane-d4	8.311	65	133018	23.048	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	92.200%	
32) Benzene-d6	8.281	84	456030	22.748	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	9.274	67	136489	23.525	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	94.120%	
41) Toluene-d8	10.329	98	401658	22.020	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	88.080%	
43) trans-1,3-Dichloroprop...	10.579	79	52419	21.139	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	84.560%	
47) 2-Hexanone-d5	10.927	63	33687	41.957	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	83.920%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	95813	21.409	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	85.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152	113523	23.792	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	95.160%	
Target Compounds						
13) Acetone	4.129	43	3011m	3.266	ug/L	Qvalue
16) Methylene chloride	4.922	84	52816	8.778	ug/L	96
34) Trichloroethene	9.091	95	3513	0.692	ug/L	95
42) Toluene	10.390	91	6524	0.324	ug/L	95
46) Tetrachloroethene	10.866	164	8602	2.192	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092121\
Data File : VW020108.D
Acq On : 21 Sep 2021 21:51
Operator : SY/VA
Sample : M3837-03
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW7T3

Manual Integrations
APPROVED

MMDadoda
9/23/2021 11:04:59 AM

Quant Time: Sep 22 05:11:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 22 05:02:48 2021
Response via : Initial Calibration

