


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW092218\
 Data File : VW005549.D
 Acq On : 21 Sep 2018 09:53
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
 Title : SW846 8260
 Last Update : Fri Sep 21 09:05:42 2018

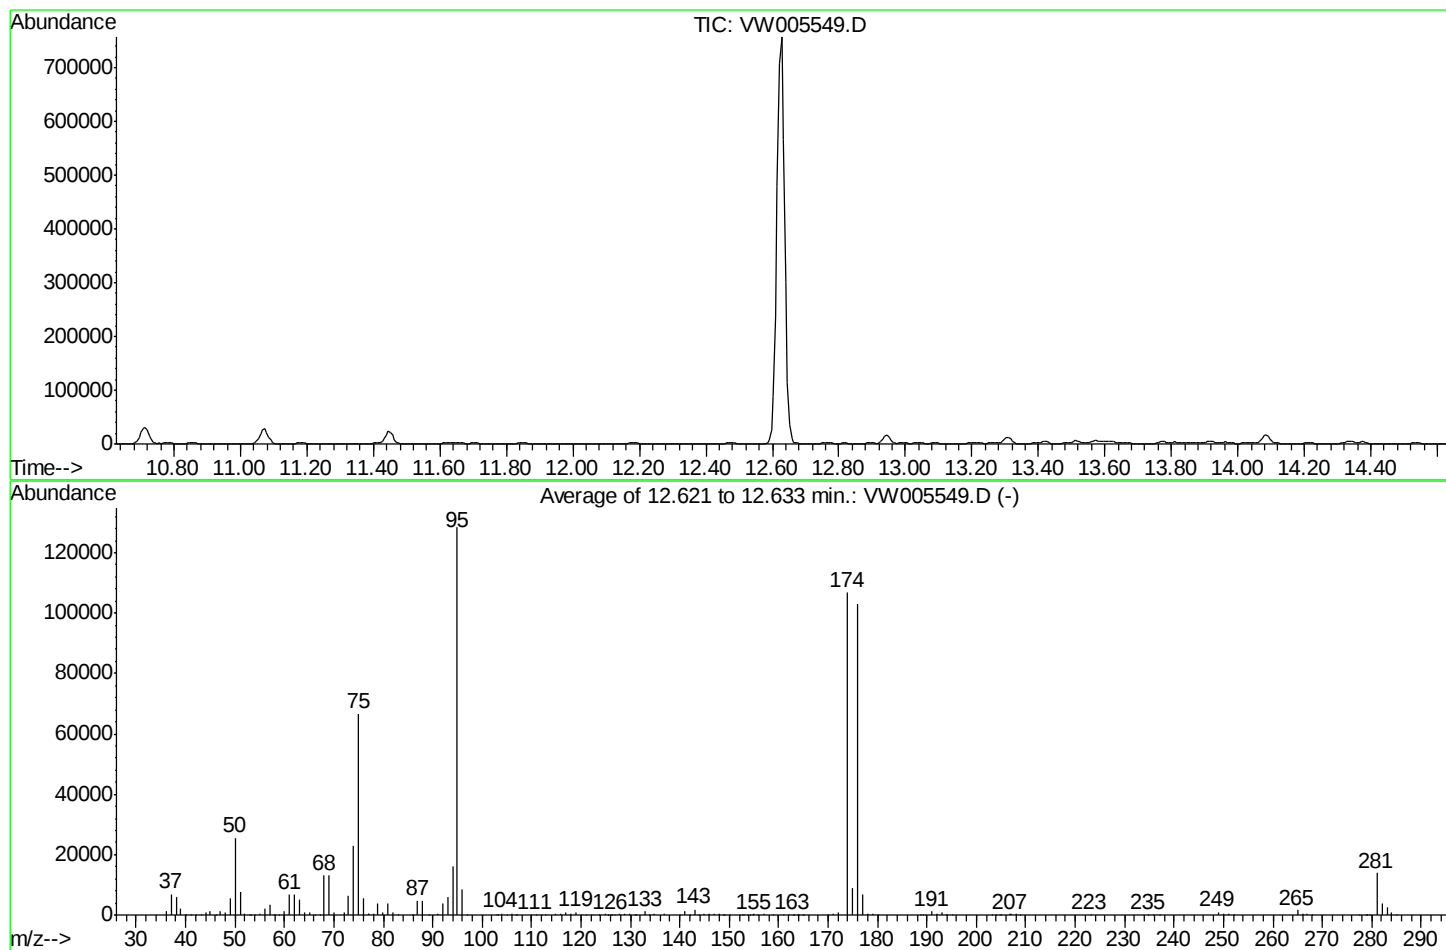

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	25640	PASS
75	95	30	60	51.9	66642	PASS
95	95	100	100	100.0	128421	PASS
96	95	5	9	6.7	8616	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.2	106834	PASS
175	174	5	9	8.4	8968	PASS
176	174	95	101	96.4	102992	PASS
177	176	5	9	6.8	7004	PASS