
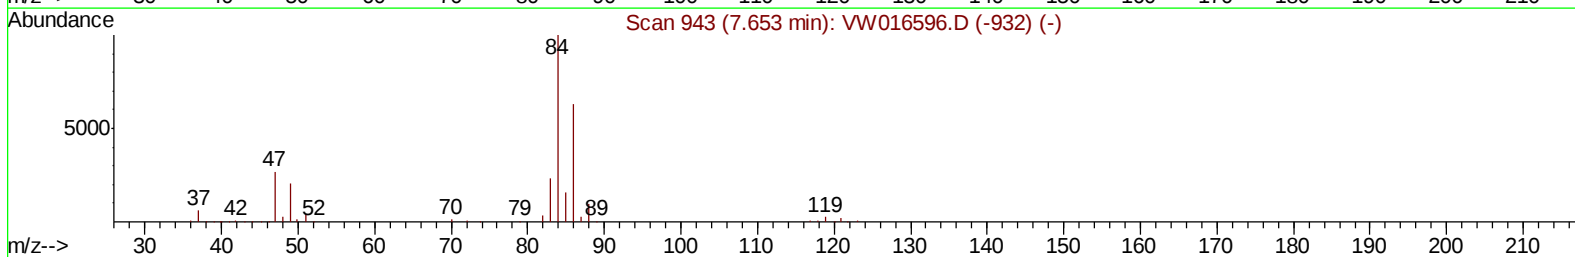
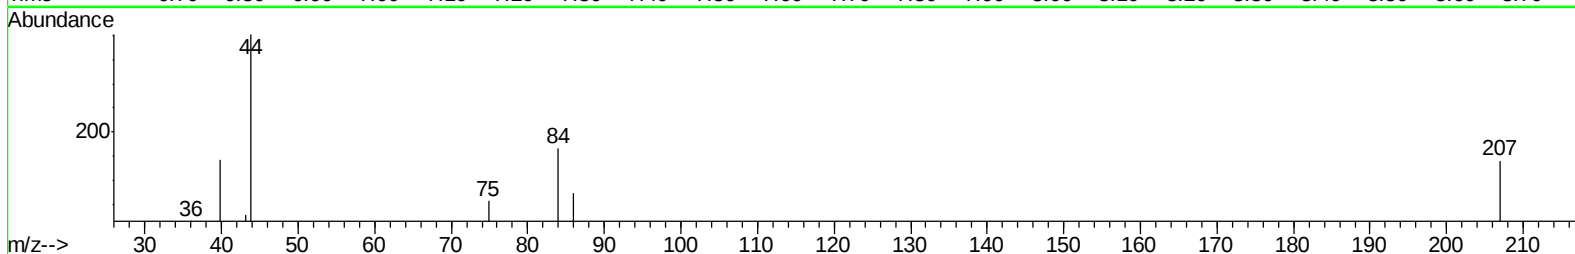


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092220\
Data File : VW016599.D
Acq On : 21 Sep 2020 16:29
Operator : SY/VA
Sample : VW0921SBL03
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Sep 22 03:01:15 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM091820SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 22 02:54:10 2020
Response via : Initial Calibration

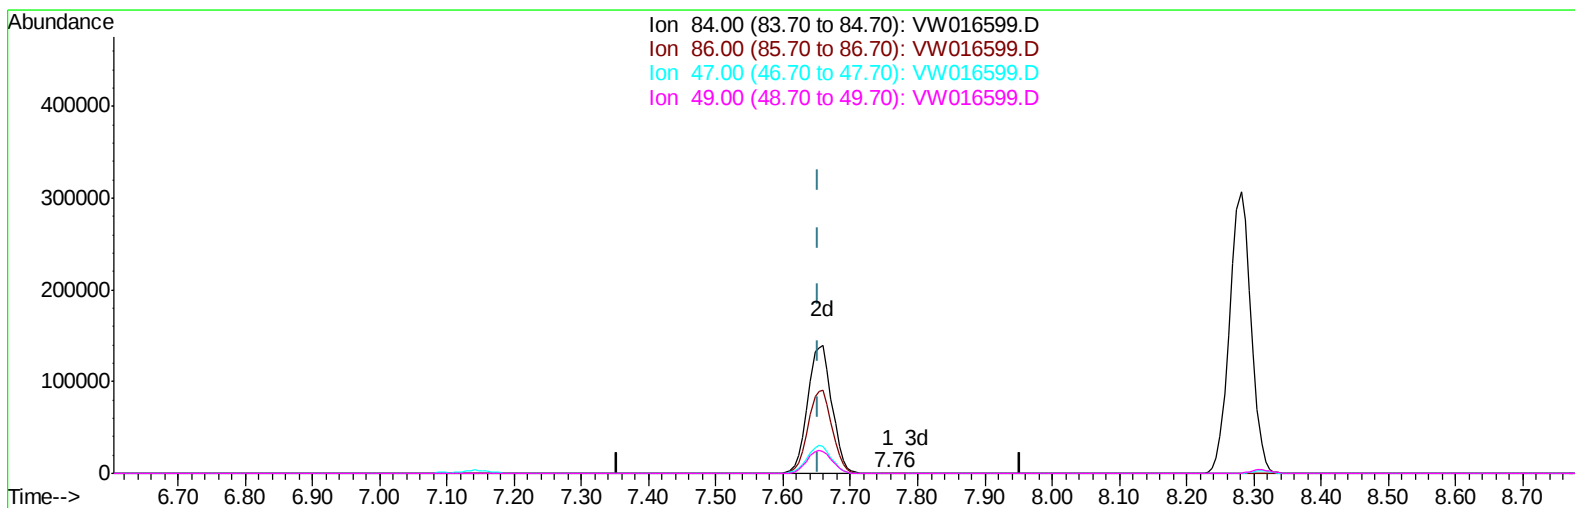

TIC: VW016599.D

(24) Chloroform-d (S)

7.756min (+0.104) 0.01ug/L

response 187

Ion	Exp%	Act%
84.00	100	100
86.00	63.00	74.87
47.00	43.20	33.69
49.00	25.30	18.72