

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092220\
 Data File : VW016598.D
 Acq On : 21 Sep 2020 16:05
 Operator : SY/VA
 Sample : VW0921SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK106

Quant Time: Sep 22 03:11:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM091820SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 22 02:54:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	523070	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	458477	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.56	152	232957	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	140740	24.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.36%
7) Chloroethane-d5	2.90	69	111137	23.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.68%
11) 1,1-Dichloroethene-d2	4.03	63	208318	16.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.60%
21) 2-Butanone-d5	7.09	46	80793	61.15	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.30%
24) Chloroform-d	7.65	84	288810	23.43	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.72%
26) 1,2-Dichloroethane-d4	8.31	65	160230	25.46	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.84%
32) Benzene-d6	8.28	84	561996	24.00	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	9.28	67	156488	24.30	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.20%
41) Toluene-d8	10.33	98	540498	23.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.64%
43) trans-1,3-Dichloropropene-	10.58	79	77758	24.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.56%
47) 2-Hexanone-d5	10.93	63	64534	63.67	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.34%
56) 1,1,2,2-Tetrachloroethane-	12.69	84	144620	28.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.40%
66) 1,2-Dichlorobenzene-d4	13.85	152	207949	24.65	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.60%


Target Compounds					Ovalue
16) Methylene chloride	4.93	84	13465	1.757 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092220\
Data File : VW016598.D
Acq On : 21 Sep 2020 16:05
Operator : SY/VA
Sample : VW0921SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK106

Quant Time: Sep 22 03:11:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM091820SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 22 02:54:10 2020
Response via : Initial Calibration

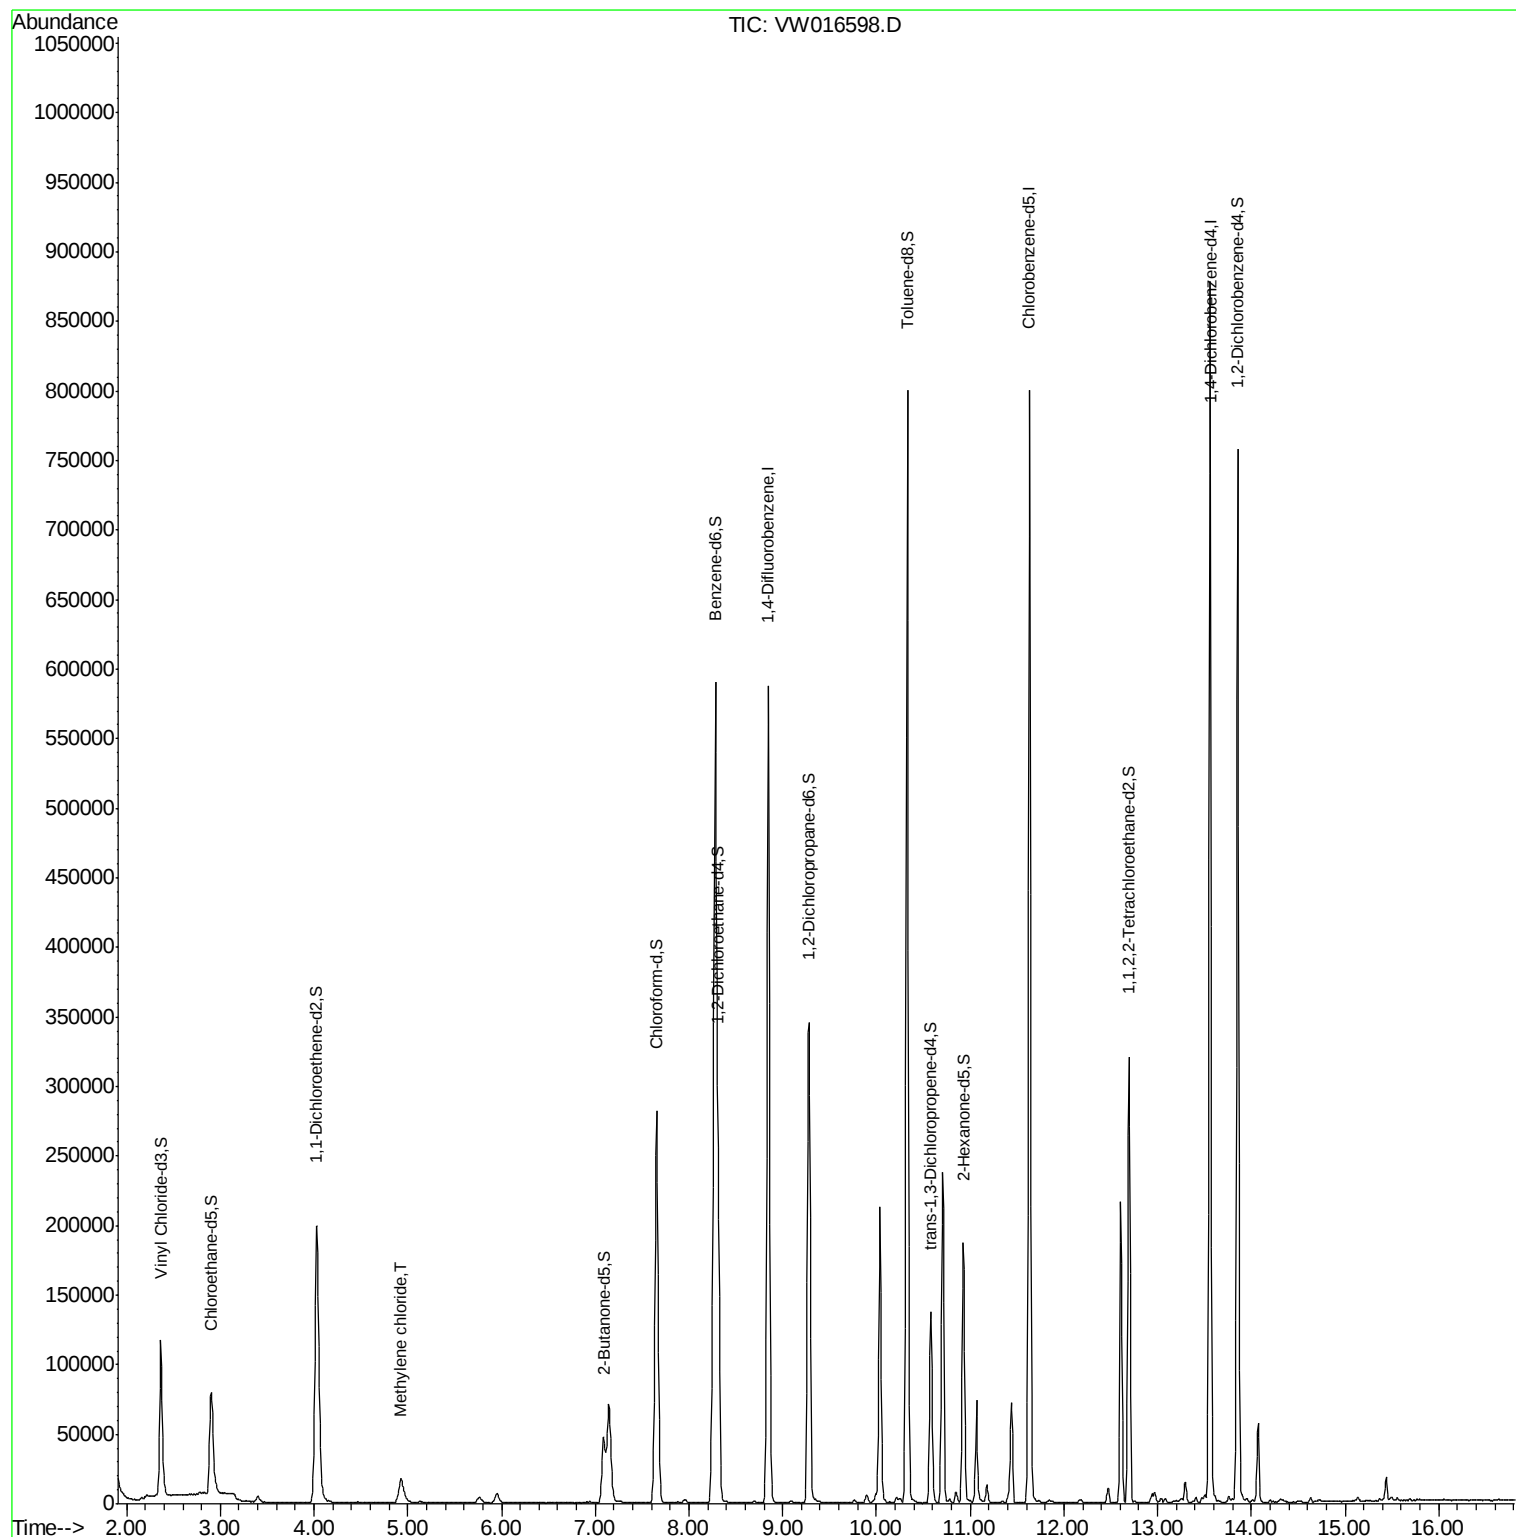

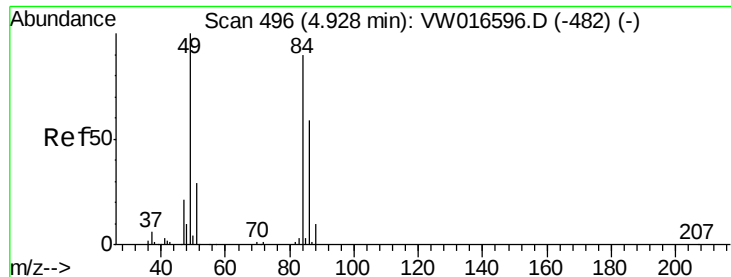

#16
 Methvlene chloride
 Concen: 1.757 ug/L
 RT: 4.93 min Scan# 497
 Delta R.T. 0.01 min
 Lab File: VW016598.D
 Acq: 21 Sep 2020 16:05

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK106

Tot Ion	Ion	Ratio	Lower	Upper
84	100			
86	57.7	46.2	85.8	
49	95.4	82.8	153.8	

