

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016606.D
 Acq On : 22 Sep 2020 13:31
 Operator : SY/VA
 Sample : L4110-02
 Misc : 3.60G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AL0

Quant Time: Sep 23 07:28:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	665709	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	547134	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	224262	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	176078	27.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.32%
7) Chloroethane-d5	2.91	69	147563	28.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.20%
10) 1,1-Dichloroethene-d2	4.03	63	271043	18.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.24%
20) 2-Butanone-d5	7.09	46	55080	31.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.70%
24) Chloroform-d	7.65	84	345100	24.78	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.12%
26) 1,2-Dichloroethane-d4	8.31	65	164046	22.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.80%
29) Benzene-d6	8.28	84	685614	27.94	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.76%
33) 1,2-Dichloropropane-d6	9.28	67	181770	27.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.36%
37) Toluene-d8	10.33	98	654064	27.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.36%
38) trans-1,3-Dichloropropene-	10.58	79	74894	22.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.36%
39) 2-Hexanone-d5	10.93	63	44915	37.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.28%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	112150	19.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.28%
61) 1,2-Dichlorobenzene-d4	13.85	152	182569	25.48	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.92%

Target Compounds


					Ovalue
13) Acetone	4.15	43	1541	1.120 ug/L	98
16) Methylene chloride	4.93	84	56055	5.460 ug/L	96
59) 1,2,3-Trichloropropane	13.56	75	24915	5.206 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092320\
Data File : VW016606.D
Acq On : 22 Sep 2020 13:31
Operator : SY/VA
Sample : L4110-02
Misc : 3.60G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AL0

Quant Time: Sep 23 07:28:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 23 07:21:48 2020
Response via : Initial Calibration

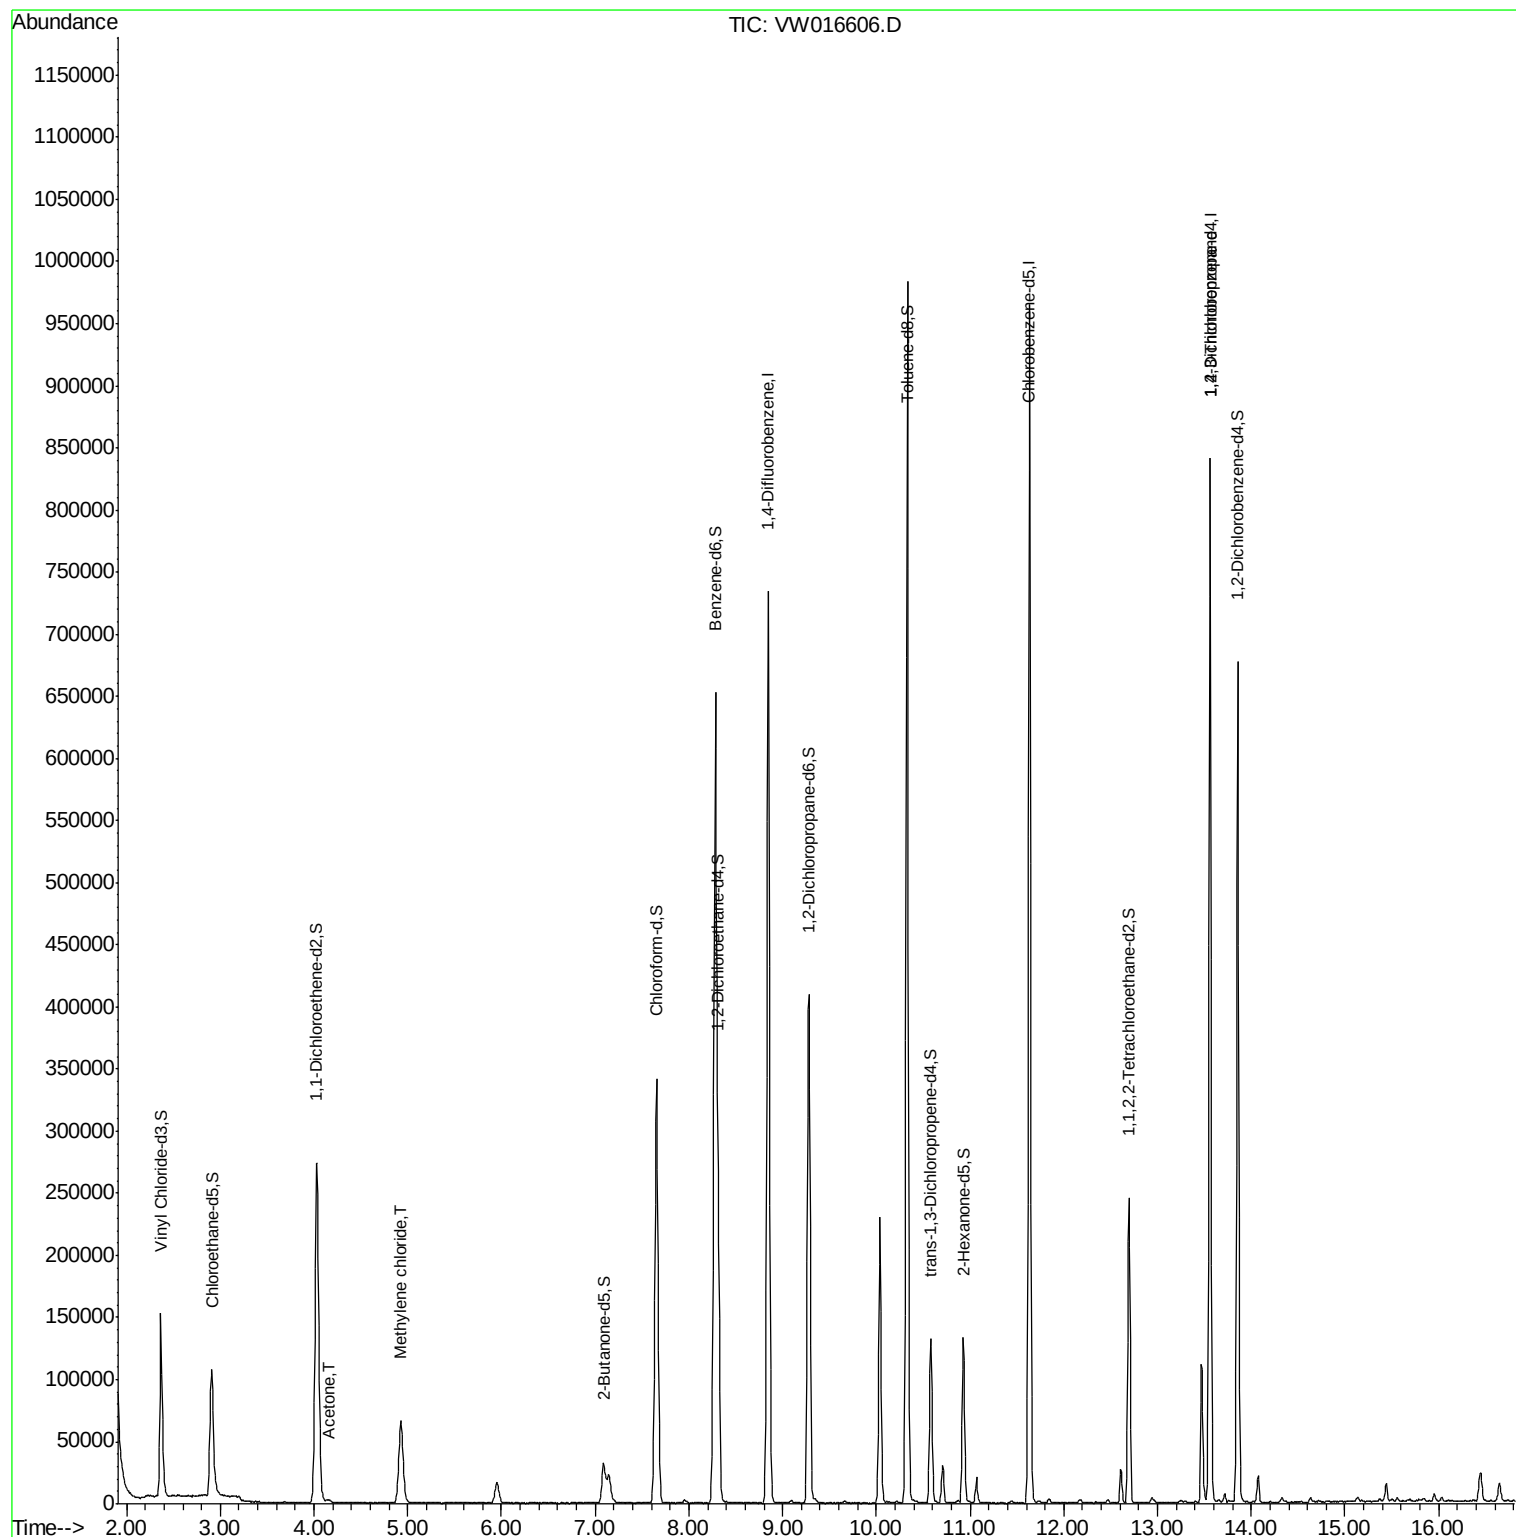

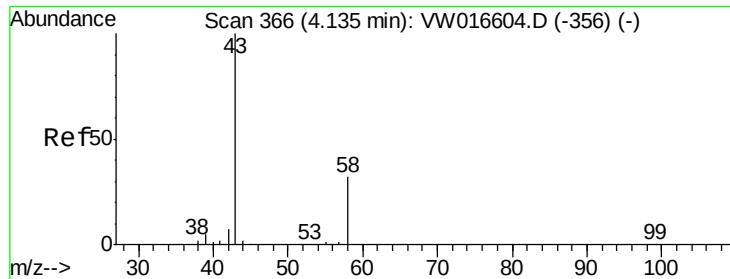

#13

Acetone

Concen: 1.120 ug/L

RT: 4.15 min Scan# 368

Delta R.T. 0.01 min

Lab File: VW016606.D

Acq: 22 Sep 2020 13:31

Instrument :

MSVOA_W

ClientSampled :





COAL0

Tot Ion: 43 Resp: 1541

Ion Ratio Lower Upper

43 100

58 28.9 0.0 60.2

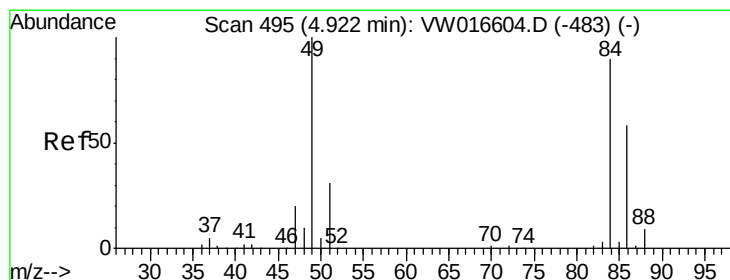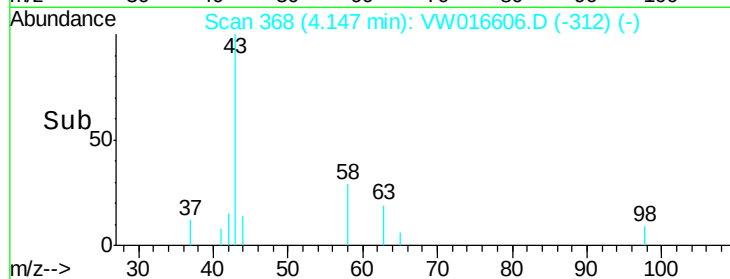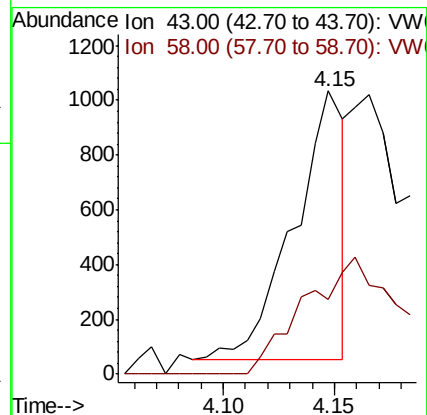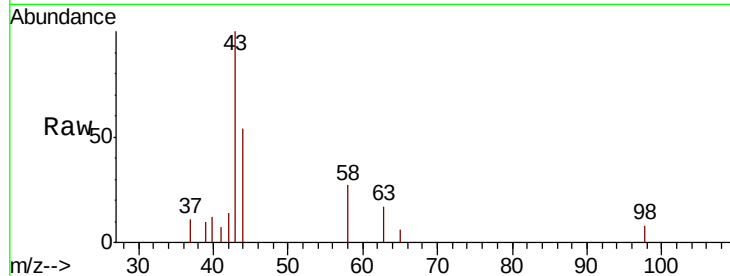

#16

Methylene chloride

Concen: 5.460 ug/L

RT: 4.93 min Scan# 496

Delta R.T. 0.01 min

Lab File: VW016606.D

Acq: 22 Sep 2020 13:31




Tgt Ion: 84 Resp: 56055


Ion Ratio Lower Upper

84 100

49 106.0 76.0 141.2

86 60.7 45.6 84.6

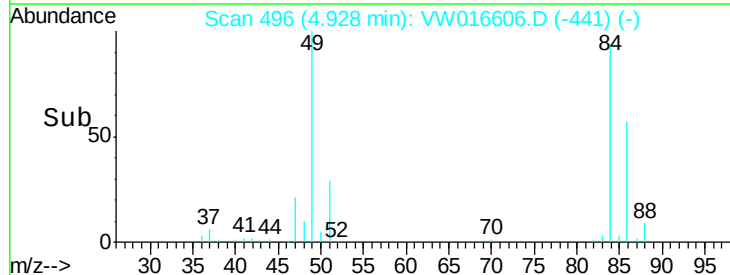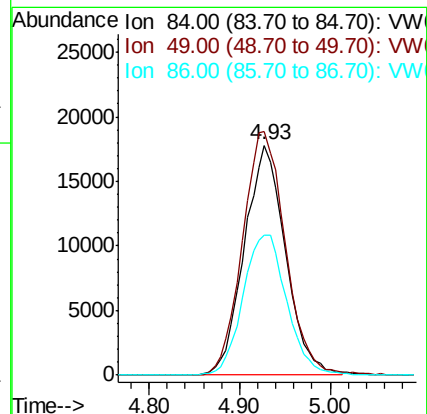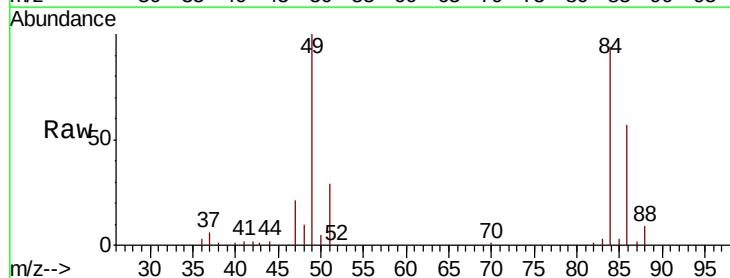

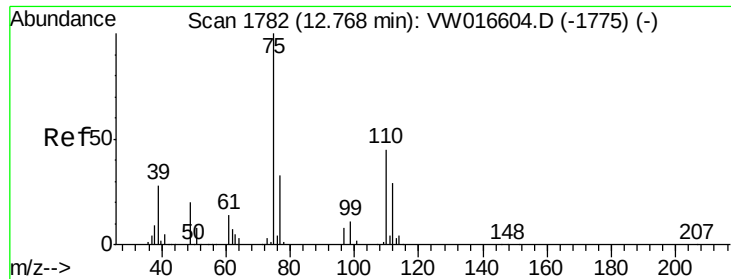

#59

1,2,3-Trichloropropane

Concen: 5.206 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW016606.D

Acq: 22 Sep 2020 13:31

Instrument :

MSVOA_W

ClientSampleId :

C0AL0

Tot Ion: 75 Resp: 24915

Ion Ratio Lower Upper

75 100

77 38.5 26.2 39.4

