

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016606.D
 Acq On : 22 Sep 2020 13:31
 Operator : SY/VA
 Sample : L4110-02
 Misc : 3.60G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 COAL0

Manual Integrations
APPROVED

MMDadoda
 9/28/2020 3:15:53 PM

Quant Time: Sep 23 07:40:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

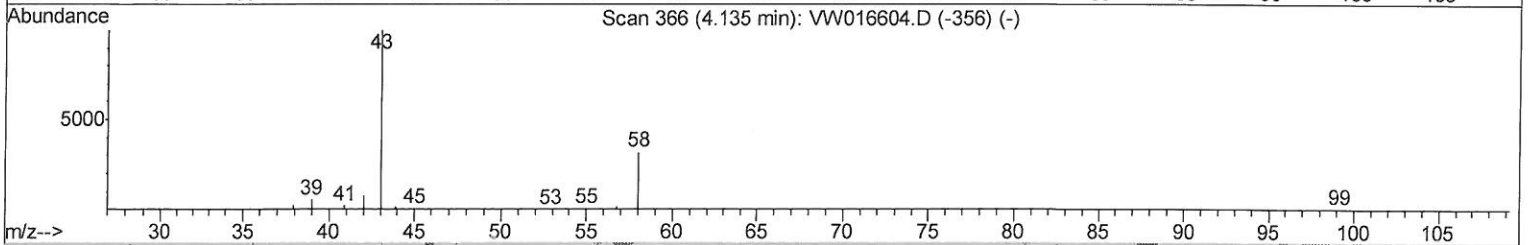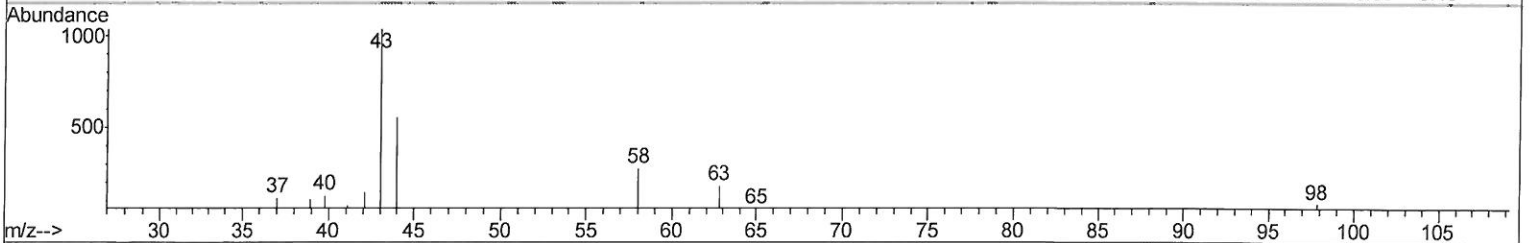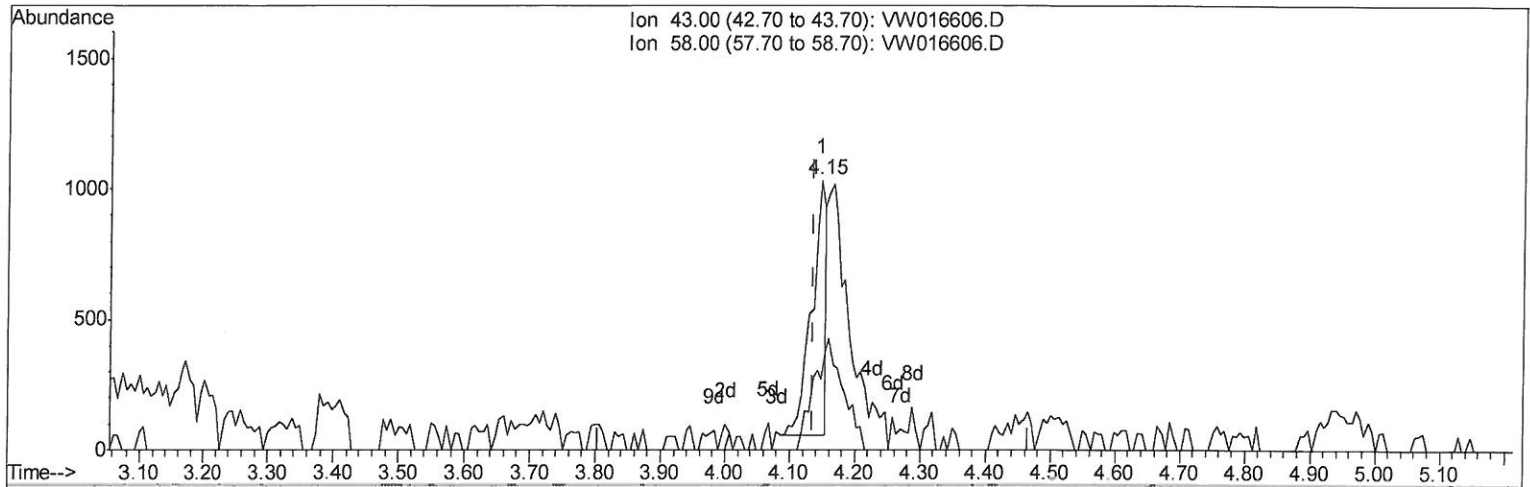

TIC: VW016606.D

(13) Acetone (T)
 4.147min (+0.012) 1.12ug/L
 response 1541

Ion	Exp%	Act%
43.00	100	100
58.00	30.10	28.88
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016606.D
 Acq On : 22 Sep 2020 13:31
 Operator : SY/VA
 Sample : L4110-02
 Misc : 3.60G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 COAL0

Manual Integrations
APPROVED

MMDadoda
 9/28/2020 3:15:53 PM

Quant Time: Sep 23 07:40:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

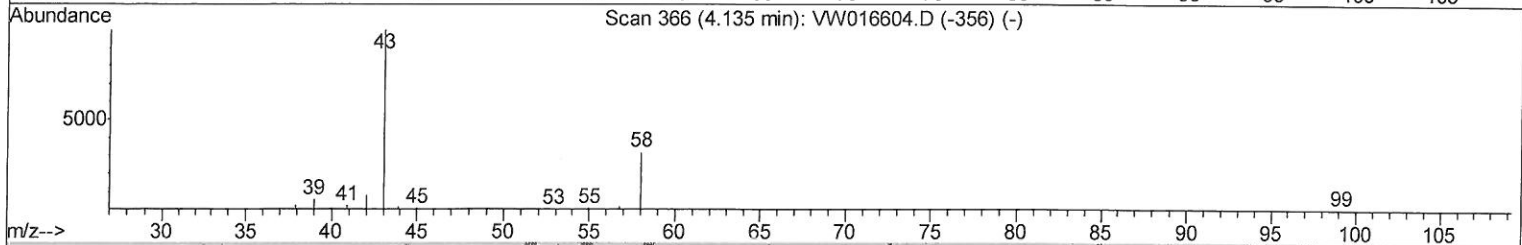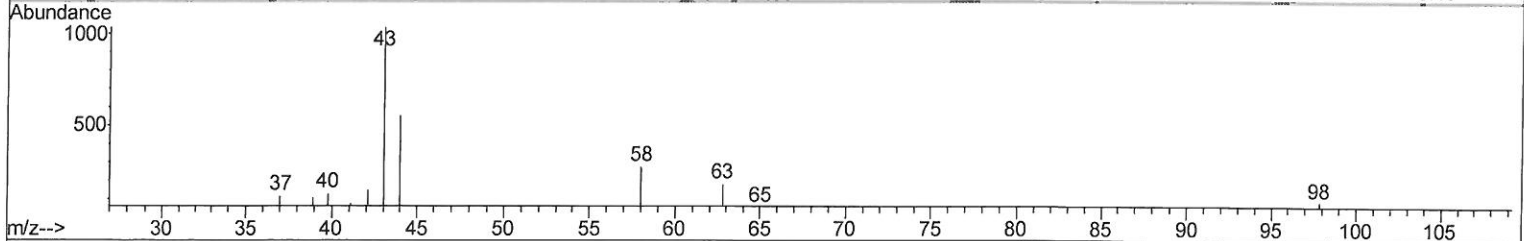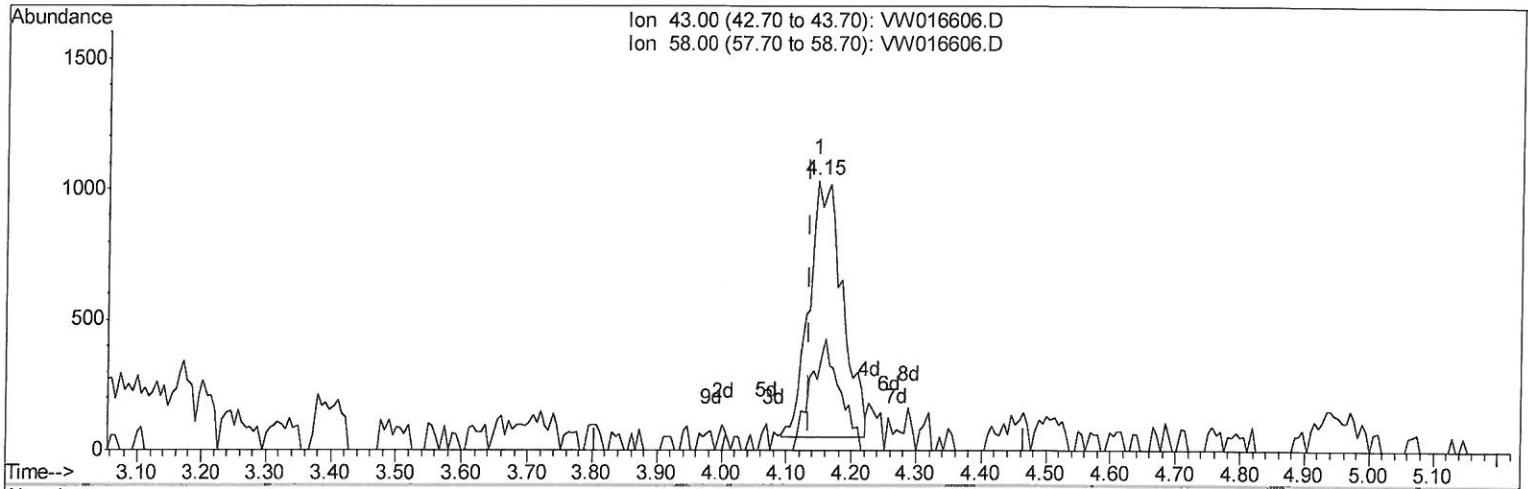

TIC: VW016606.D

(13) Acetone (T)

4.147min (+0.012) 2.53ug/L m

response 3488

Ion	Exp%	Act%
43.00	100	100
58.00	30.10	12.76
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten signature: 9/29/20 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016606.D
 Acq On : 22 Sep 2020 13:31
 Operator : SY/VA
 Sample : L4110-02
 Misc : 3.60G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleID :
 COALO

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:15:53 PM

Quant Time: Sep 23 07:49:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	665709	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	547134	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	224262	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	176078	27.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.32%
7) Chloroethane-d5	2.91	69	147563	28.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.20%
10) 1,1-Dichloroethene-d2	4.03	63	271043	18.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.24%
20) 2-Butanone-d5	7.09	46	55080	31.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.70%
24) Chloroform-d	7.65	84	345100	24.78	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.12%
26) 1,2-Dichloroethane-d4	8.31	65	164046	22.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.80%
29) Benzene-d6	8.28	84	685614	27.94	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.76%
33) 1,2-Dichloropropane-d6	9.28	67	181770	27.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.36%
37) Toluene-d8	10.33	98	654064	27.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.36%
38) trans-1,3-Dichloropropene-	10.58	79	74894	22.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.36%
39) 2-Hexanone-d5	10.93	63	44915	37.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.28%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	112150	19.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.28%
61) 1,2-Dichlorobenzene-d4	13.85	152	182569	25.48	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.92%

Target Compounds

13) Acetone	4.15	43	3488m	2.535	ug/L	Ovalue
16) Methylene chloride	4.93	84	56055	5.460	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
Data File : VW016606.D
Acq On : 22 Sep 2020 13:31
Operator : SY/VA
Sample : L4110-02
Misc : 3.60G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
COAL0

Manual Integrations
APPROVED

MMDadoda
9/28/2020 3:15:53 PM

Quant Time: Sep 23 07:49:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 23 07:21:48 2020
Response via : Initial Calibration

