

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016614.D
 Acq On : 22 Sep 2020 16:41
 Operator : SY/VA
 Sample : L4109-04
 Misc : 6.04G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3W8

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:16:18 PM

Quant Time: Sep 23 07:30:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

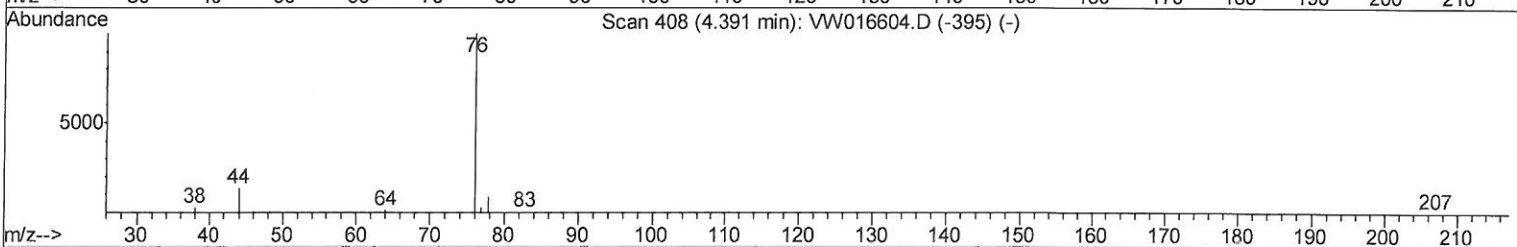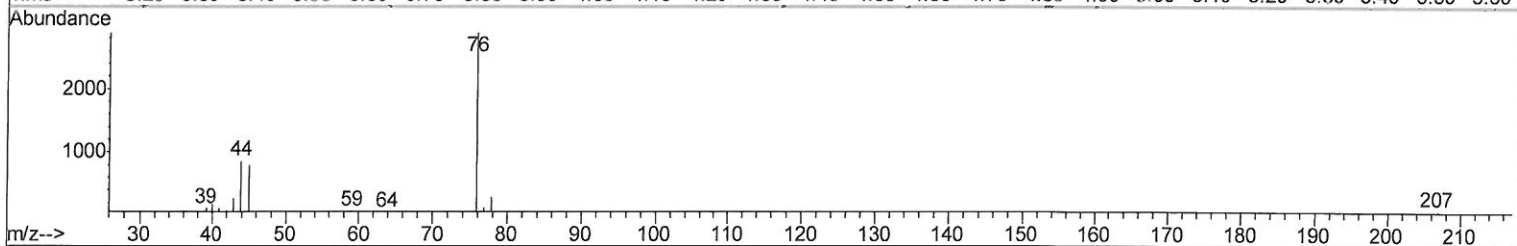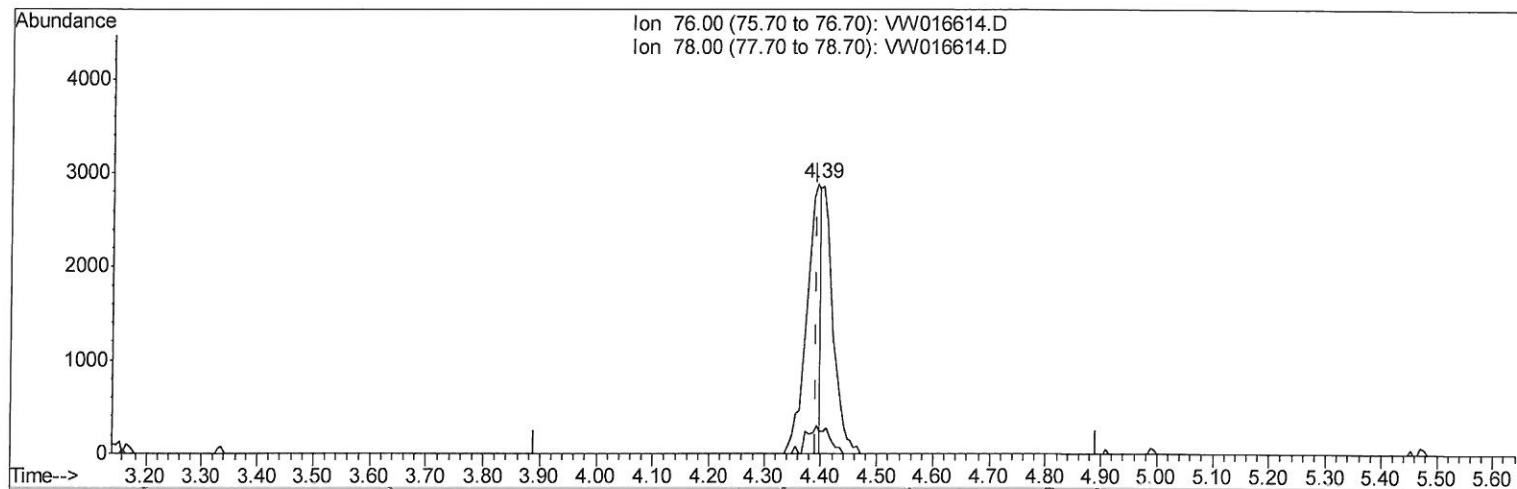

TIC: VW016614.D

(14) Carbon disulfide (T)

4.391min (0.000) 0.19ug/L

response 5109

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	10.27
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016614.D
 Acq On : 22 Sep 2020 16:41
 Operator : SY/VA
 Sample : L4109-04
 Misc : 6.04G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3W8

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:16:18 PM

Quant Time: Sep 23 07:30:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

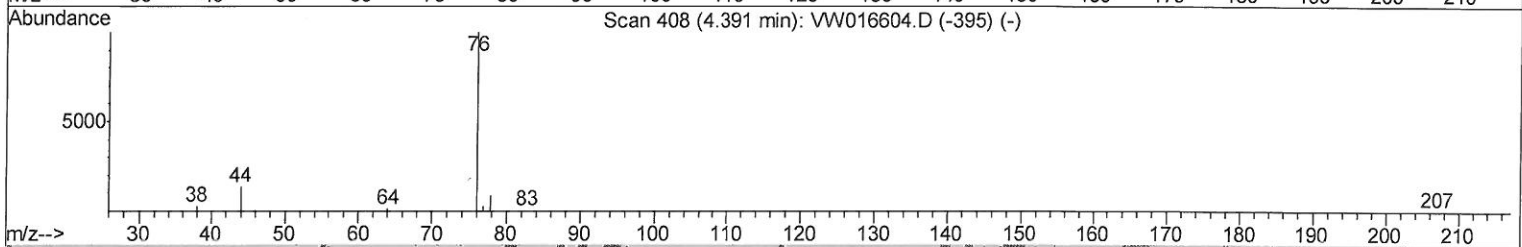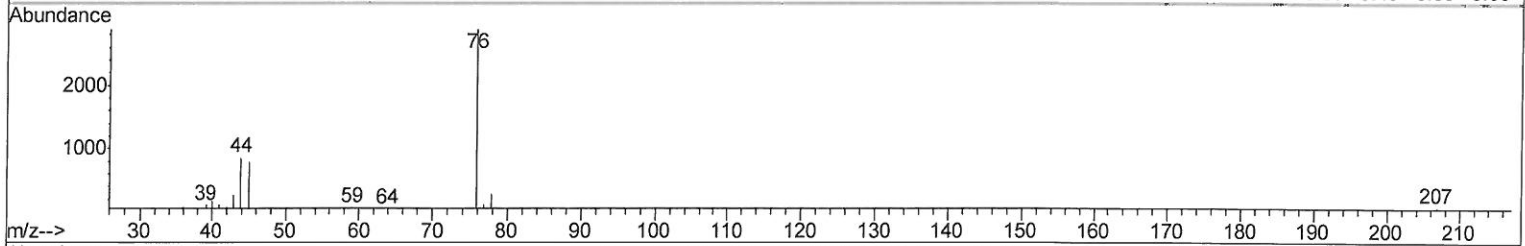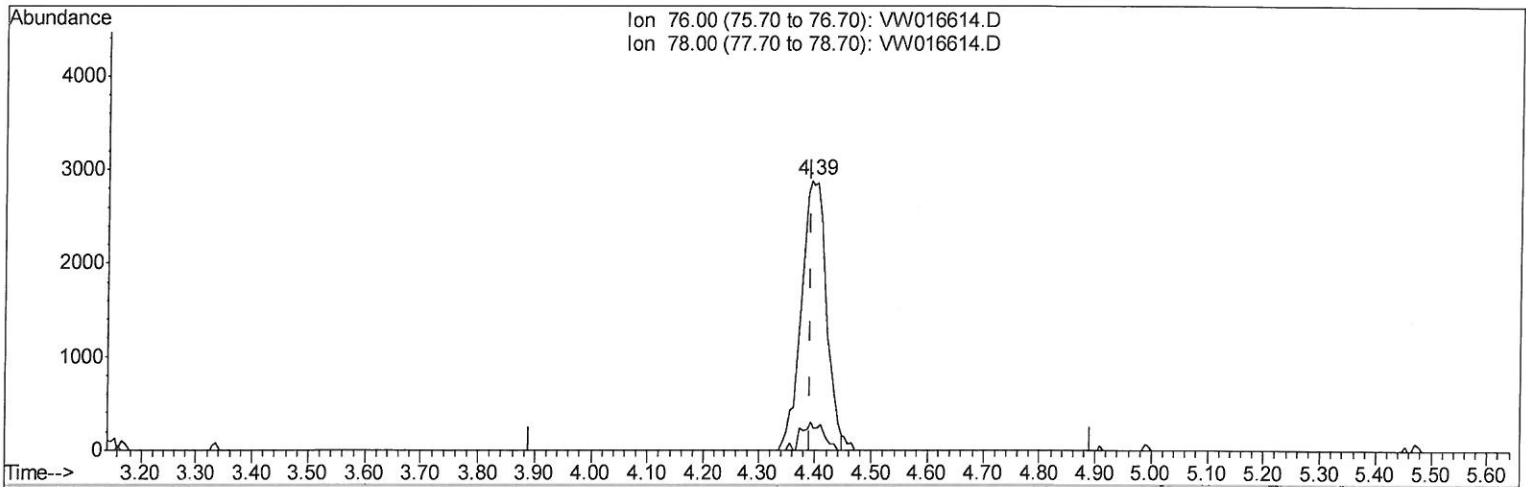

TIC: VW016614.D

(14) Carbon disulfide (T)

4.391min (0.000) 0.33ug/L m

response 8859

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	10.27
0.00	0.00	0.00
0.00	0.00	0.00

09/29/2020

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016614.D
 Acq On : 22 Sep 2020 16:41
 Operator : SY/VA
 Sample : L4109-04
 Misc : 6.04G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BG3W8

Manual Integrations
APPROVED

MMDadoda
 9/28/2020 3:16:18 PM

Quant Time: Sep 23 07:30:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

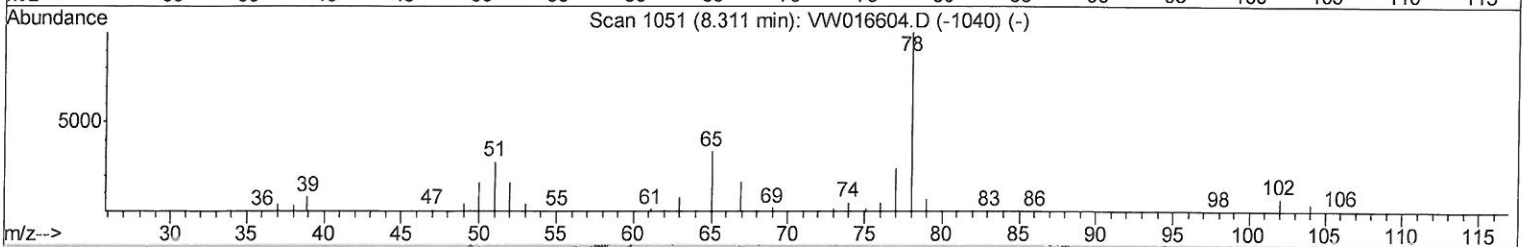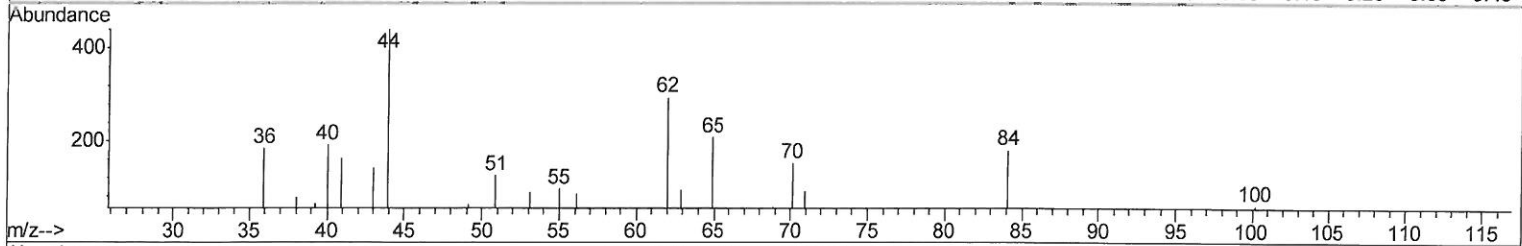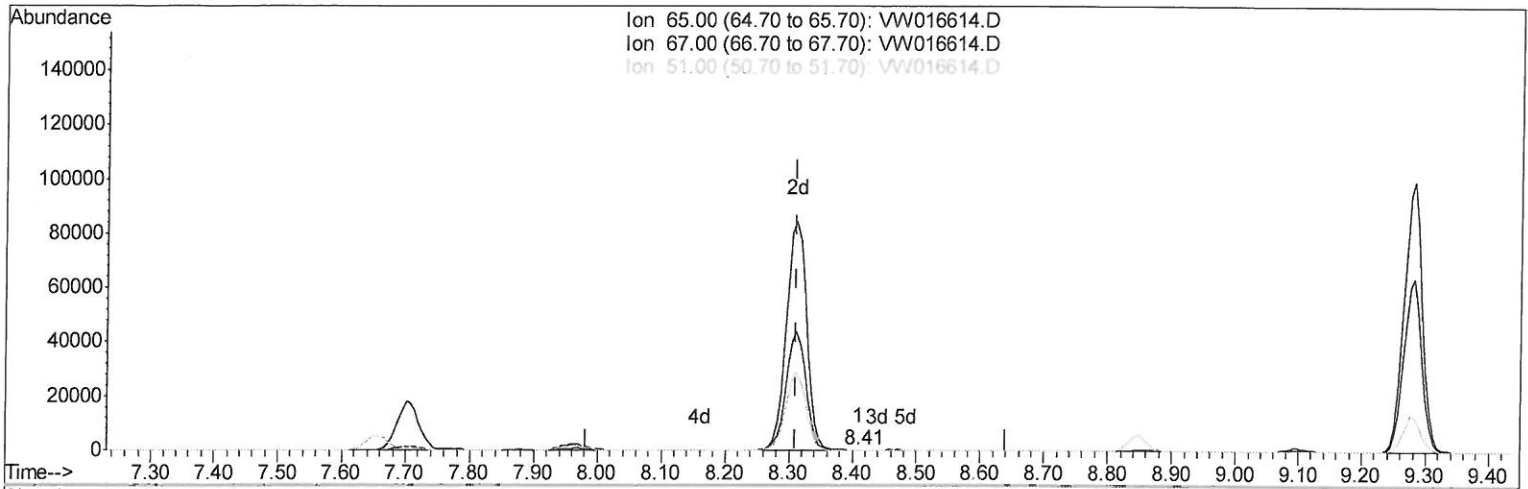

TIC: VW016614.D

(26) 1,2-Dichloroethane-d4 (S)

8.409min (+0.098) 0.03ug/L

response 191

Ion	Exp%	Act%
65.00	100	100
67.00	52.90	39.79
51.00	113.40	80.10
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016614.D
 Acq On : 22 Sep 2020 16:41
 Operator : SY/VA
 Sample : L4109-04
 Misc : 6.04G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BG3W8

Manual Integrations
APPROVED

MMDadoda
 9/28/2020 3:16:18 PM

Quant Time: Sep 23 07:30:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

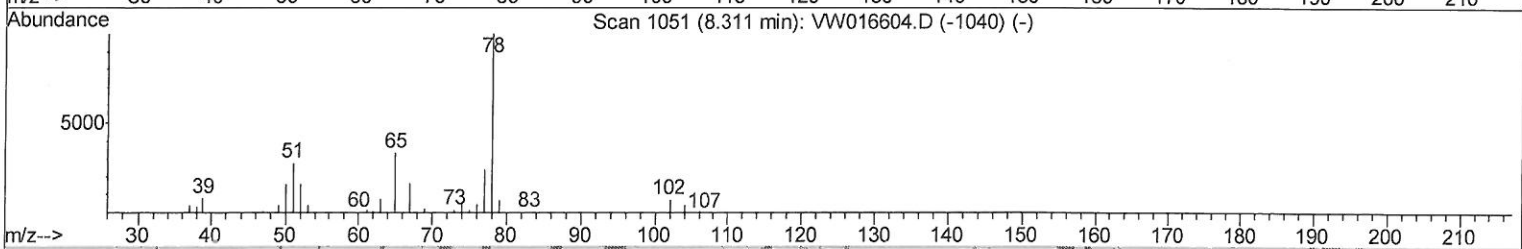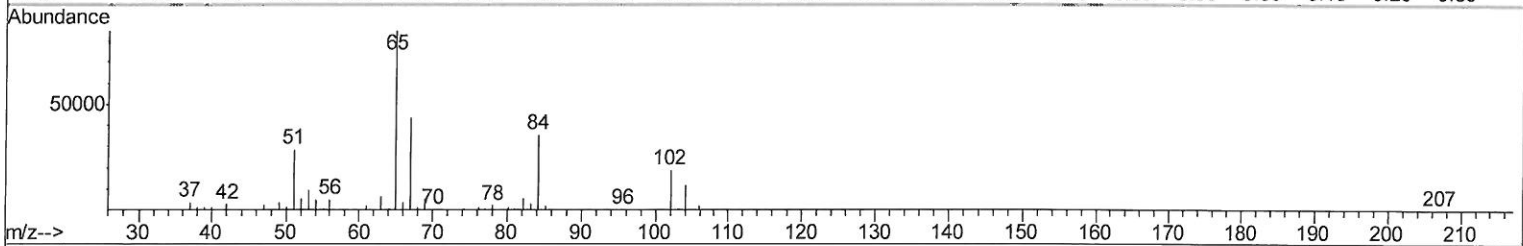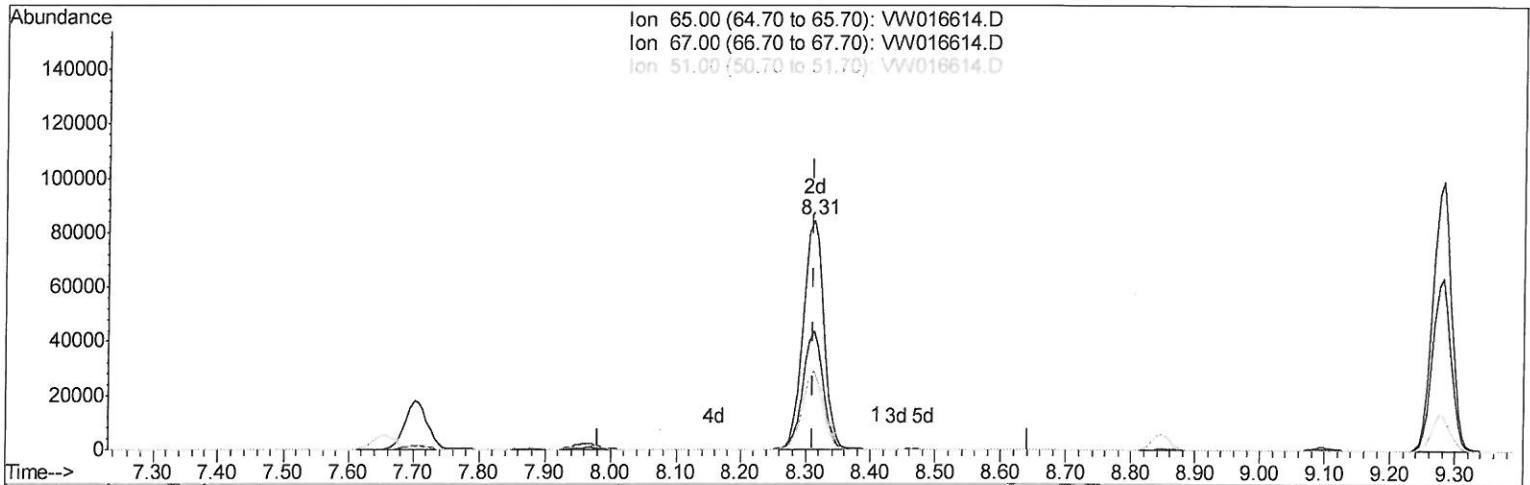

TIC: VW016614.D

(26) 1,2-Dichloroethane-d4 (S)

8.311min (0.000) 24.98ug/L m

> 09/29/20 84

response 186705

Ion	Exp%	Act%
65.00	100	100
67.00	52.90	0.04#
51.00	113.40	0.08#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
 Data File : VW016614.D
 Acq On : 22 Sep 2020 16:41
 Operator : SY/VA
 Sample : L4109-04
 Misc : 6.04G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3W8

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:16:18 PM

Quant Time: Sep 23 08:44:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 07:21:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	695923	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	611487	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	298141	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	171477	25.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.84%
7) Chloroethane-d5	2.90	69	146707	26.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.68%
10) 1,1-Dichloroethene-d2	4.03	63	323144	21.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.84%
20) 2-Butanone-d5	7.09	46	76222	41.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.00%
24) Chloroform-d	7.65	84	361960	24.86	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.44%
26) 1,2-Dichloroethane-d4	8.31	65	186705m	24.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.92%
29) Benzene-d6	8.28	84	718397	26.20	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.80%
33) 1,2-Dichloropropane-d6	9.28	67	197177	26.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.12%
37) Toluene-d8	10.33	98	700975	25.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.92%
38) trans-1,3-Dichloropropene-	10.58	79	86625	23.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.48%
39) 2-Hexanone-d5	10.93	63	61973	45.85	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.70%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	145333	22.98	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.92%
61) 1,2-Dichlorobenzene-d4	13.86	152	249957	26.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.96%

Target Compounds

					Ovalue	
5) Vinyl chloride	2.37	62	2422	0.261	ug/L #	1
12) 1,1-Dichloroethene	4.06	96	116798	13.250	ug/L #	76
13) Acetone	4.13	43	13218	9.188	ug/L	99
14) Carbon disulfide	4.39	76	8859m	0.333	ug/L	99
16) Methylene chloride	4.93	84	66874	6.230	ug/L	90
18) trans-1,2-Dichloroethene	5.43	96	5722	0.627	ug/L	92
19) 1,1-Dichloroethane	6.23	63	77891	5.396	ug/L	98
22) cis-1,2-Dichloroethene	7.18	96	1565717	165.305	ug/L	98
30) Cyclohexane	7.96	56	99273	7.429	ug/L	99
31) 1,1,1-Trichloroethane	7.88	97	2097764	146.888	ug/L	100
34) Benzene	8.33	78	10886	0.332	ug/L	100
35) Trichloroethene	9.10	95	179529	18.933	ug/L	99
44) Toluene	10.39	91	11177337	303.285	ug/L	89
52) Chlorobenzene	11.66	112	10440	0.422	ug/L	92
53) Ethylbenzene	11.73	91	364681	8.716	ug/L	97
54) m,p-Xylene	11.84	106	558760	34.104	ug/L	100
55) o-Xylene	12.17	106	282442	17.994	ug/L	93

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
Data File : VW016614.D
Acq On : 22 Sep 2020 16:41
Operator : SY/VA
Sample : L4109-04
Misc : 6.04G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3W8

Manual Integrations
APPROVED

MMDadoda
9/28/2020 3:16:18 PM

Quant Time: Sep 23 08:44:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 23 07:21:48 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
57) Isopropylbenzene	12.47	105	127230	2.966 ug/L	99
65) 1,2-Dichlorobenzene	13.88	146	7830	0.452 ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092320\
Data File : VW016614.D
Acq On : 22 Sep 2020 16:41
Operator : SY/VA
Sample : L4109-04
Misc : 6.04G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3W8

Manual Integrations
APPROVED

MMDadoda
9/28/2020 3:16:18 PM

Quant Time: Sep 23 08:44:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 23 07:21:48 2020
Response via : Initial Calibration

