

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020172.D
 Acq On : 24 Sep 2021 02:59
 Operator : SY/VA
 Sample : M3874-06
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7T0

Quant Time: Sep 24 04:13:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:54:02 AM

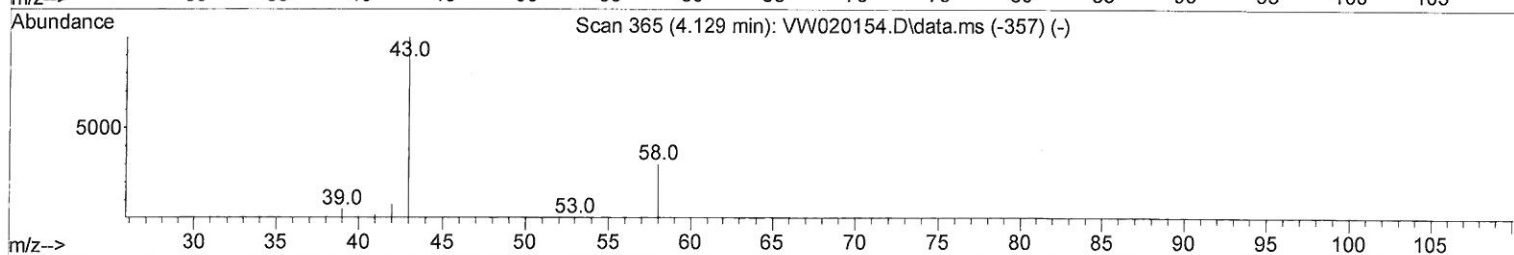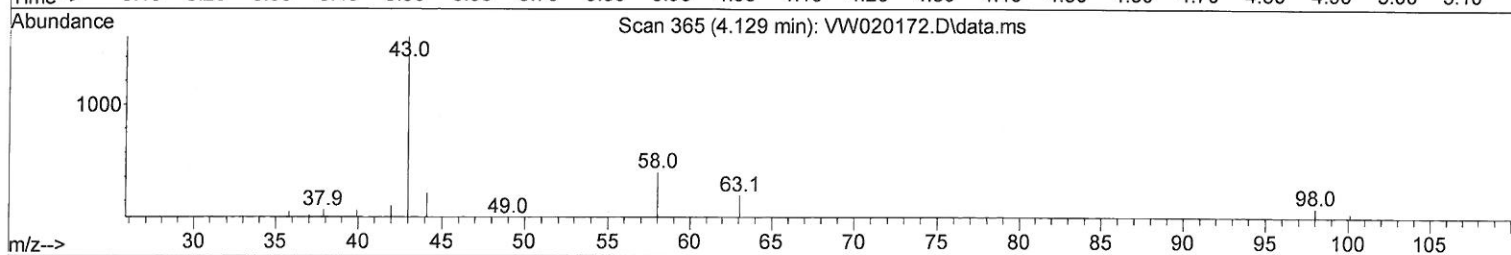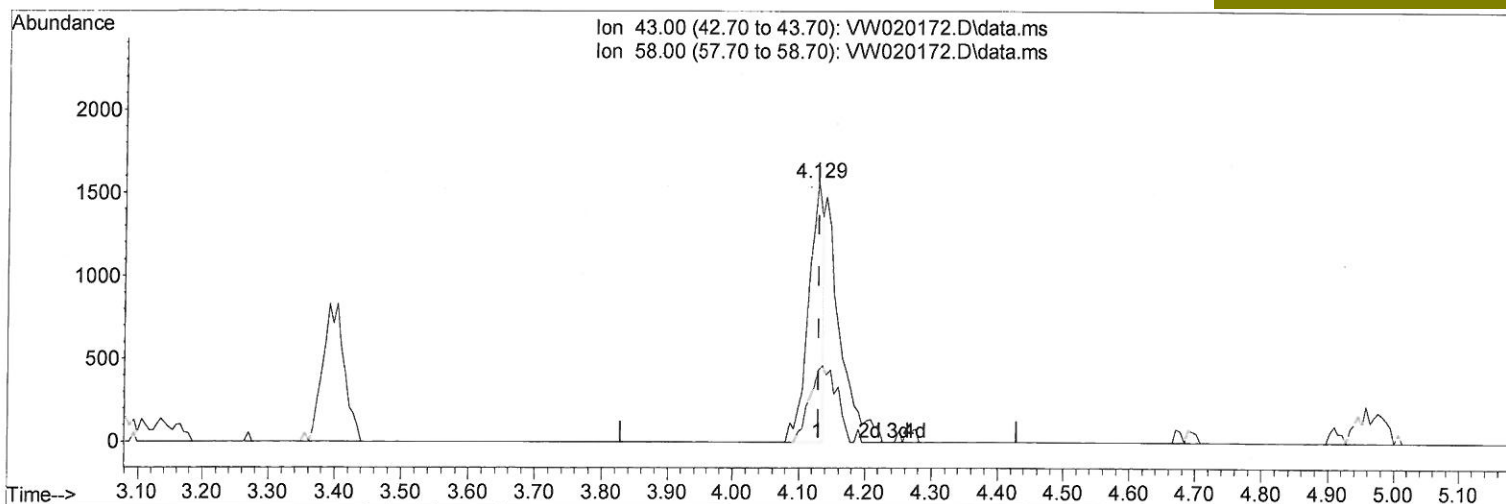

TIC: VW020172.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 2.74 ug/L

response 2434

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.80	53.45
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020172.D
 Acq On : 24 Sep 2021 02:59
 Operator : SY/VA
 Sample : M3874-06
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7T0

Quant Time: Sep 24 04:13:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:54:02 AM

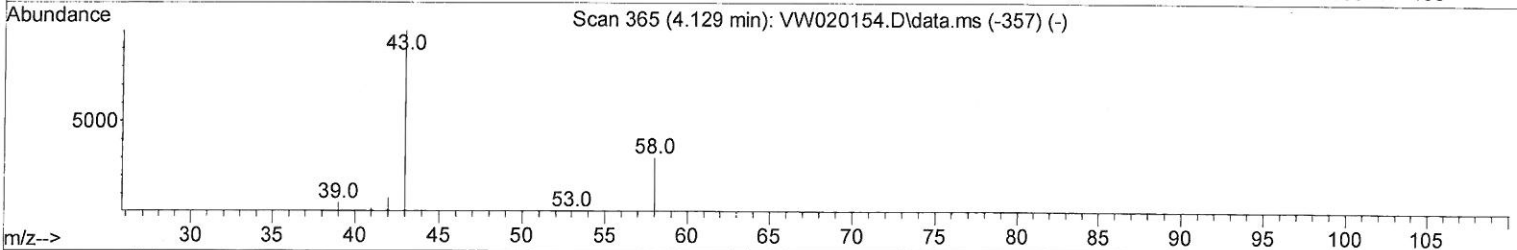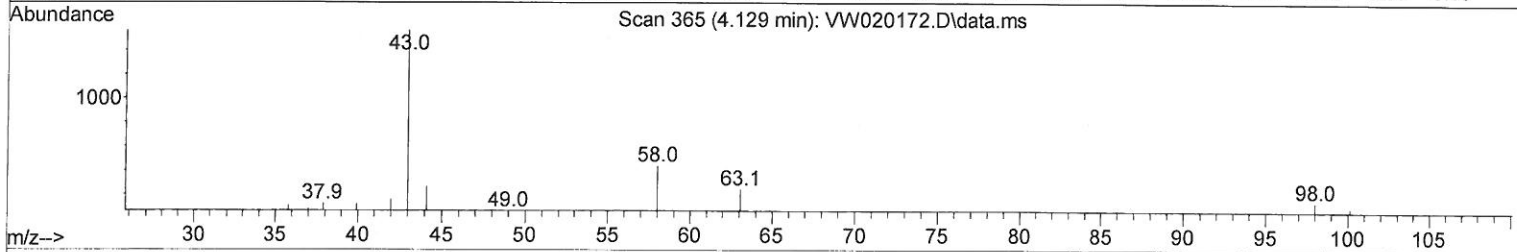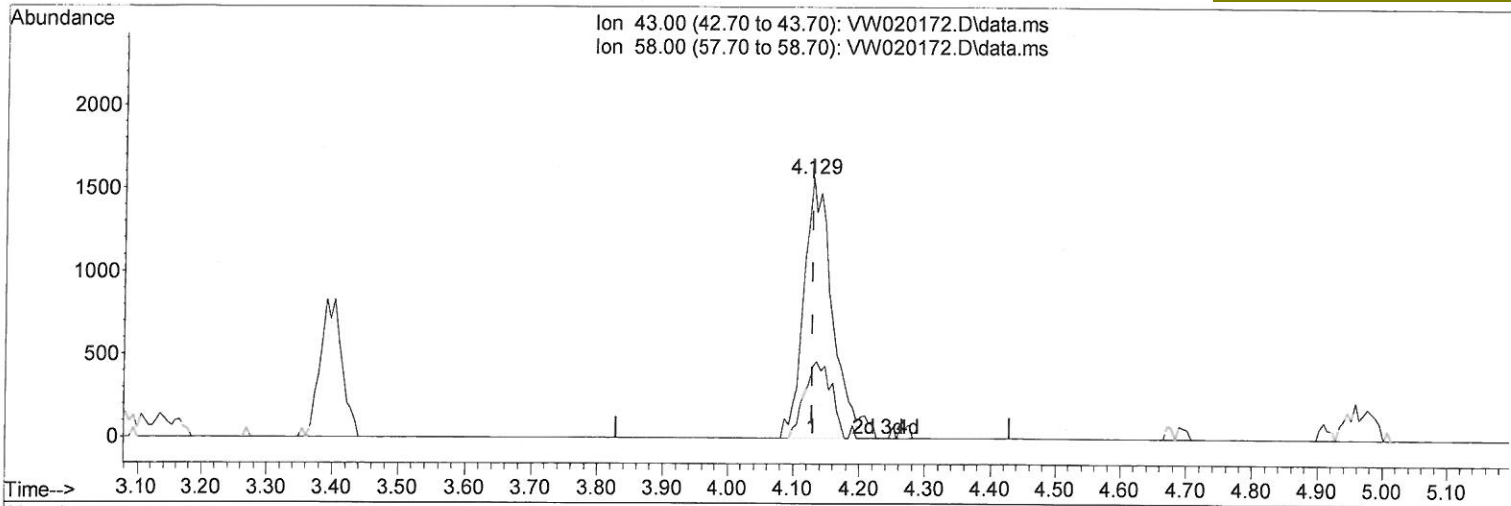

TIC: VW020172.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 5.24 ug/L m

response 4664

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.80	27.89
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020172.D
 Acq On : 24 Sep 2021 02:59
 Operator : SY/VA
 Sample : M3874-06
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW7T0

Quant Time: Sep 24 04:13:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:54:02 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	329108	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	237361	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	45805	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	137566	20.432	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	81.720%	
7) Chloroethane-d5	2.897	69	108628	21.417	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	85.680%	
11) 1,1-Dichloroethene-d2	4.025	63	163221	15.483	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	61.920%	
21) 2-Butanone-d5	7.080	46	38570	37.124	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	74.240%	
24) Chloroform-d	7.653	84	236476	22.847	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	91.400%	
26) 1,2-Dichloroethane-d4	8.311	65	122201	21.937	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	87.760%	
32) Benzene-d6	8.281	84	428646	28.306	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	113.240%	
36) 1,2-Dichloropropane-d6	9.274	67	125356	28.603	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	114.400%	
41) Toluene-d8	10.329	98	330222	23.966	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	95.880%	
43) trans-1,3-Dichloroprop...	10.579	79	41675	22.248	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	89.000%	
47) 2-Hexanone-d5	10.926	63	25574	42.167	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	84.340%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	63282	18.719	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	74.880%	
66) 1,2-Dichlorobenzene-d4	13.853	152	36899	21.484	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	85.920%	
Target Compounds						
13) Acetone	4.129	43	4664m	5.241	ug/L	Qvalue 93
16) Methylene chloride	4.921	84	17470	3.008	ug/L	93
17) trans-1,2-Dichloroethene	5.434	96	8485	1.845	ug/L	99
20) cis-1,2-Dichloroethene	7.171	96	16117	3.447	ug/L	98
34) Trichloroethene	9.091	95	3040	0.793	ug/L	96
42) Toluene	10.390	91	6813	0.448	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020172.D
 Acq On : 24 Sep 2021 02:59
 Operator : SY/VA
 Sample : M3874-06
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7T0

Quant Time: Sep 24 04:13:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:54:02 AM

