

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020156.D
 Acq On : 23 Sep 2021 20:37
 Operator : SY/VA
 Sample : M3877-01
 Misc : 6.32g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2L6

Quant Time: Sep 24 02:50:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	441759	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	401514	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	157628	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	139201	15.403	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.600%
7) Chloroethane-d5	2.897	69	111715	16.409	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.640%
11) 1,1-Dichloroethene-d2	4.019	63	179735	12.702	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.800%
21) 2-Butanone-d5	7.080	46	31634	22.683	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	45.360%
24) Chloroform-d	7.653	84	261148	18.797	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.200%
26) 1,2-Dichloroethane-d4	8.311	65	137533	18.393	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.560%
32) Benzene-d6	8.275	84	487759	19.041	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.160%
36) 1,2-Dichloropropane-d6	9.274	67	147974	19.960	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.840%
41) Toluene-d8	10.323	98	429554	18.430	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.720%
43) trans-1,3-Dichloroprop...	10.579	79	51448	16.237	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.960%
47) 2-Hexanone-d5	10.927	63	22016	21.460	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	42.920%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	94143	16.463	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	65.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	123862	20.956	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.840%
Target Compounds						Qvalue
16) Methylene chloride	4.921	84	14044	1.802	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
Data File : VW020156.D
Acq On : 23 Sep 2021 20:37
Operator : SY/VA
Sample : M3877-01
Misc : 6.32g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2L6

Quant Time: Sep 24 02:50:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 24 02:49:39 2021
Response via : Initial Calibration

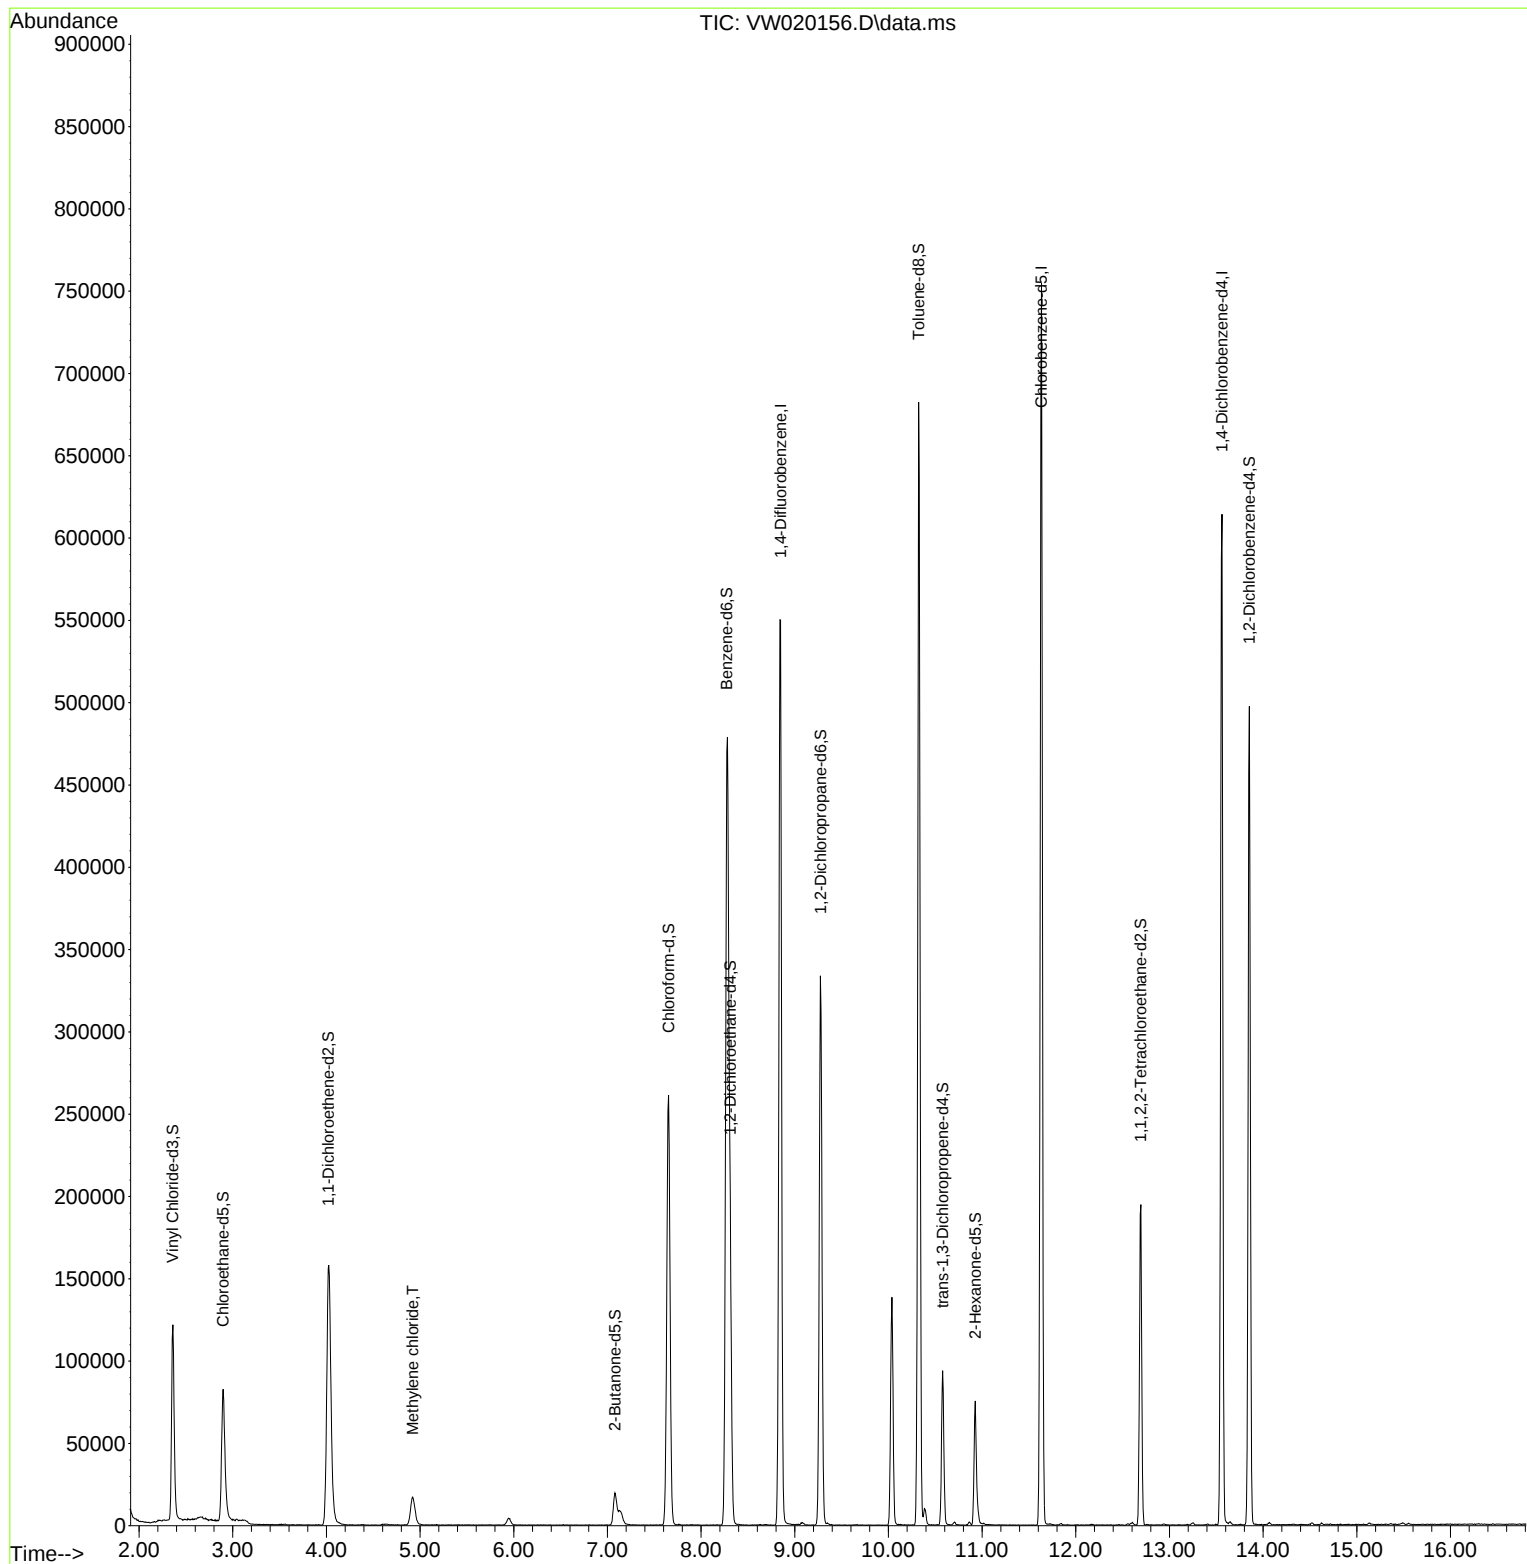

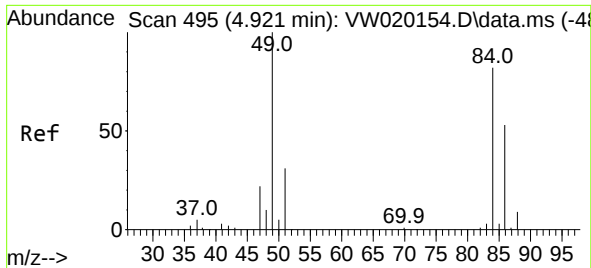

#16
Methylene chloride
Concen: 1.802 ug/L
RT: 4.921 min Scan# 495
Delta R.T. 0.000 min
Lab File: VW020156.D
Acq: 23 Sep 2021 20:37

Instrument :
MSVOA_W
ClientSampleId :
EW2L6

Tgt Ion:	84	Resp:	14044
Ion	Ratio	Lower	Upper
84	100		
86	63.6	42.6	79.0
49	128.8	83.4	154.8

