

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020161.D
 Acq On : 23 Sep 2021 22:37
 Operator : SY/VA
 Sample : M3877-06
 Misc : 5.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2M2

Quant Time: Sep 24 03:03:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	375145	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	316895	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	101627	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	127584	16.624	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.480%
7) Chloroethane-d5	2.898	69	106213	18.371	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.480%
11) 1,1-Dichloroethene-d2	4.032	63	157394	13.098	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.400%
21) 2-Butanone-d5	7.080	46	32949	27.822	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	55.640%
24) Chloroform-d	7.653	84	244447	20.719	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.880%
26) 1,2-Dichloroethane-d4	8.311	65	131027	20.635	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.520%
32) Benzene-d6	8.281	84	415174	20.536	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.160%
36) 1,2-Dichloropropane-d6	9.274	67	138160	23.613	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.440%
41) Toluene-d8	10.329	98	348836	18.963	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.840%
43) trans-1,3-Dichloroprop...	10.579	79	36329	14.527	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	58.120%
47) 2-Hexanone-d5	10.927	63	13769	17.005	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	34.000%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	87204	19.322	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	84287	22.119	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.480%
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	11135	1.682	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
Data File : VW020161.D
Acq On : 23 Sep 2021 22:37
Operator : SY/VA
Sample : M3877-06
Misc : 5.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2M2

Quant Time: Sep 24 03:03:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 24 02:49:39 2021
Response via : Initial Calibration

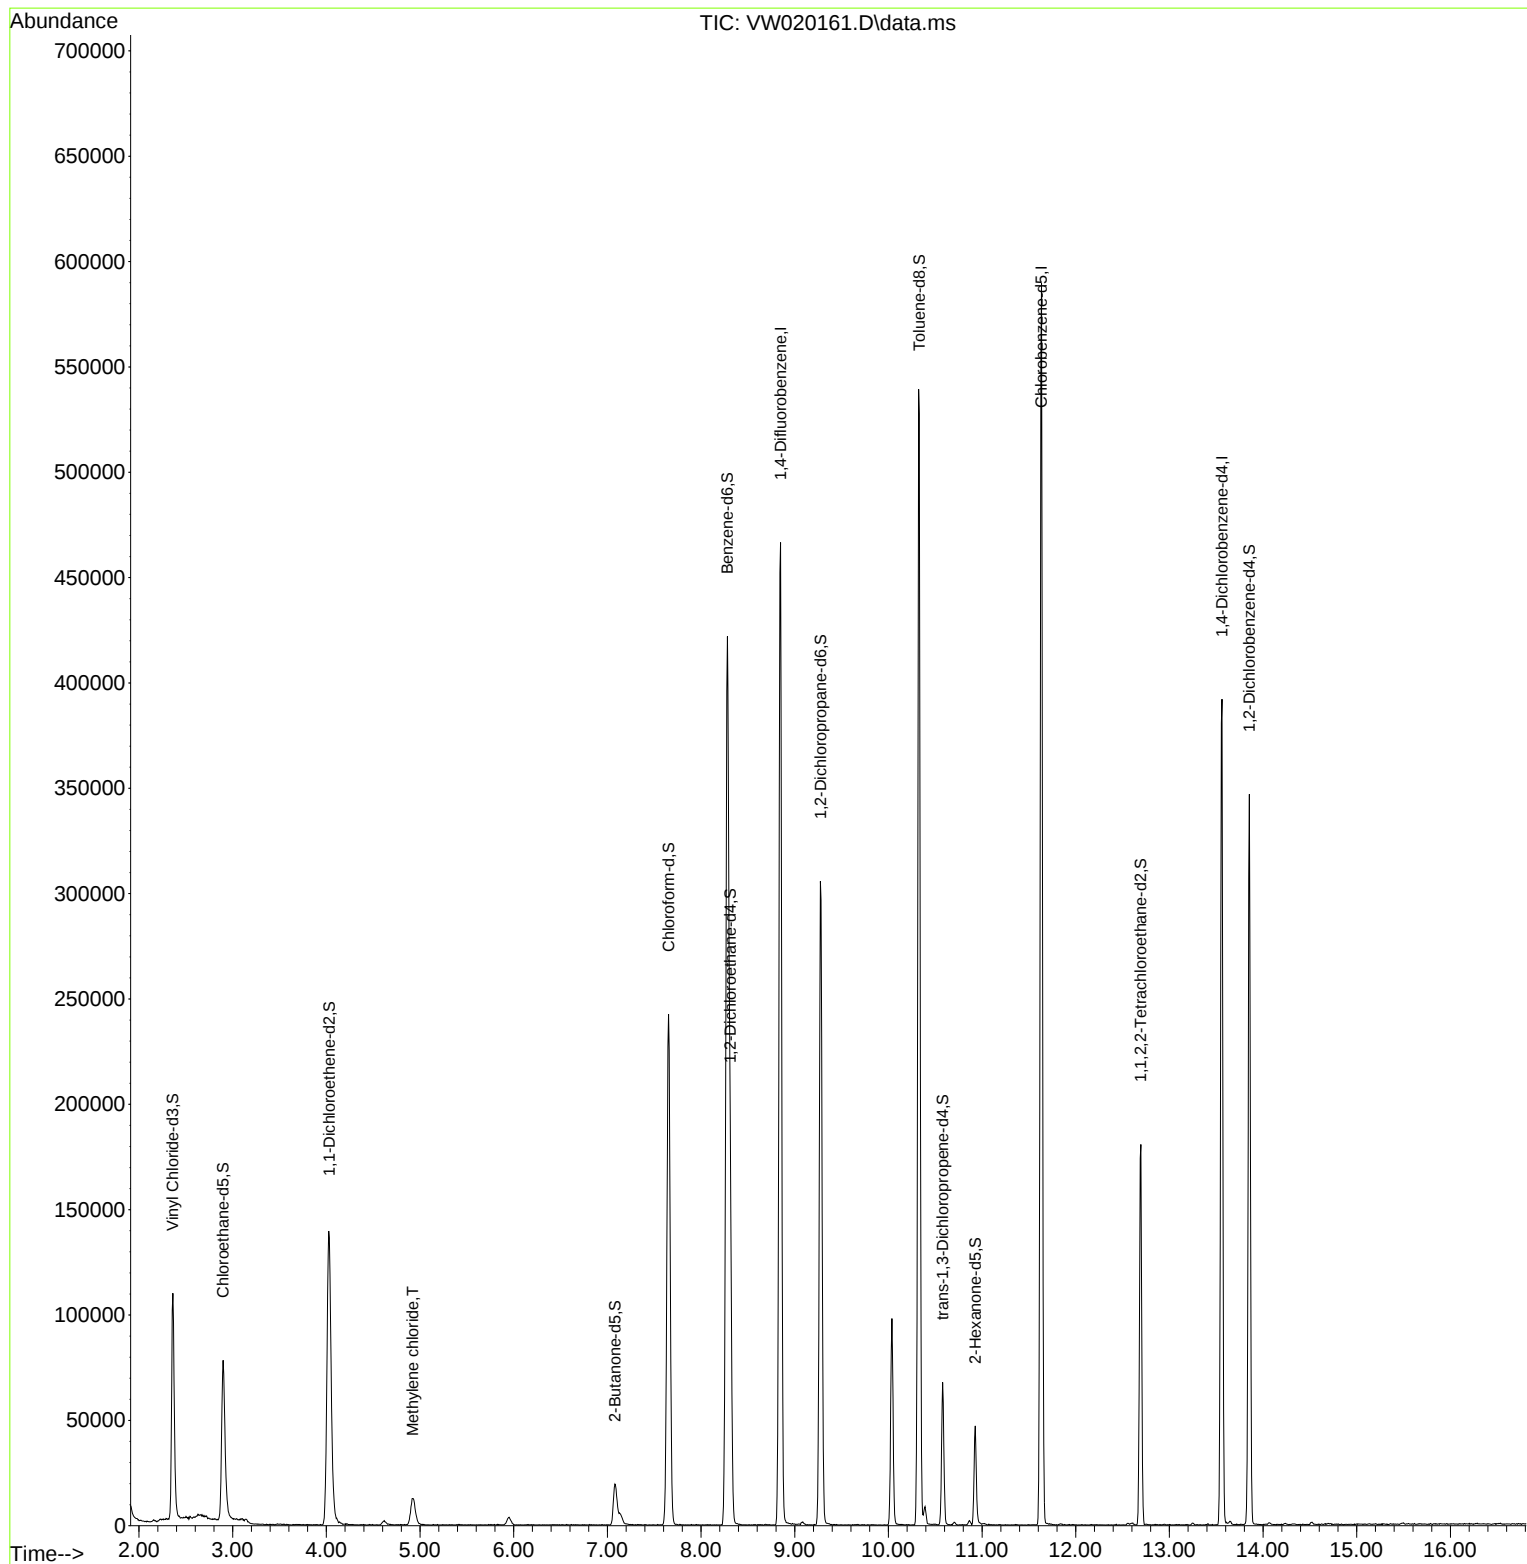

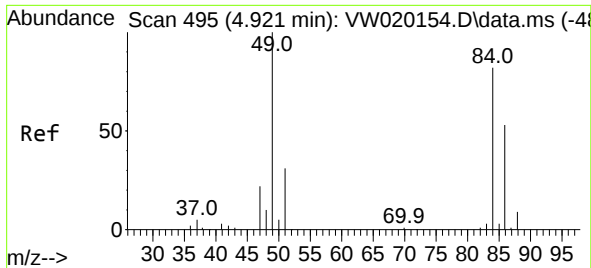

#16
Methylene chloride
Concen: 1.682 ug/L
RT: 4.922 min Scan# 495
Delta R.T. 0.000 min
Lab File: VW020161.D
Acq: 23 Sep 2021 22:37

Instrument :
MSVOA_W
ClientSampled :
EW2M2

Tgt Ion: 84 Resp: 11135
Ion Ratio Lower Upper
84 100
86 56.1 42.6 79.0
49 115.2 83.4 154.8

