

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
 Data File : VW020168.D
 Acq On : 24 Sep 2021 01:24
 Operator : SY/VA
 Sample : M3877-13
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2M9

Quant Time: Sep 24 03:04:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 24 02:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	401667	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	357978	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	128134	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	141271	17.192	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.760%
7) Chloroethane-d5	2.898	69	113097	18.270	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.080%
11) 1,1-Dichloroethene-d2	4.025	63	173181	13.460	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.840%
21) 2-Butanone-d5	7.080	46	25683	20.254	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	40.500%
24) Chloroform-d	7.653	84	262738	20.799	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.200%
26) 1,2-Dichloroethane-d4	8.311	65	133841	19.686	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.760%
32) Benzene-d6	8.281	84	476996	20.886	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.560%
36) 1,2-Dichloropropane-d6	9.275	67	145758	22.053	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.200%
41) Toluene-d8	10.323	98	413800	19.913	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.640%
43) trans-1,3-Dichloroprop...	10.579	79	44479	15.745	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.960%
47) 2-Hexanone-d5	10.927	63	17339	18.956	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	37.920%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	88387	17.336	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	69.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	107342	22.341	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.360%
Target Compounds						Qvalue
16) Methylene chloride	4.928	84	14978	2.113	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092321\
Data File : VW020168.D
Acq On : 24 Sep 2021 01:24
Operator : SY/VA
Sample : M3877-13
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2M9

Quant Time: Sep 24 03:04:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 24 02:49:39 2021
Response via : Initial Calibration

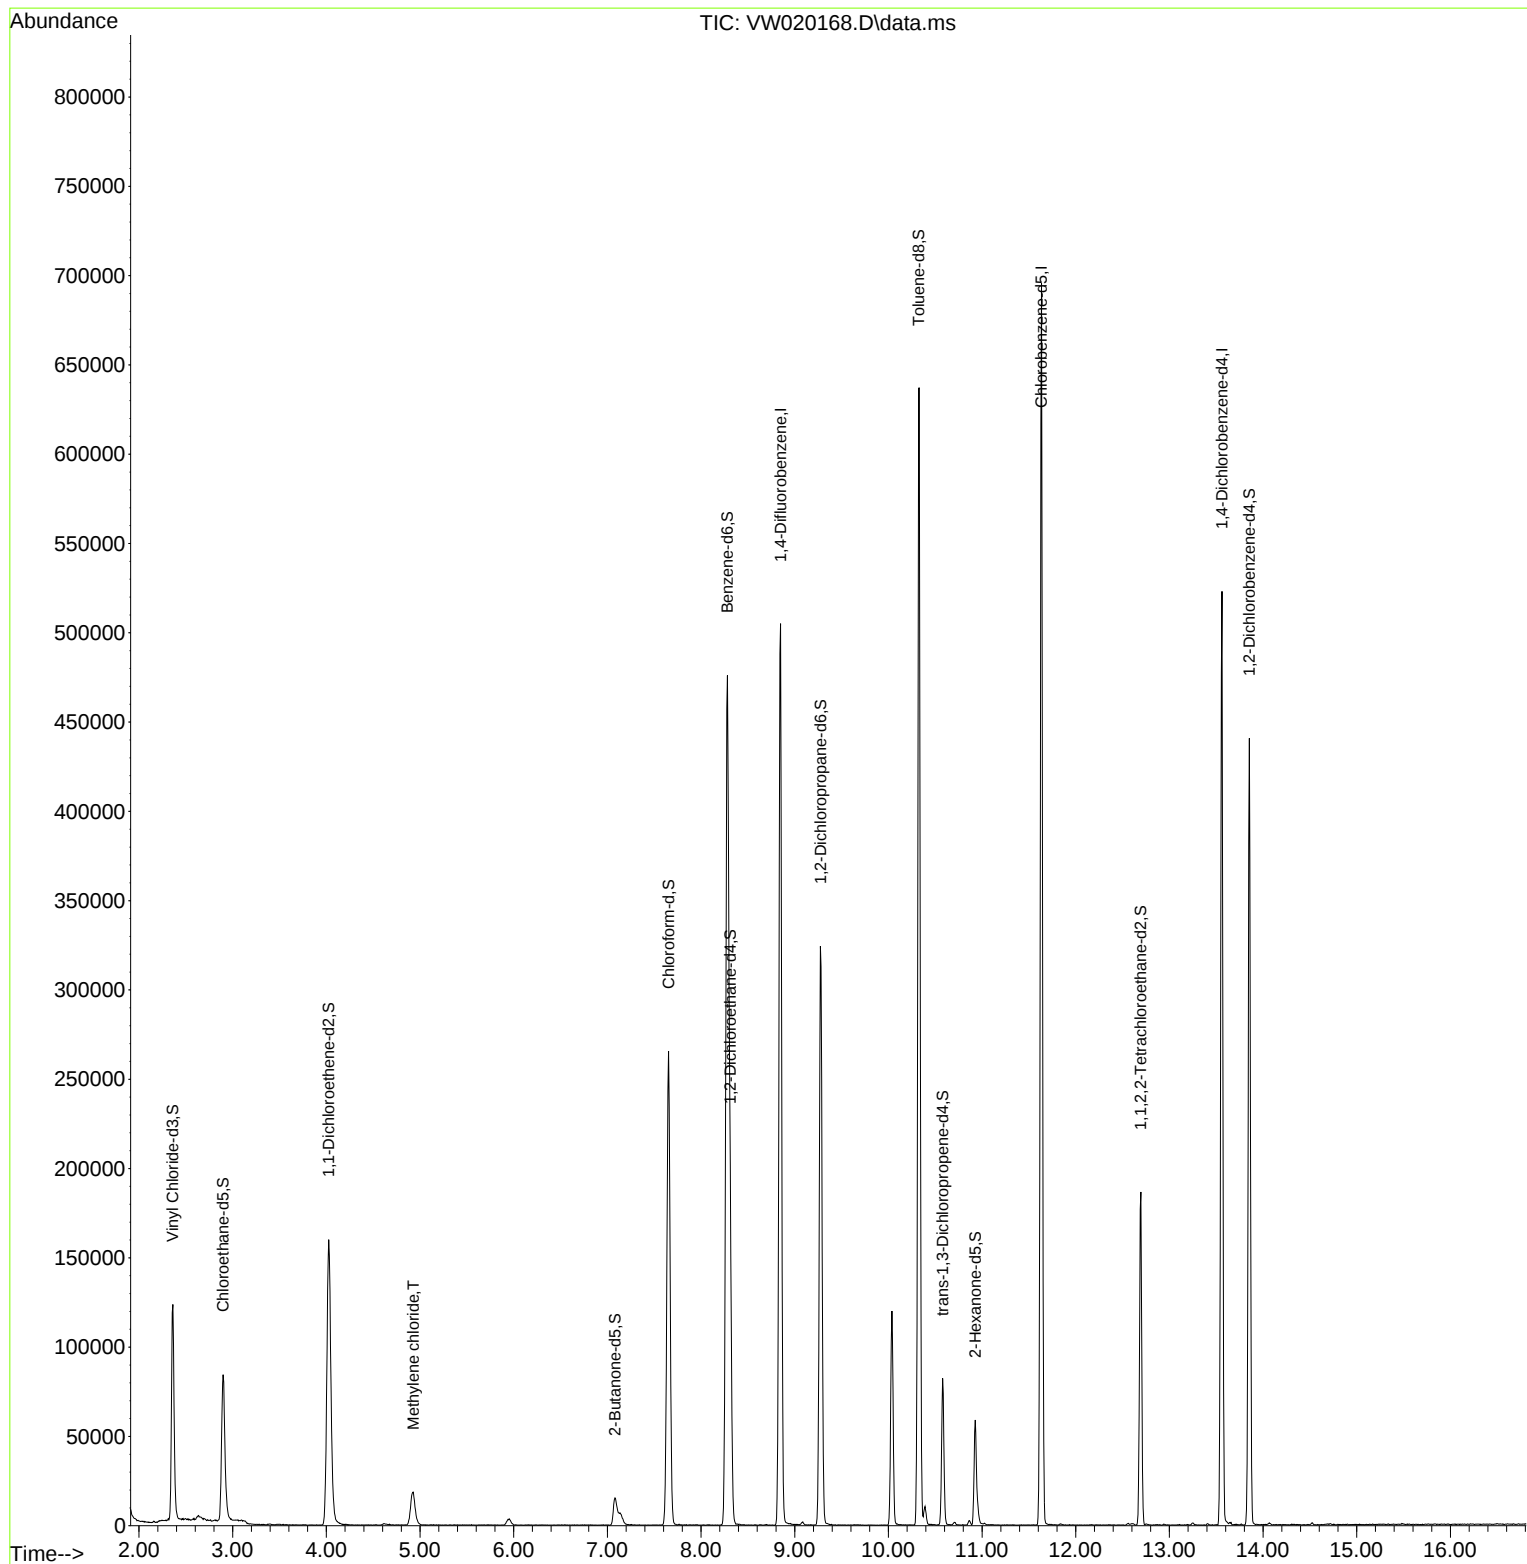

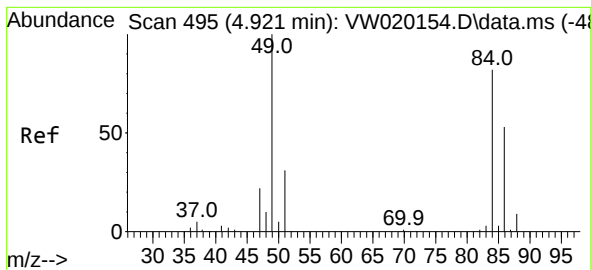

#16
Methylene chloride
Concen: 2.113 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW020168.D
Acq: 24 Sep 2021 01:24

Instrument :
MSVOA_W
ClientSampleId :
EW2M9

Tgt Ion:	84	Resp:	14978
Ion	Ratio	Lower	Upper
84	100		
86	66.4	42.6	79.0
49	123.0	83.4	154.8

