
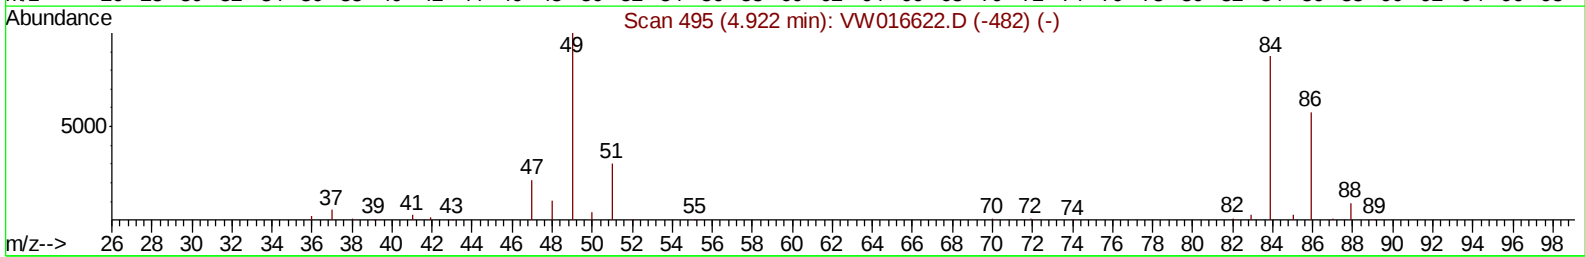
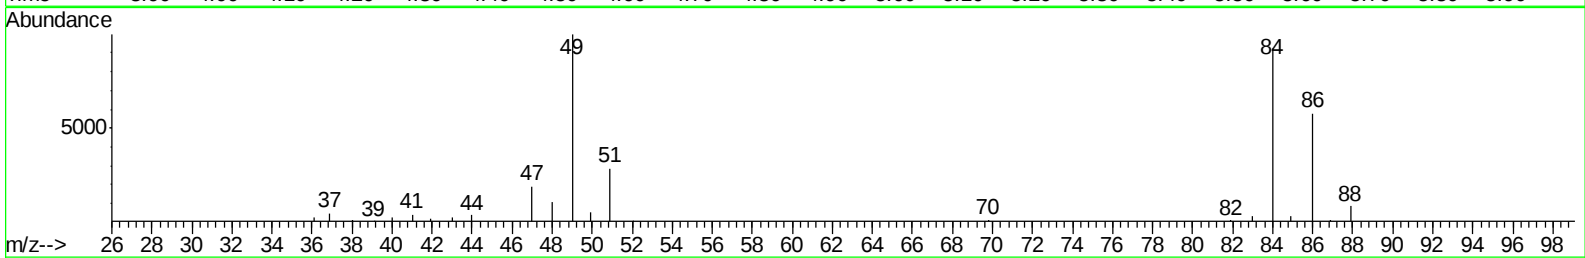


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092420\
Data File : VW016631.D
Acq On : 23 Sep 2020 15:14
Operator : SY/VA
Sample : VIBLK06
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Sep 24 04:42:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 24 04:34:20 2020
Response via : Initial Calibration

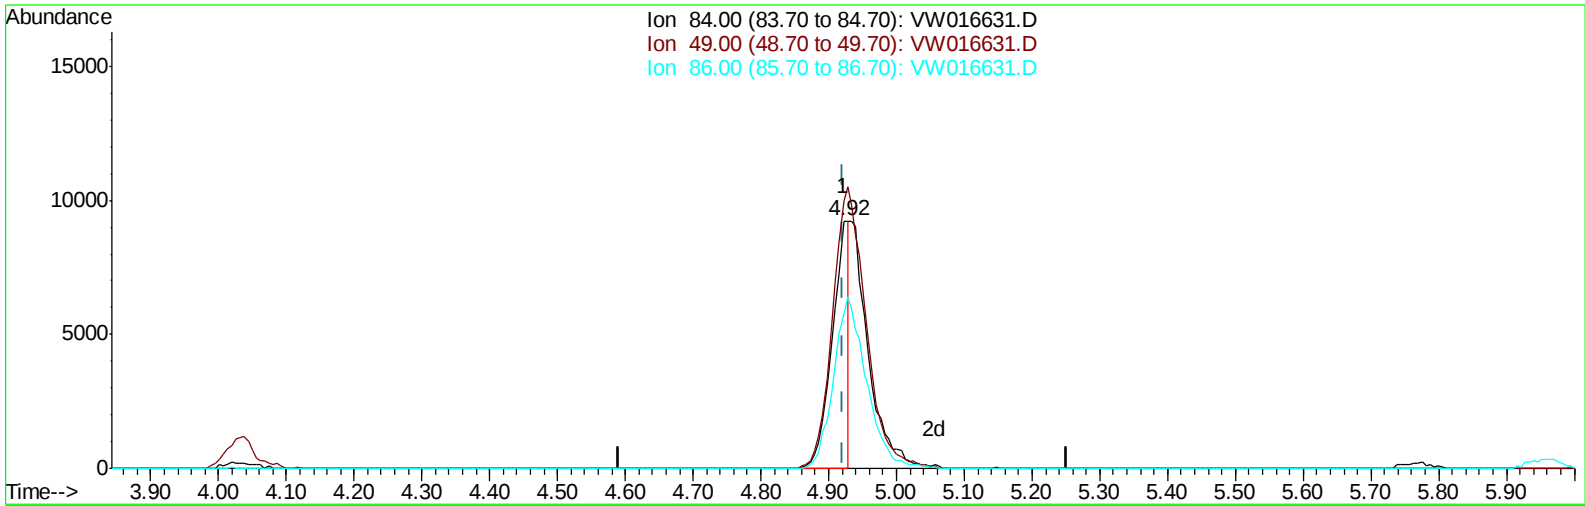

TIC: VW016631.D

(16) Methylene chloride (T)

4.922min (+0.000) 1.95ug/L

response 15676

Ion	Exp%	Act%
84.00	100	100
49.00	108.60	108.16
86.00	65.10	62.62
0.00	0.00	0.00