

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092420\
Data File : VW016625.D
Acq On : 23 Sep 2020 12:37
Operator : SY/VA
Sample : L4110-08
Misc : 5.45G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
C0AL3

Manual Integrations
APPROVED

MMDadoda
9/28/2020 3:14:10 PM

9/28/2020 3:14:10 PM

Quant Time: Sep 24 04:41:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 24 04:34:20 2020
Response via : Initial Calibration

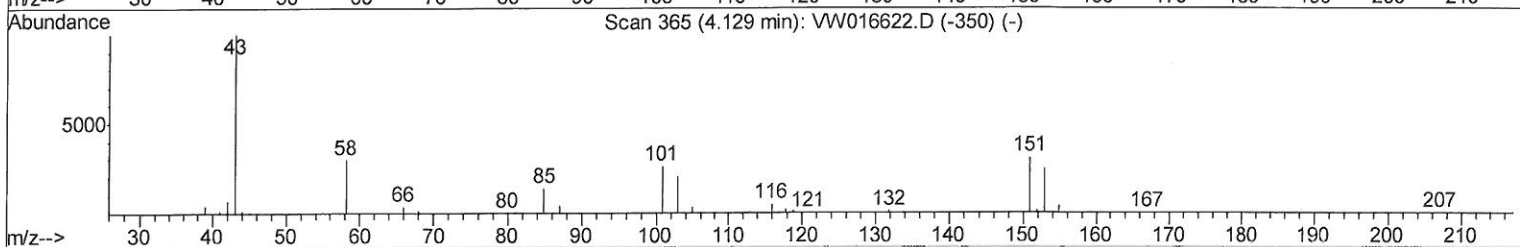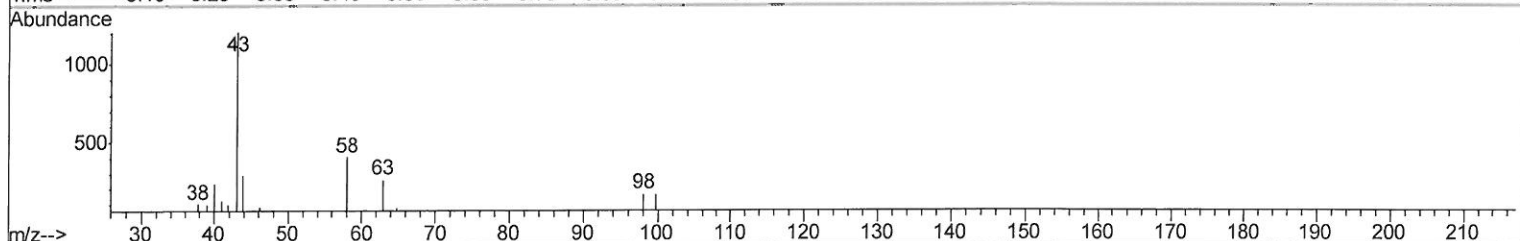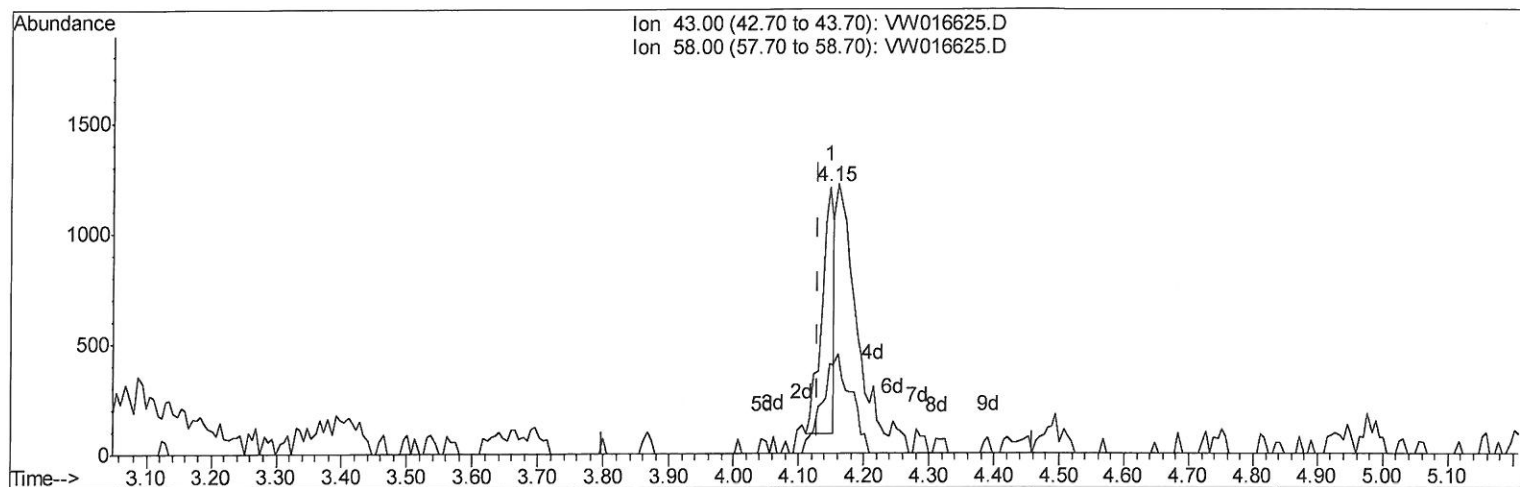

TIC: VW016625.D

(13) Acetone (T)

4.147min (+0.018) 1.05ug/L

response 1557

Ion	Exp%	Act%
43.00	100	100
58.00	30.10	72.51#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092420\
 Data File : VW016625.D
 Acq On : 23 Sep 2020 12:37
 Operator : SY/VA
 Sample : L4110-08
 Misc : 5.45G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0AL3

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:14:10 PM

9/28/2020 3:14:10 PM

Quant Time: Sep 24 04:41:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 24 04:34:20 2020
 Response via : Initial Calibration

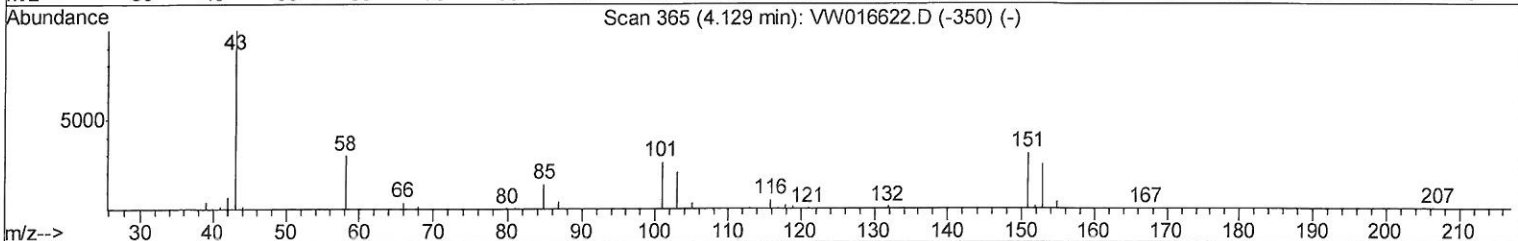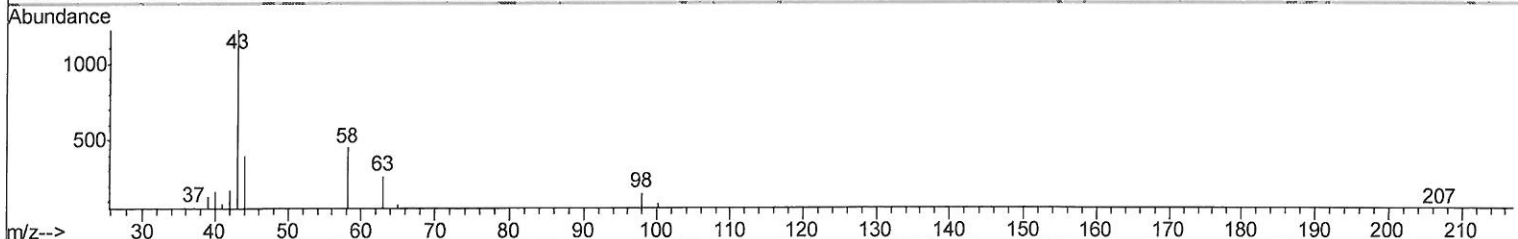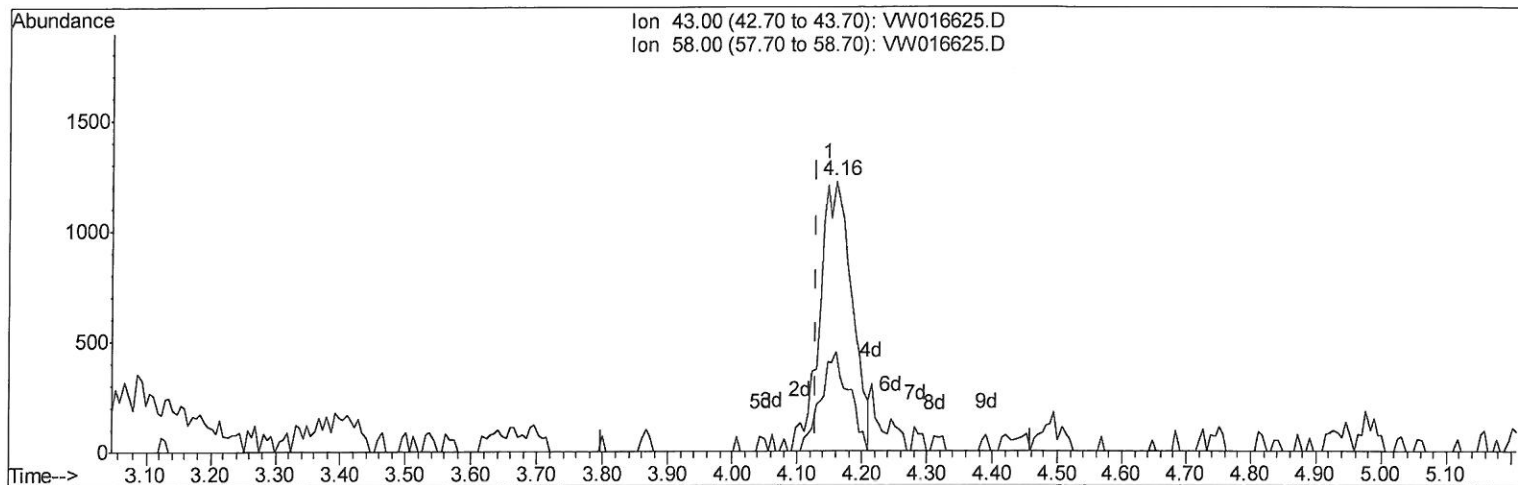

TIC: VW016625.D

(13) Acetone (T)

4.159min (+0.030) 2.87ug/L m

09/29/2020

response 4246

Ion	Exp%	Act%
43.00	100	100
58.00	30.10	26.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092420\
 Data File : VW016625.D
 Acq On : 23 Sep 2020 12:37
 Operator : SY/VA
 Sample : L4110-08
 Misc : 5.45G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AL3

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:14:10 PM

9/28/2020 3:14:10 PM

Quant Time: Sep 24 04:56:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 24 04:34:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	715089	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	611031	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	275359	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	160718	23.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.88%
7) Chloroethane-d5	2.90	69	138305	24.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.88%
10) 1,1-Dichloroethene-d2	4.03	63	256909	16.60	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.40%
20) 2-Butanone-d5	7.09	46	61386	32.53	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.06%
24) Chloroform-d	7.66	84	346127	23.14	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.56%
26) 1,2-Dichloroethane-d4	8.31	65	173871	22.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.56%
29) Benzene-d6	8.28	84	688714	25.13	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.52%
33) 1,2-Dichloropropane-d6	9.28	67	186566	25.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.48%
37) Toluene-d8	10.33	98	661256	24.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.12%
38) trans-1,3-Dichloropropene-	10.58	79	80162	21.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.64%
39) 2-Hexanone-d5	10.93	63	50685	37.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	125605	19.88	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	206360	23.45	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.80%

Target Compounds

13) Acetone	4.16	43	4246m	2.872	ug/L	Ovalue
16) Methylene chloride	4.93	84	19740	1.790	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092420\
Data File : VW016625.D
Acq On : 23 Sep 2020 12:37
Operator : SY/VA
Sample : L4110-08
Misc : 5.45G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0AL3

Manual Integrations
APPROVED

MMDadoda
9/28/2020 3:14:10 PM

9/28/2020 3:14:10 PM

Quant Time: Sep 24 04:56:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 24 04:34:20 2020
Response via : Initial Calibration

