

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092421\
 Data File : VW020191.D
 Acq On : 24 Sep 2021 14:44
 Operator : SY/VA
 Sample : M3877-10
 Misc : 5.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2M6

Quant Time: Sep 25 00:42:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 25 00:37:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	399658	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	335966	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	104440	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	136290	16.669	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.680%
7) Chloroethane-d5	2.897	69	107731	17.491	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.960%
11) 1,1-Dichloroethene-d2	4.019	63	164726	12.868	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.480%
21) 2-Butanone-d5	7.086	46	32586	25.827	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	51.660%
24) Chloroform-d	7.653	84	245760	19.553	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.200%
26) 1,2-Dichloroethane-d4	8.311	65	125477	18.549	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.200%
32) Benzene-d6	8.281	84	451801	21.079	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.320%
36) 1,2-Dichloropropane-d6	9.280	67	136325	21.977	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.920%
41) Toluene-d8	10.323	98	378481	19.407	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.640%
43) trans-1,3-Dichloroprop...	10.579	79	47694	17.989	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.960%
47) 2-Hexanone-d5	10.926	63	24277	28.280	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.560%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	79898	16.698	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	66.800%
66) 1,2-Dichlorobenzene-d4	13.853	152	77709	19.843	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.360%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	10955	1.553	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092421\
Data File : VW020191.D
Acq On : 24 Sep 2021 14:44
Operator : SY/VA
Sample : M3877-10
Misc : 5.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2M6

Quant Time: Sep 25 00:42:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 25 00:37:21 2021
Response via : Initial Calibration

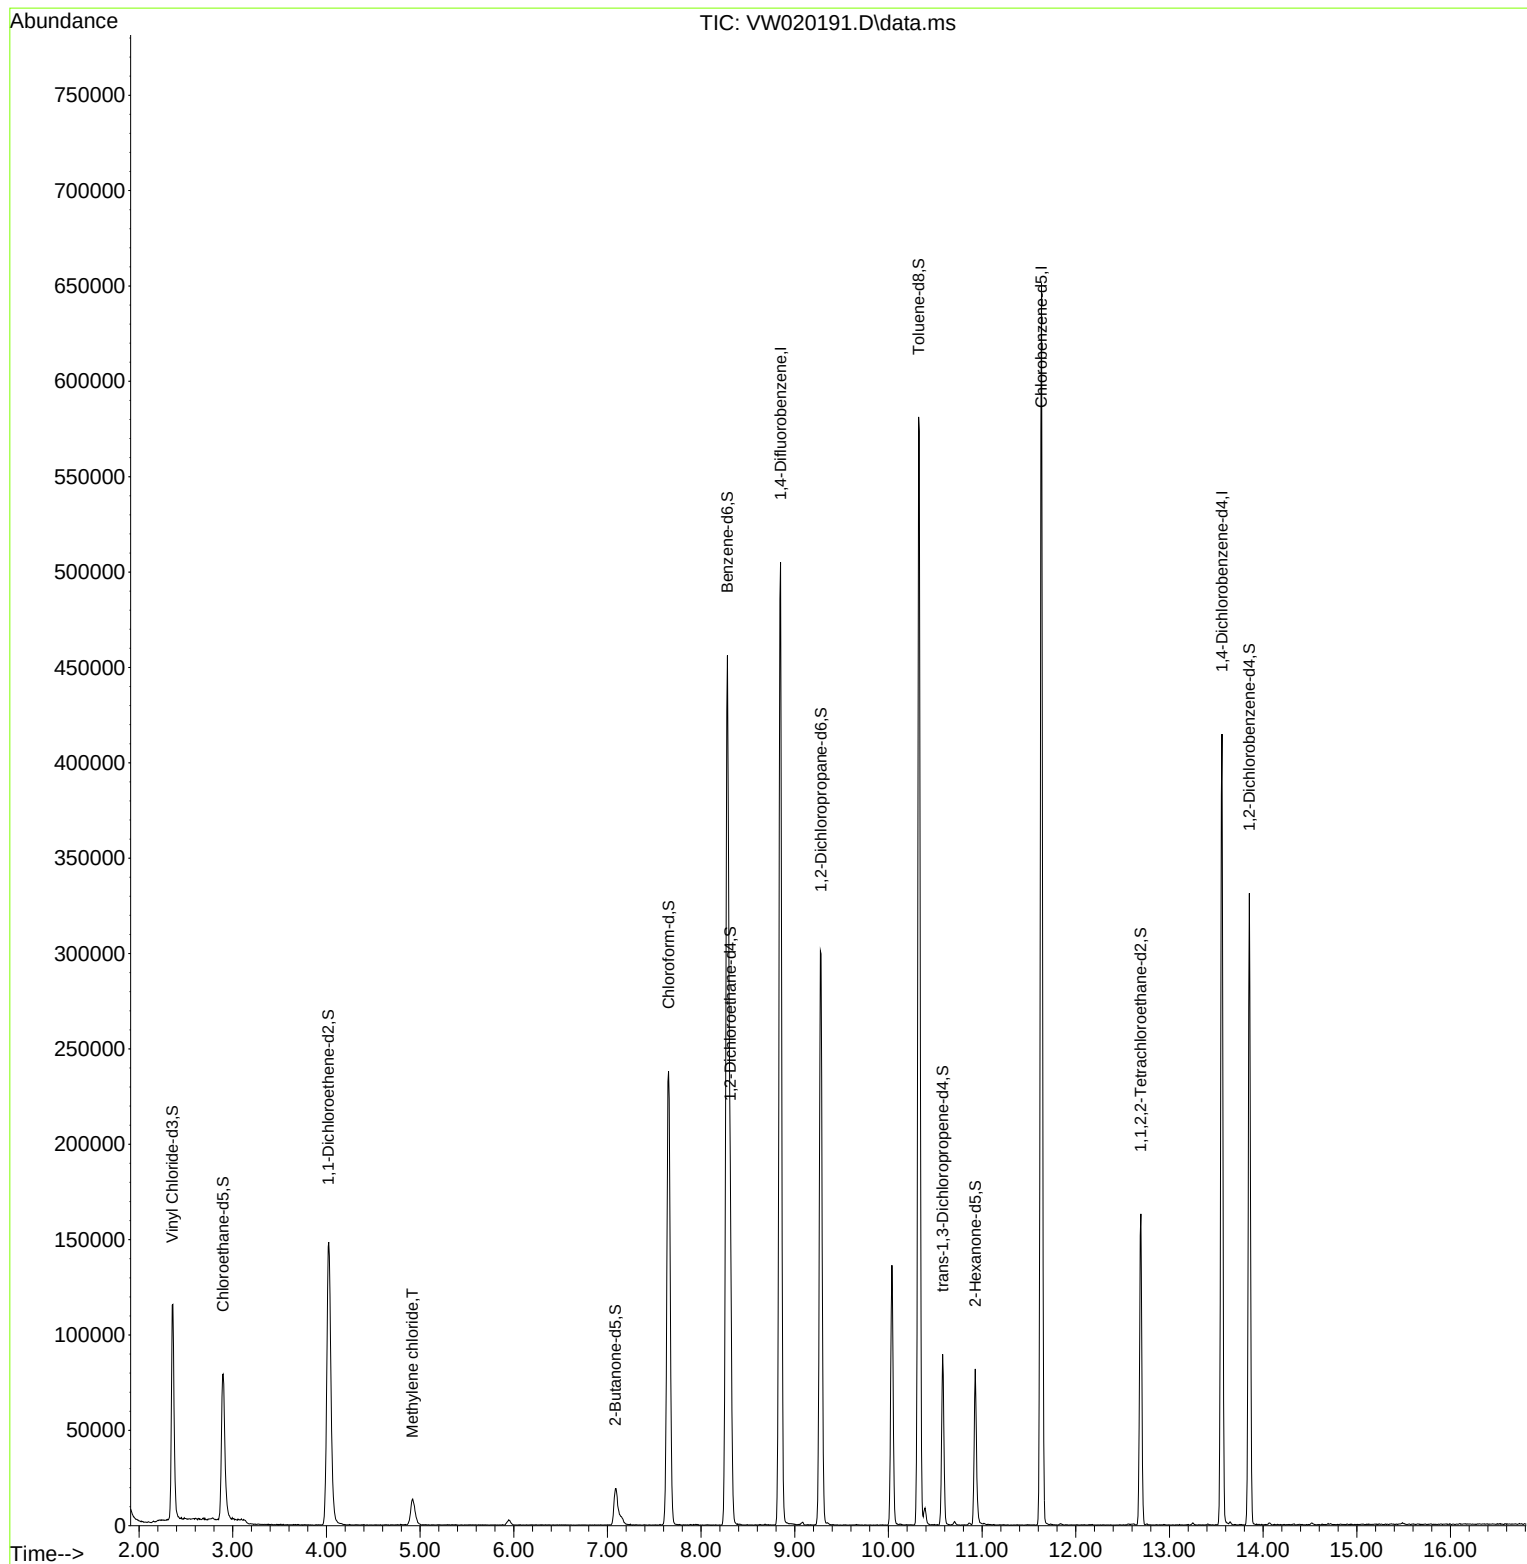

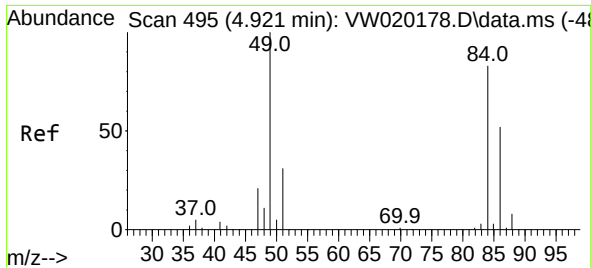

#16
Methylene chloride
Concen: 1.553 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW020191.D
Acq: 24 Sep 2021 14:44

Instrument :
MSVOA_W
ClientSampleId :
EW2M6

Tgt Ion:	84	Resp:	10955
Ion	Ratio	Lower	Upper
84	100		
86	69.0	42.6	79.0
49	116.0	83.4	154.8

