


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW092518\
Data File : VW005600.D
Acq On : 25 Sep 2018 10:01
Operator : VA/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
Title : SW846 8260
Last Update : Fri Sep 21 09:05:42 2018

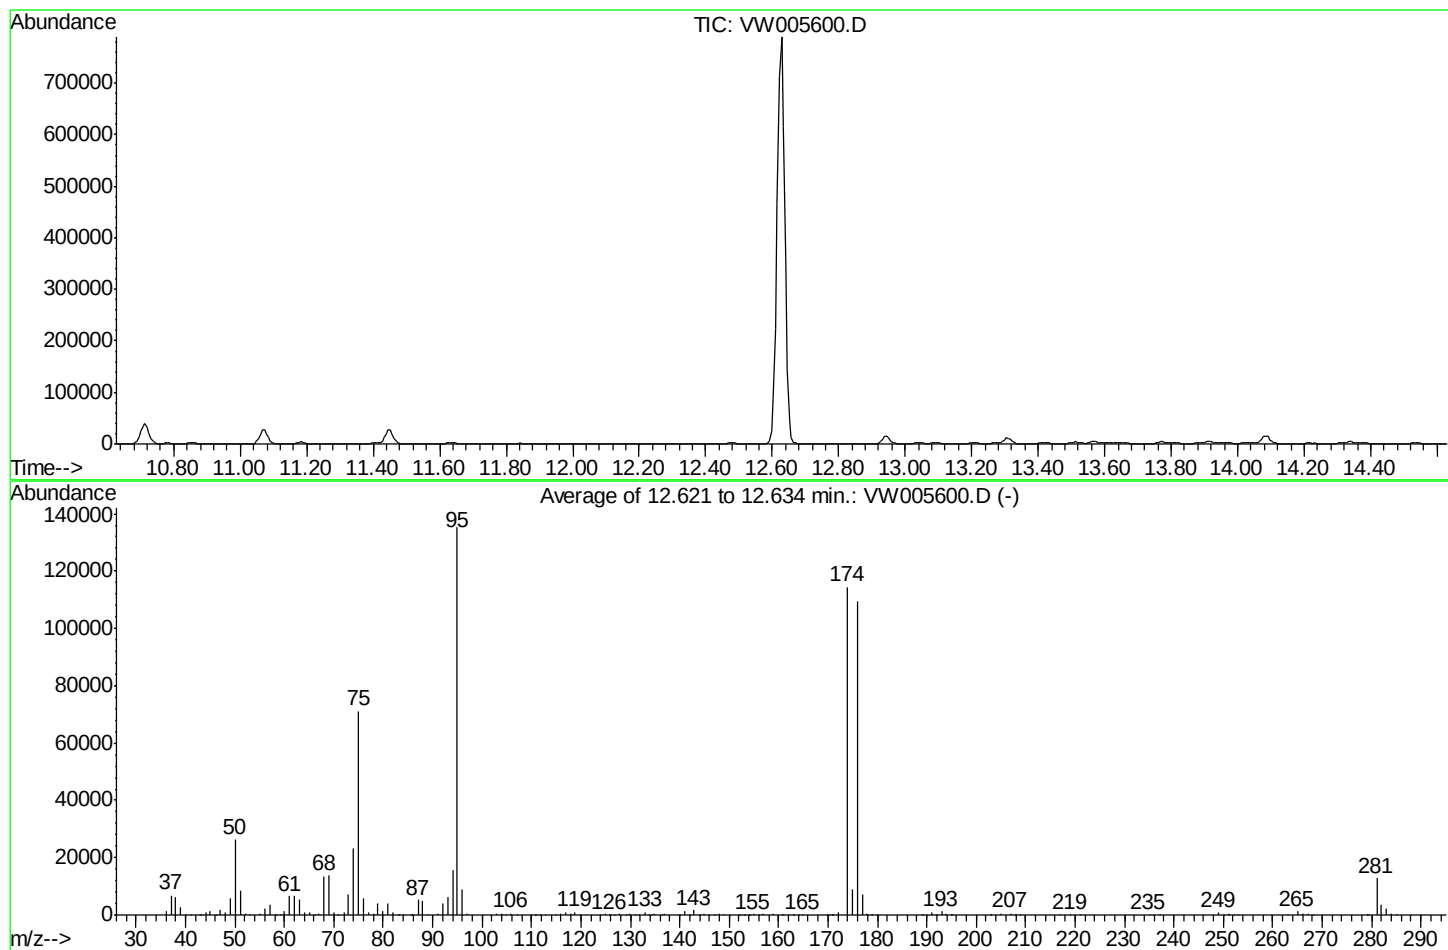

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	26157	PASS
75	95	30	60	52.5	71048	PASS
95	95	100	100	100.0	135264	PASS
96	95	5	9	6.6	8959	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.6	114378	PASS
175	174	5	9	7.8	8964	PASS
176	174	95	101	95.6	109320	PASS
177	176	5	9	6.5	7152	PASS