


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW092518\
 Data File : VW005627.D
 Acq On : 25 Sep 2018 23:03
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
 Title : SW846 8260
 Last Update : Fri Sep 21 09:05:42 2018

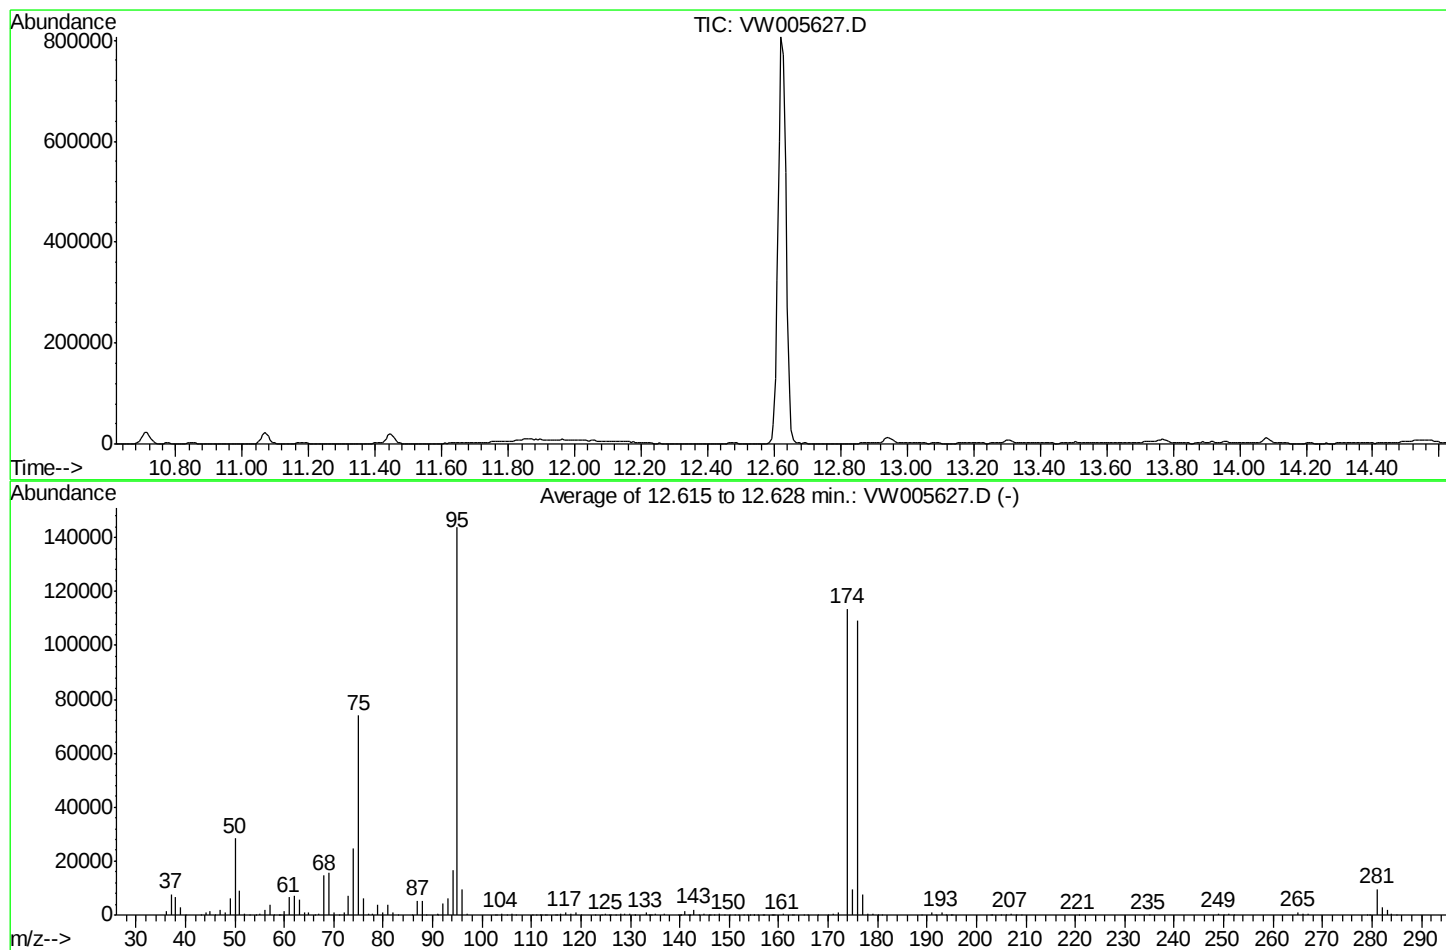

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	28402	PASS
75	95	30	60	51.4	73981	PASS
95	95	100	100	100.0	143805	PASS
96	95	5	9	6.8	9730	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.1	113730	PASS
175	174	5	9	8.3	9472	PASS
176	174	95	101	96.2	109360	PASS
177	176	5	9	7.0	7607	PASS