

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092520\
 Data File : VW016638.D
 Acq On : 24 Sep 2020 10:18
 Operator : SY/VA
 Sample : VW0924SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 VBLK20

Manual Integrations
APPROVED

MMDadoda
 9/28/2020 3:14:58 PM

Quant Time: Sep 25 08:02:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 25 07:55:30 2020
 Response via : Initial Calibration

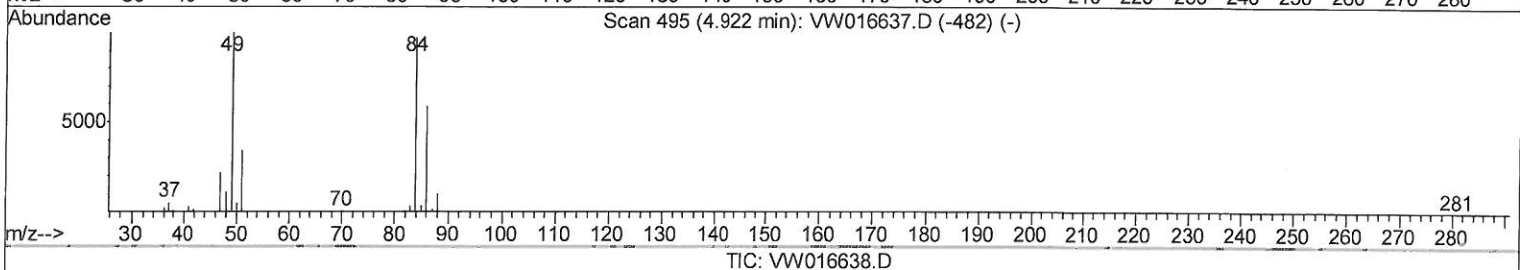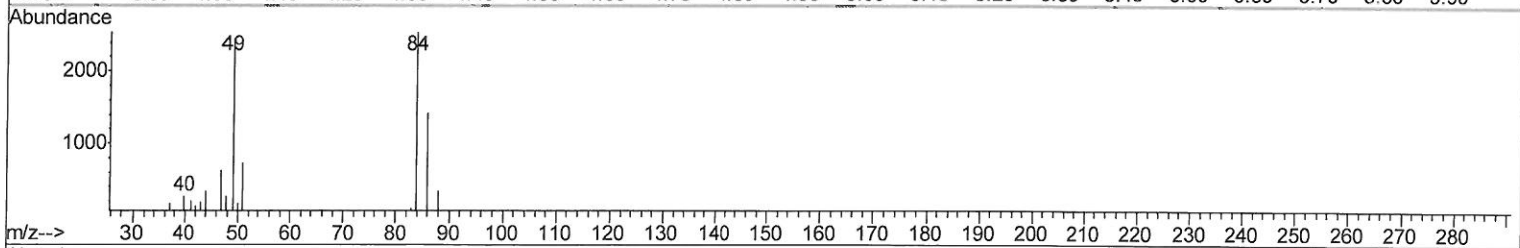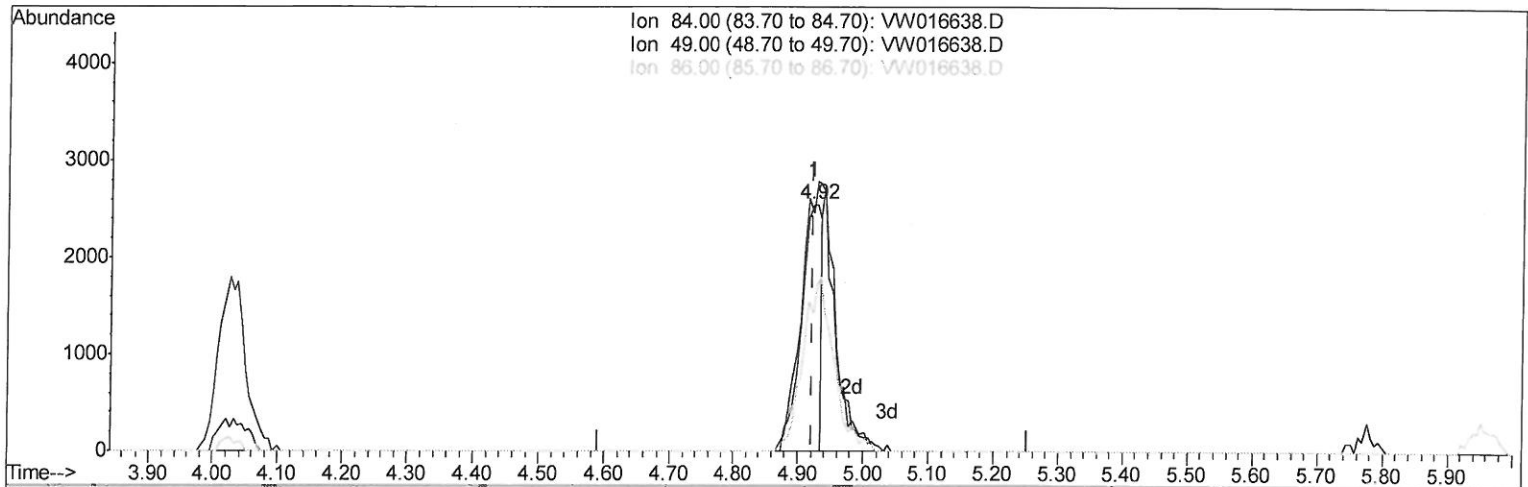

(16) Methylene chloride (T)

4.922min (-0.000) 0.58ug/L

response 5429

Ion	Exp%	Act%
84.00	100	100
49.00	108.60	96.39
86.00	65.10	55.81
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092520\
 Data File : VW016638.D
 Acq On : 24 Sep 2020 10:18
 Operator : SY/VA
 Sample : VW0924SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VBLK20

Manual Integrations
APPROVED

MMDadoda
 9/28/2020 3:14:58 PM

Quant Time: Sep 25 08:02:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 25 07:55:30 2020
 Response via : Initial Calibration

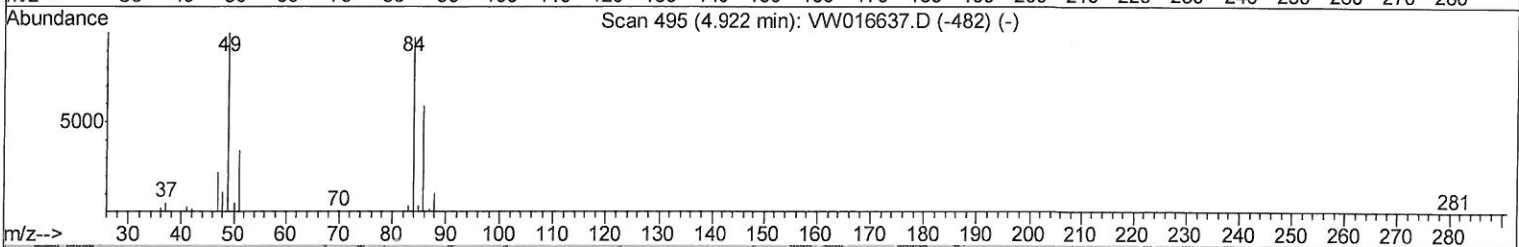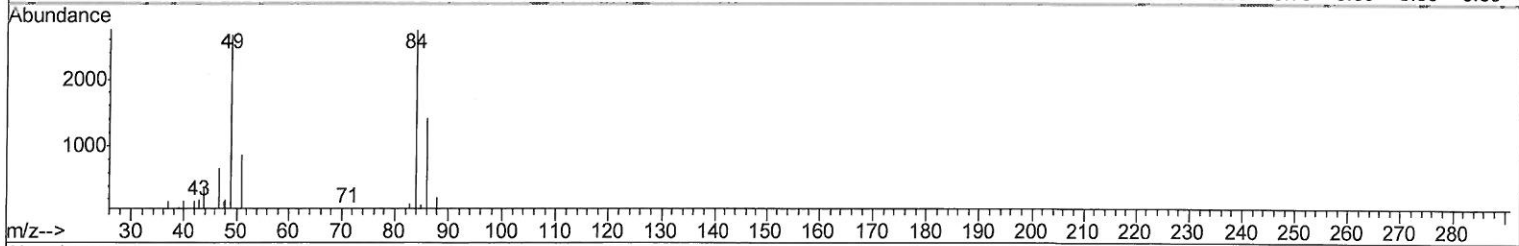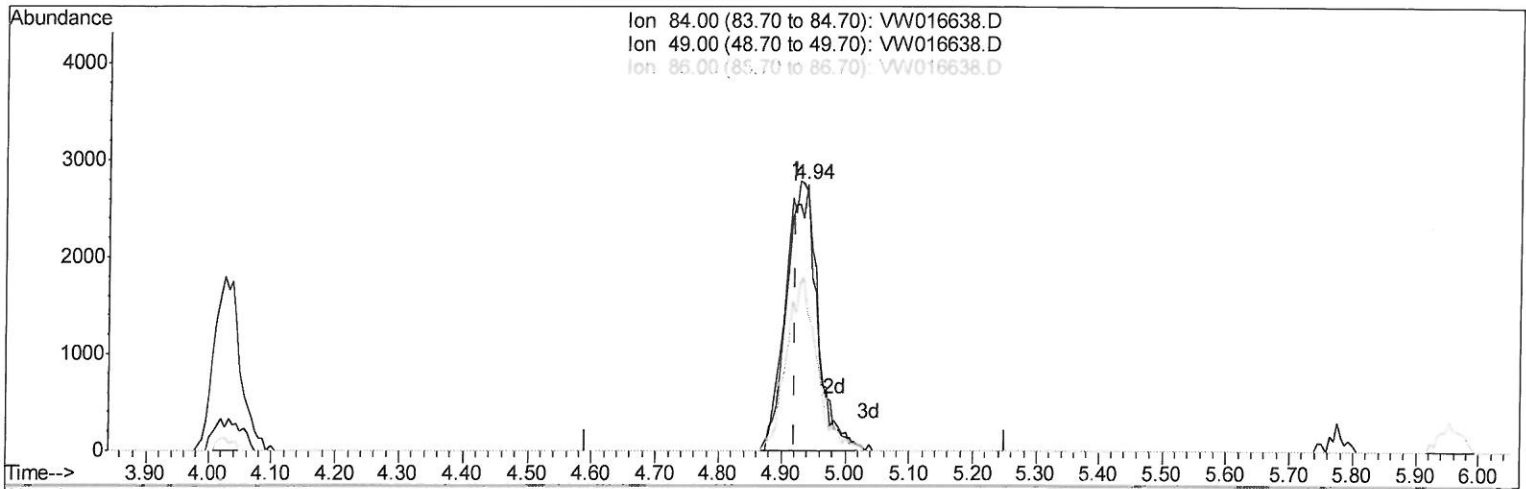

TIC: VW016638.D

(16) Methylene chloride (T)

4.940min (+0.018) 0.97ug/L m

209/28/20 SY

response 9096

Ion	Exp%	Act%
84.00	100	100
49.00	108.60	97.05
86.00	65.10	51.53
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092520\
 Data File : VW016638.D
 Acq On : 24 Sep 2020 10:18
 Operator : SY/VA
 Sample : VW0924SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK20

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 3:14:58 PM

Quant Time: Sep 25 08:08:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 25 07:55:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	607299	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	518001	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	246423	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	109946	18.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.80%
7) Chloroethane-d5	2.90	69	98696	20.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.24%
10) 1,1-Dichloroethene-d2	4.03	63	176733	13.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.80%
20) 2-Butanone-d5	7.10	46	57934	36.15	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.30%
24) Chloroform-d	7.65	84	293508	23.10	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	8.31	65	148658	22.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.16%
29) Benzene-d6	8.28	84	526049	22.64	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.56%
33) 1,2-Dichloropropane-d6	9.28	67	150943	23.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.92%
37) Toluene-d8	10.33	98	479098	20.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.84%
38) trans-1,3-Dichloropropene-	10.58	79	67006	21.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.44%
39) 2-Hexanone-d5	10.93	63	45760	39.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	119783	22.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	200922	25.52	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.08%

Target Compounds

16) Methylene chloride	4.94	84	9096m	0.971	ug/L	Ovalue
------------------------	------	----	-------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092520\
Data File : VW016638.D
Acq On : 24 Sep 2020 10:18
Operator : SY/VA
Sample : VW0924SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Manual Integrations
APPROVED

MMDadoda
9/28/2020 3:14:58 PM

Quant Time: Sep 25 08:08:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 25 07:55:30 2020
Response via : Initial Calibration

