

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092618\
 Data File : VW005681.D
 Acq On : 27 Sep 2018 05:19
 Operator : VA/AP
 Sample : VW092618SBL02
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW092618SBL02

Quant Time: Sep 27 07:57:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 21 09:05:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.96	168	211373	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	363589	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	344415	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	170899	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	142792	57.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	114.68%	
35) Dibromofluoromethane	7.89	113	122189	53.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.88%	
50) Toluene-d8	10.33	98	466287	50.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.16%	
62) 4-Bromofluorobenzene	12.63	95	169374	49.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.34%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092618\
Data File : VW005681.D
Acq On : 27 Sep 2018 05:19
Operator : VA/AP
Sample : VW092618SBL02
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW092618SBL02

Quant Time: Sep 27 07:57:38 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 21 09:05:42 2018
Response via : Initial Calibration

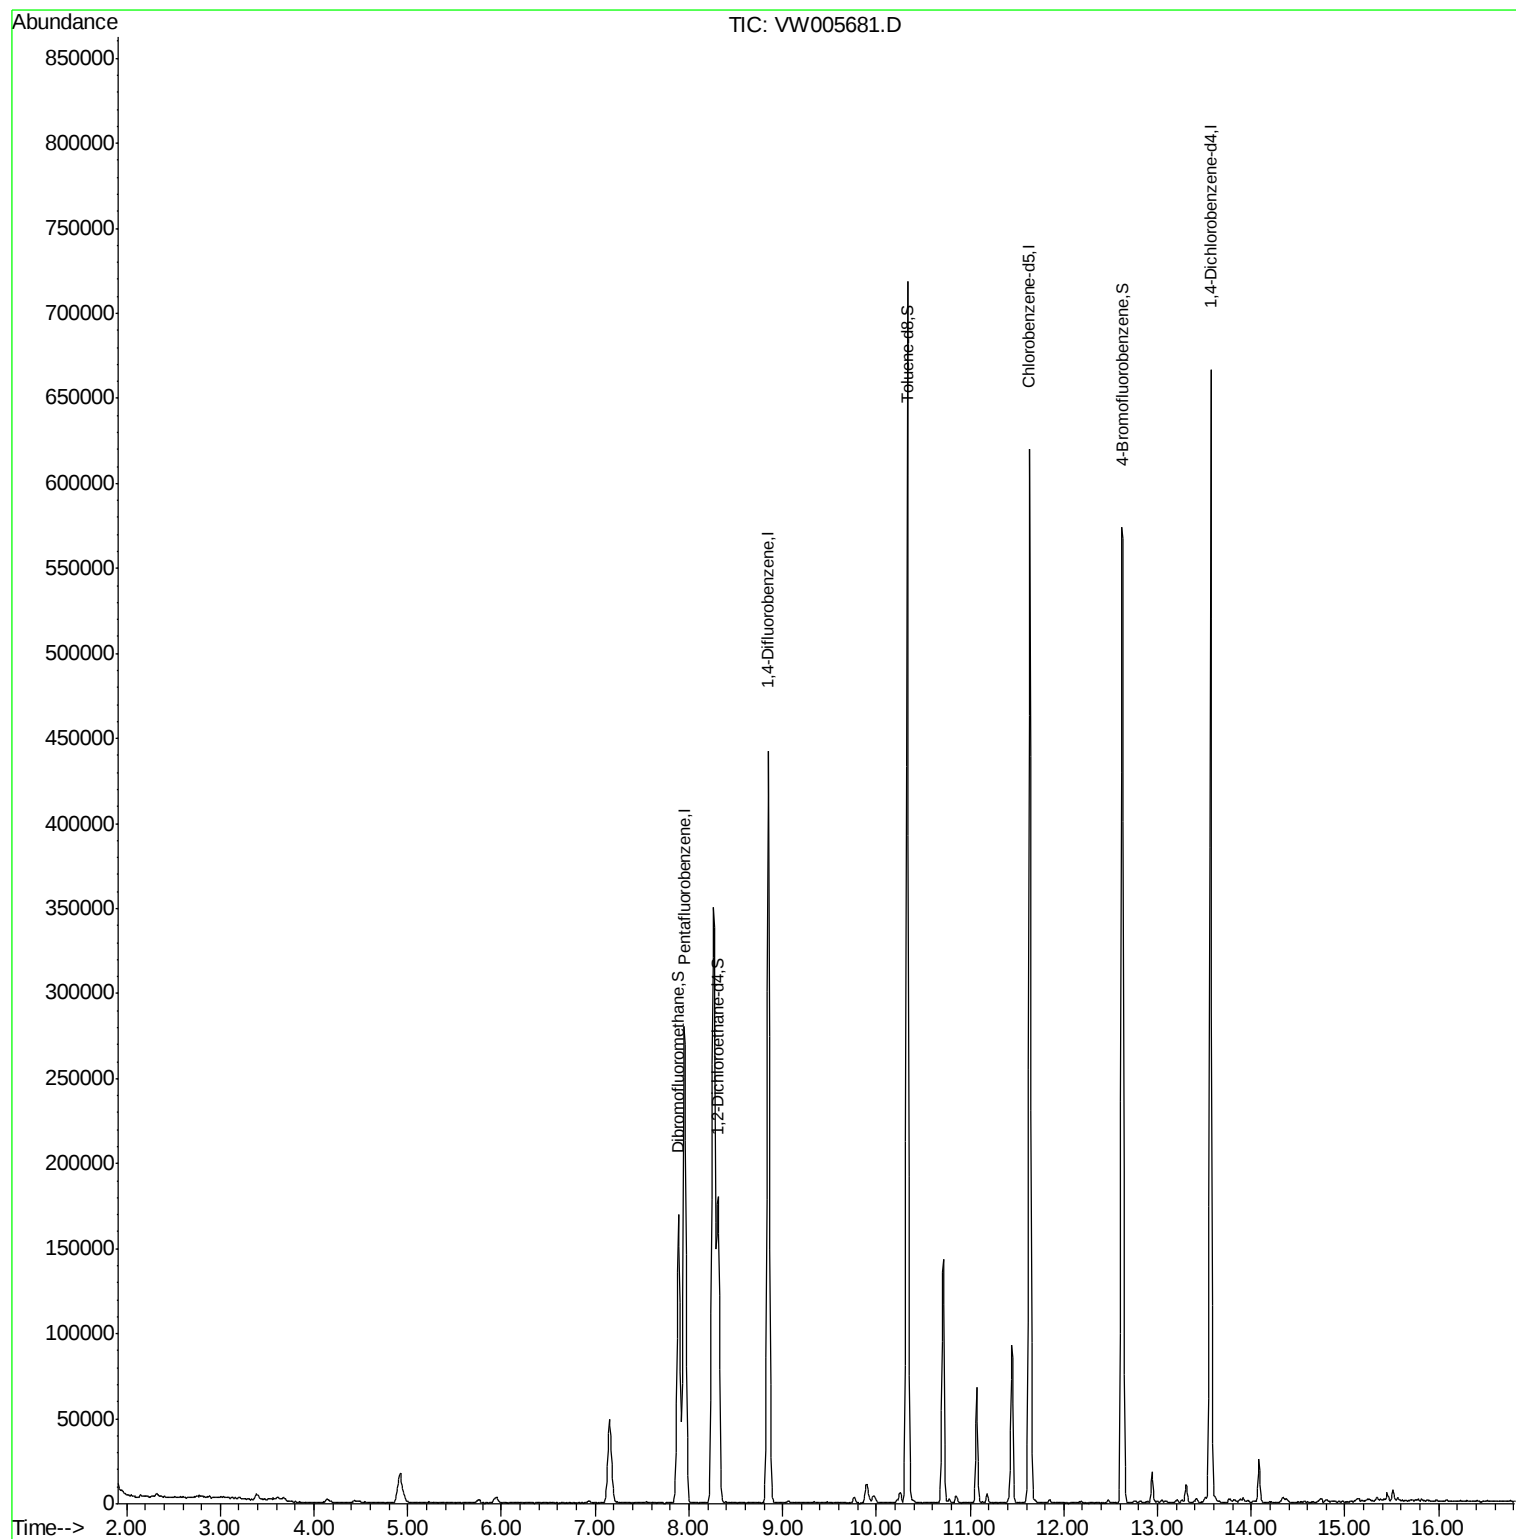

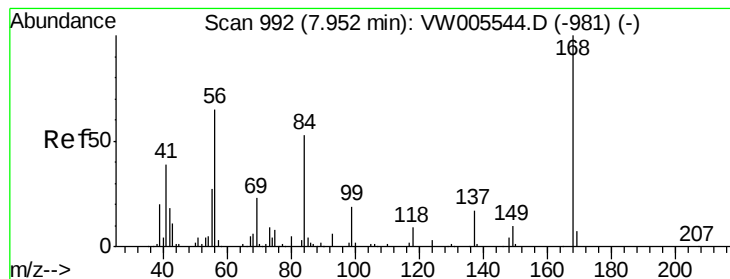

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.96 min Scan# 993

Delta R.T. 0.01 min

Lab File: VW005681.D

Acq: 27 Sep 2018 05:19

Instrument :

MSVOA_W

ClientSampleId :


VW092618SBL02

Tot Ion:168 Resp: 211373

Ion Ratio Lower Upper

168 100

99 53.8 48.4 72.6

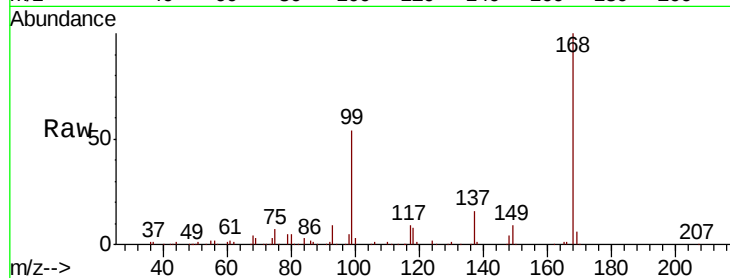

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.96

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

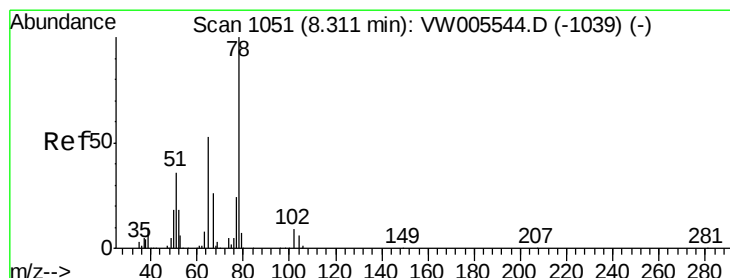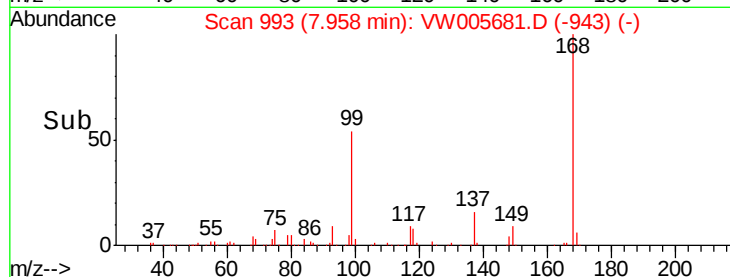

#33

1,2-Dichloroethane-d4

Concen: 57.343 ug/l

RT: 8.31 min Scan# 1051

Delta R.T. -0.00 min

Lab File: VW005681.D


Acq: 27 Sep 2018 05:19

Tgt Ion: 65 Resp: 142792

Ion Ratio Lower Upper

65 100

67 53.0 0.0 100.6

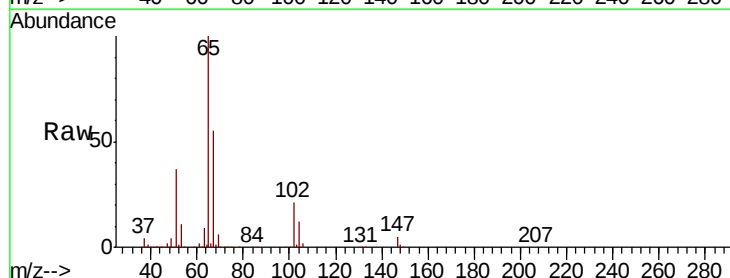

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31


60000


40000

20000

0

Time--> 8.20 8.30 8.40

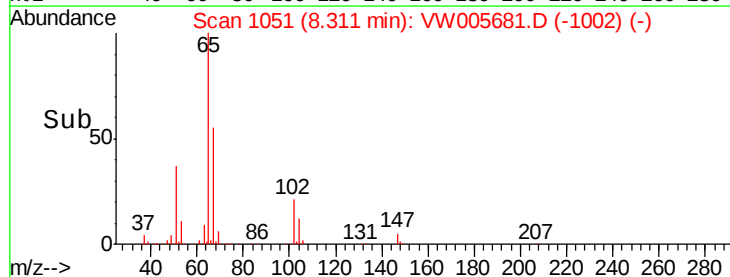


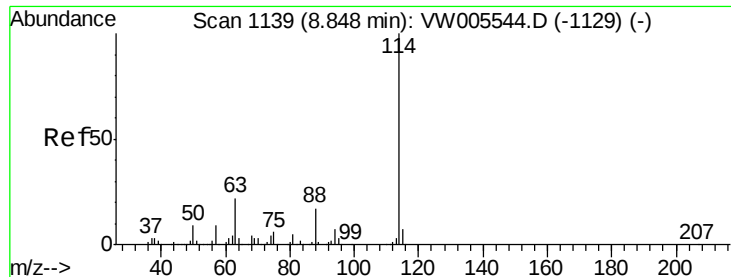




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. -0.00 min
 Lab File: VW005681.D
 Acq: 27 Sep 2018 05:19

Instrument :
 MSVOA_W
 ClientSampleId :
 VW092618SBL02

Tot Ion:114	Resp:	363589
Ion Ratio	Lower	Upper
114 100		
63 21.7	0.0	43.0
88 16.4	0.0	33.0

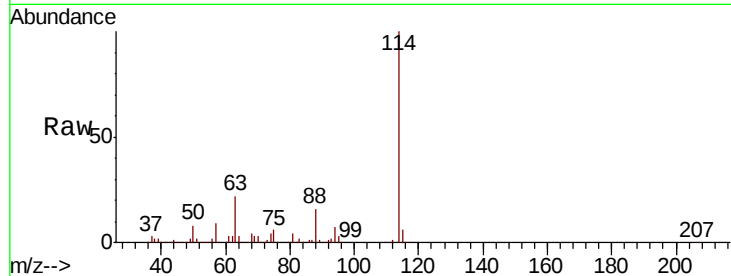


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

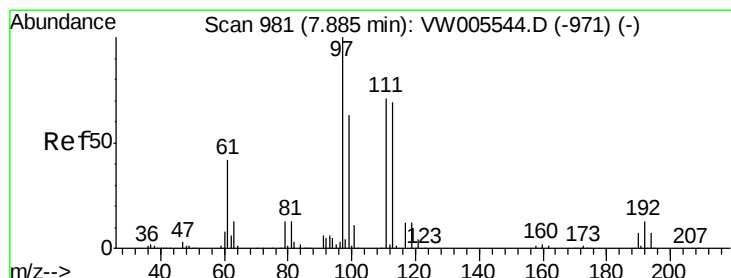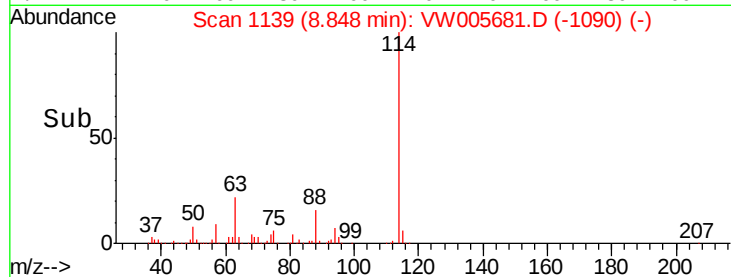
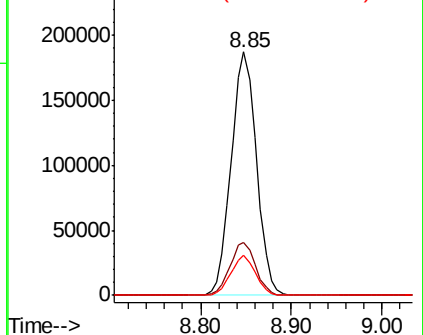



#35
 Dibromofluoromethane
 Concen: 53.440 ug/l
 RT: 7.89 min Scan# 982
 Delta R.T. 0.01 min
 Lab File: VW005681.D
 Acq: 27 Sep 2018 05:19

Tgt Ion:113	Resp:	122189
Ion Ratio	Lower	Upper
113 100		
111 102.2	82.6	123.8
192 21.0	17.0	25.4

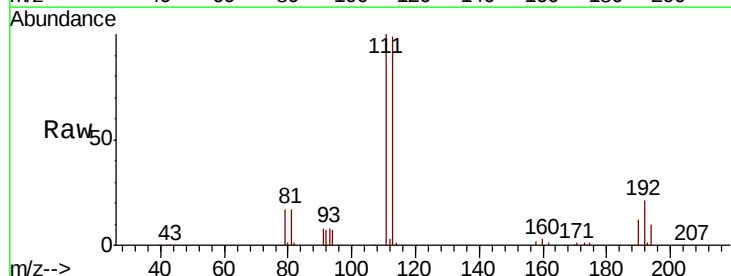

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

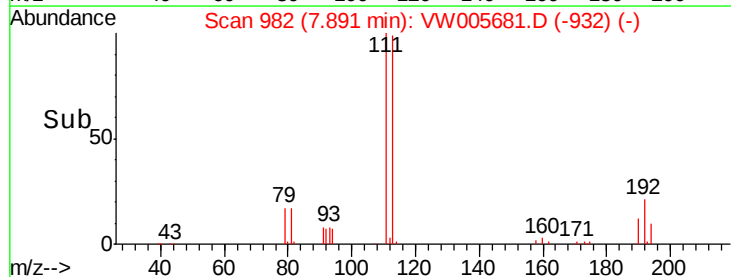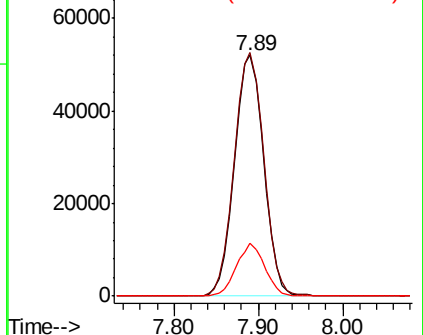

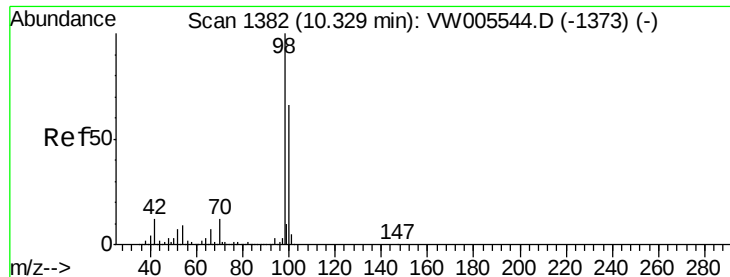

#50

Toluene-d8

Concen: 50.084 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. -0.00 min

Lab File: VW005681.D

Acq: 27 Sep 2018 05:19

Instrument :

MSVOA_W

ClientSampleId :





VW092618SBL02

Tot Ion: 98 Resp: 466287

Ion Ratio Lower Upper

98 100

100 64.2 51.6 77.4

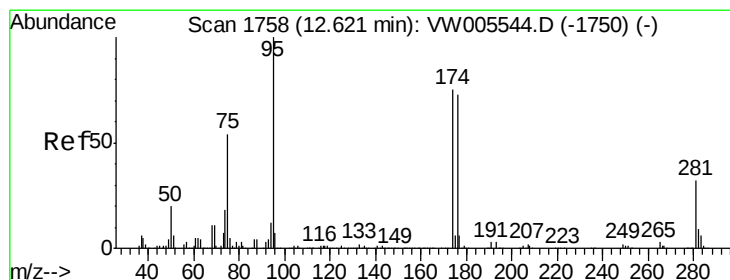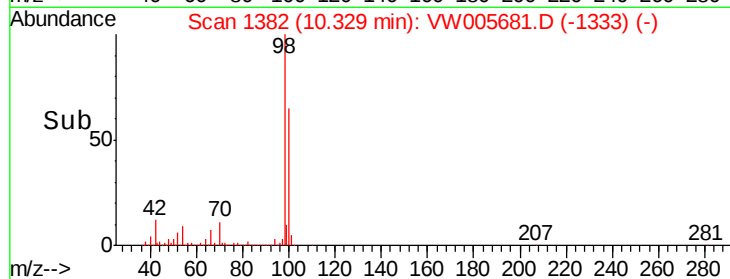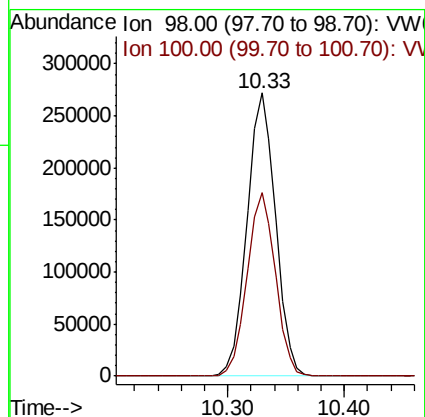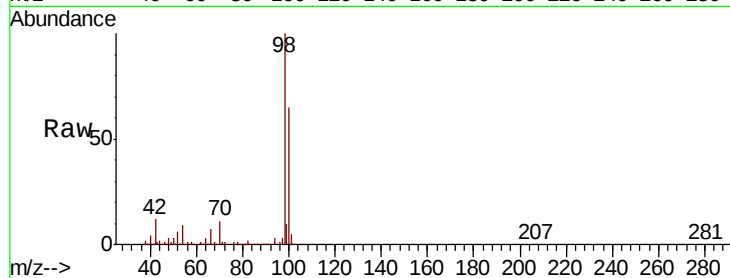

#62

4-Bromofluorobenzene

Concen: 49.166 ug/l

RT: 12.63 min Scan# 1759

Delta R.T. 0.01 min

Lab File: VW005681.D

Acq: 27 Sep 2018 05:19




Tgt Ion: 95 Resp: 169374


Ion Ratio Lower Upper

95 100

174 82.0 0.0 163.8

176 78.5 0.0 158.0


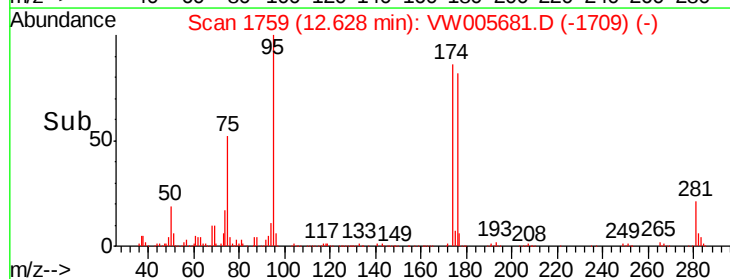
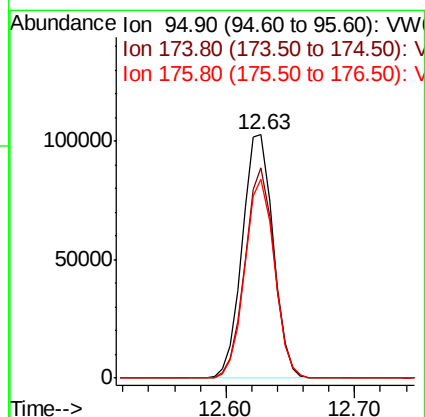
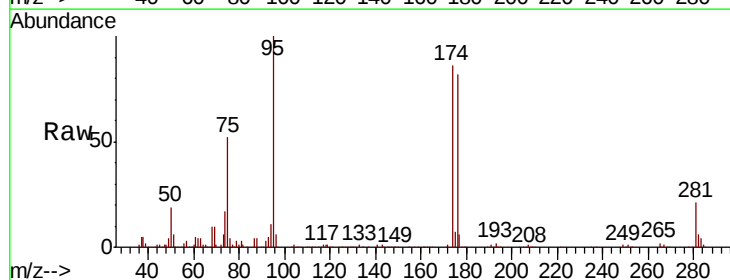


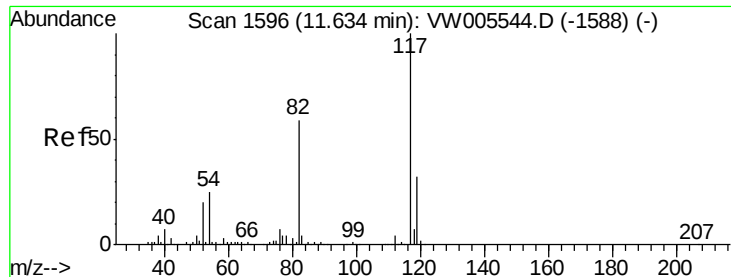

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1597
Delta R.T. 0.01 min
Lab File: VW005681.D
Acq: 27 Sep 2018 05:19

Instrument :
MSVOA_W
ClientSampleId :
VW092618SBL02

Tot Ion	Ratio	Lower	Upper
117	100		
82	55.9	46.9	70.3
119	32.2	25.7	38.5

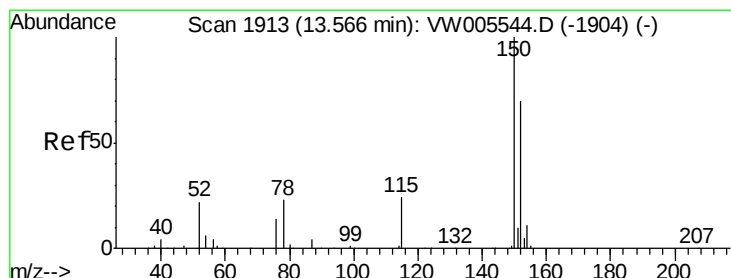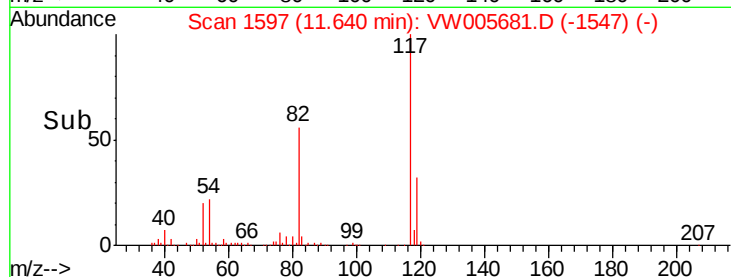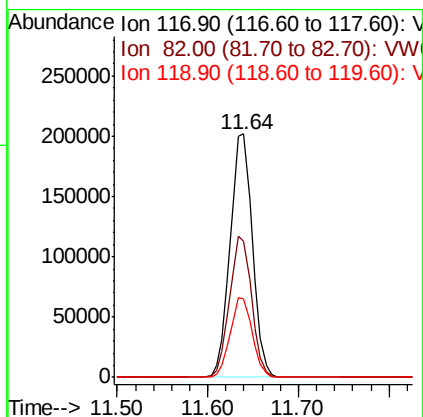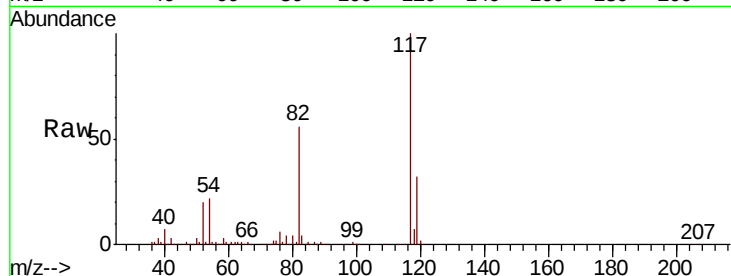

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1913
Delta R.T. -0.00 min
Lab File: VW005681.D
Acq: 27 Sep 2018 05:19

Tgt Ion	Ratio	Lower	Upper
152	100		
115	58.2	30.0	90.0
150	155.5	0.0	348.6

