


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW092618\
 Data File : VW005654.D
 Acq On : 26 Sep 2018 14:51
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
 Title : SW846 8260
 Last Update : Fri Sep 21 09:05:42 2018

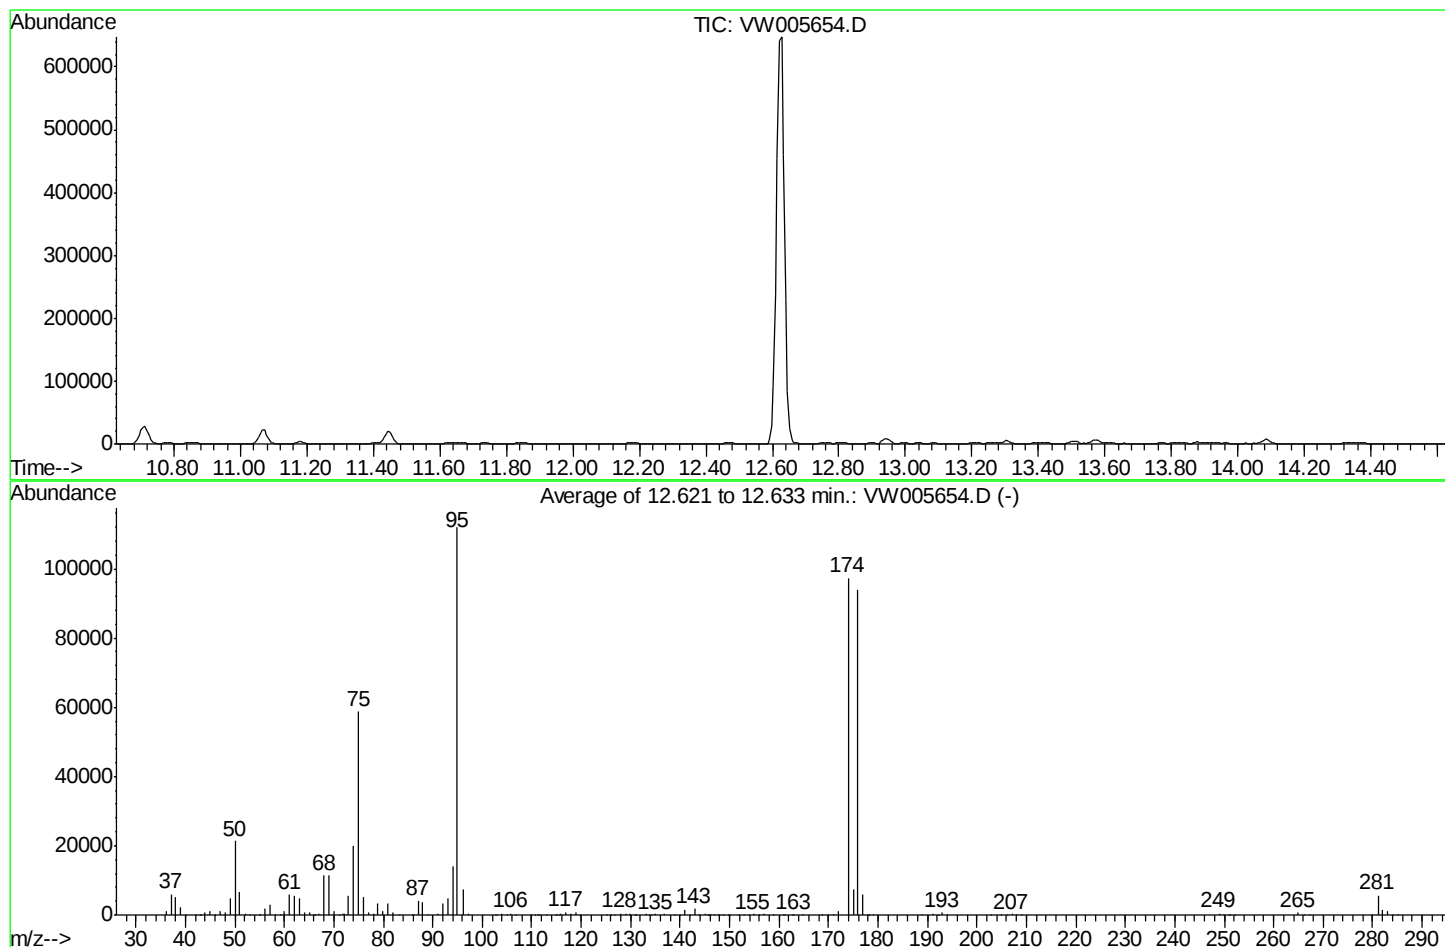

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	21315	PASS
75	95	30	60	52.4	58626	PASS
95	95	100	100	100.0	111960	PASS
96	95	5	9	6.7	7540	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.9	97274	PASS
175	174	5	9	7.7	7488	PASS
176	174	95	101	96.4	93792	PASS
177	176	5	9	6.5	6081	PASS