


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW092618\
Data File : VW005679.D
Acq On : 27 Sep 2018 03:10
Operator : VA/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
Title : SW846 8260
Last Update : Fri Sep 21 09:05:42 2018

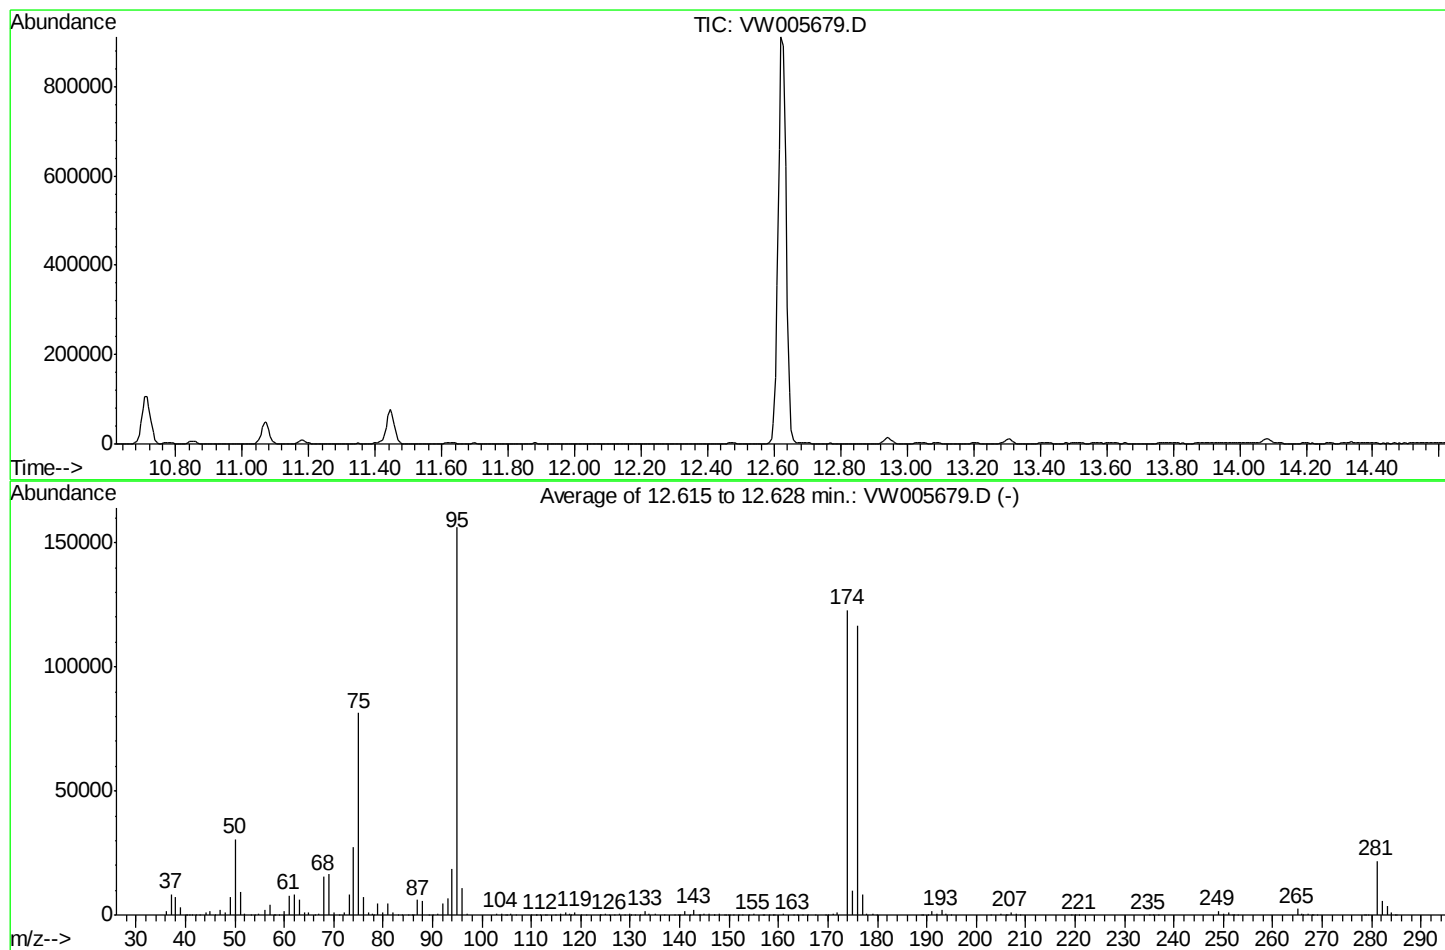

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	30648	PASS
75	95	30	60	52.1	81482	PASS
95	95	100	100	100.0	156256	PASS
96	95	5	9	7.0	10876	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.6	122869	PASS
175	174	5	9	8.1	9980	PASS
176	174	95	101	95.0	116773	PASS
177	176	5	9	7.1	8340	PASS