




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092619\
Data File : VW013304.D
Acq On : 26 Sep 2019 13:46
Operator : SY/VA
Sample : VW0926SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK01

Manual Integrations
APPROVED

MMDadoda
10/9/2019 2:13:03 PM

Quant Time: Sep 26 19:09:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092619S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 12:57:49 2019
Response via : Initial Calibration

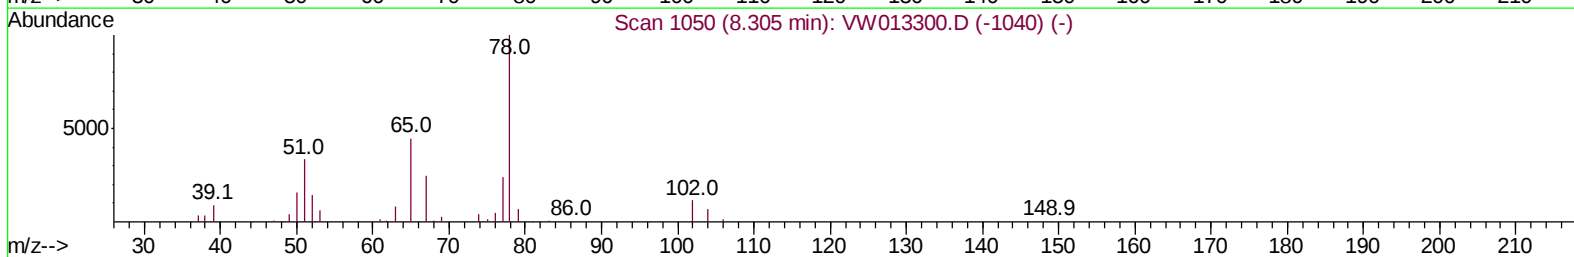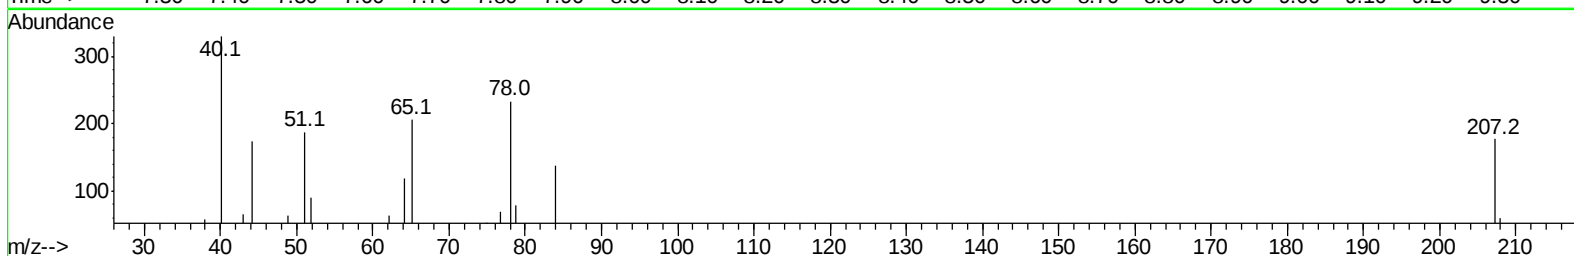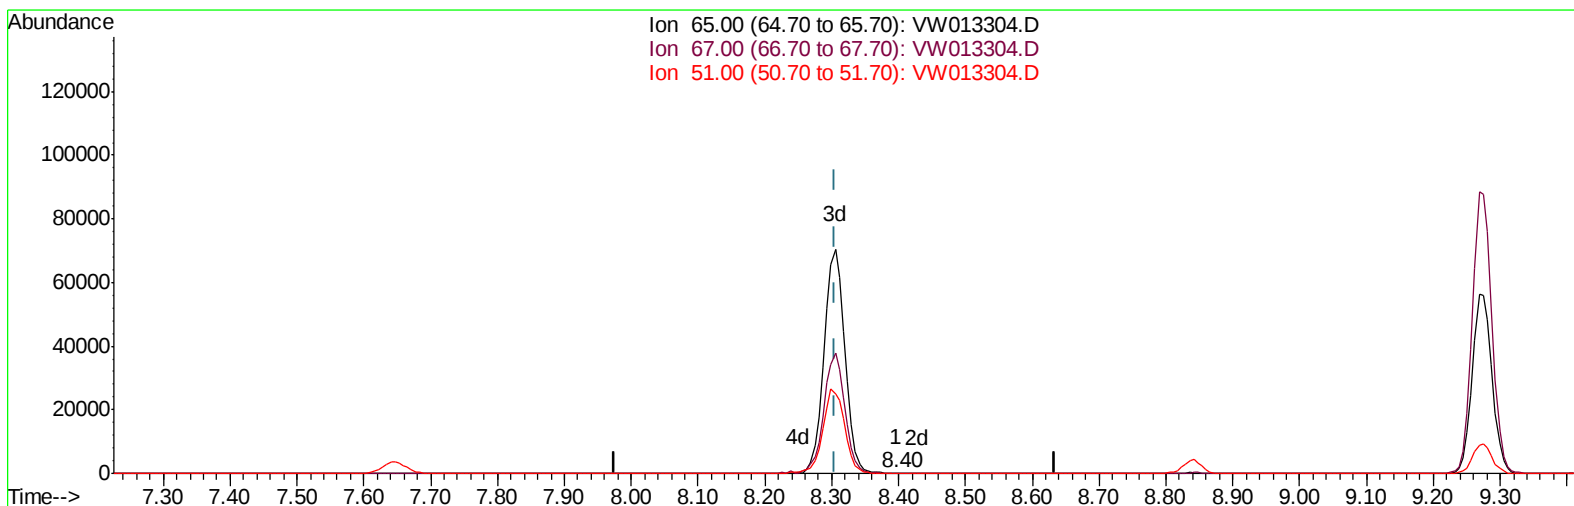

TIC: VW013304.D

(26) 1,2-Dichloroethane-d4 (S)

8.397min (+0.092) 0.04ug/L

response 218

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	42.66
51.00	109.60	113.30
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092619\
Data File : VW013304.D
Acq On : 26 Sep 2019 13:46
Operator : SY/VA
Sample : VW0926SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK01

Manual Integrations
APPROVED

MMDadoda
10/9/2019 2:13:03 PM

Quant Time: Sep 26 19:09:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092619S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 12:57:49 2019
Response via : Initial Calibration

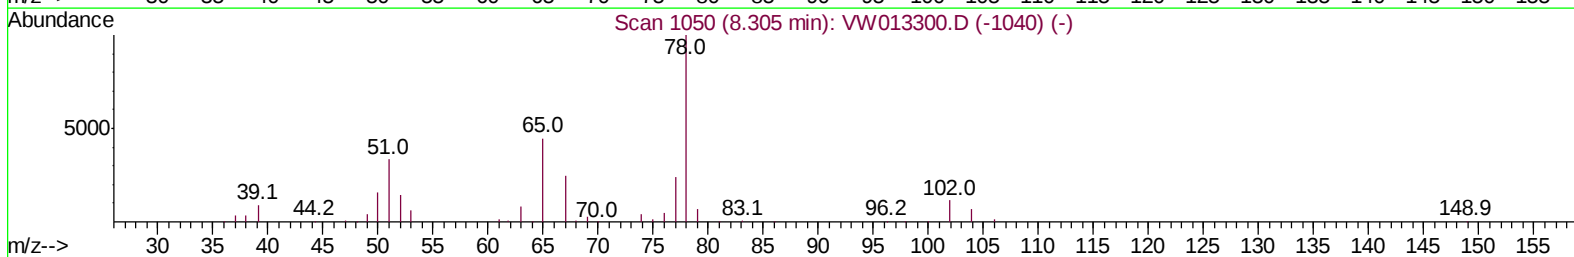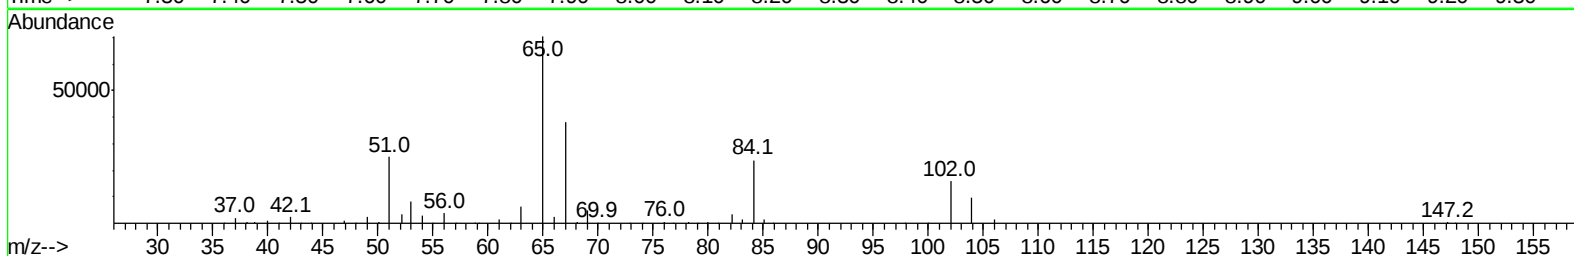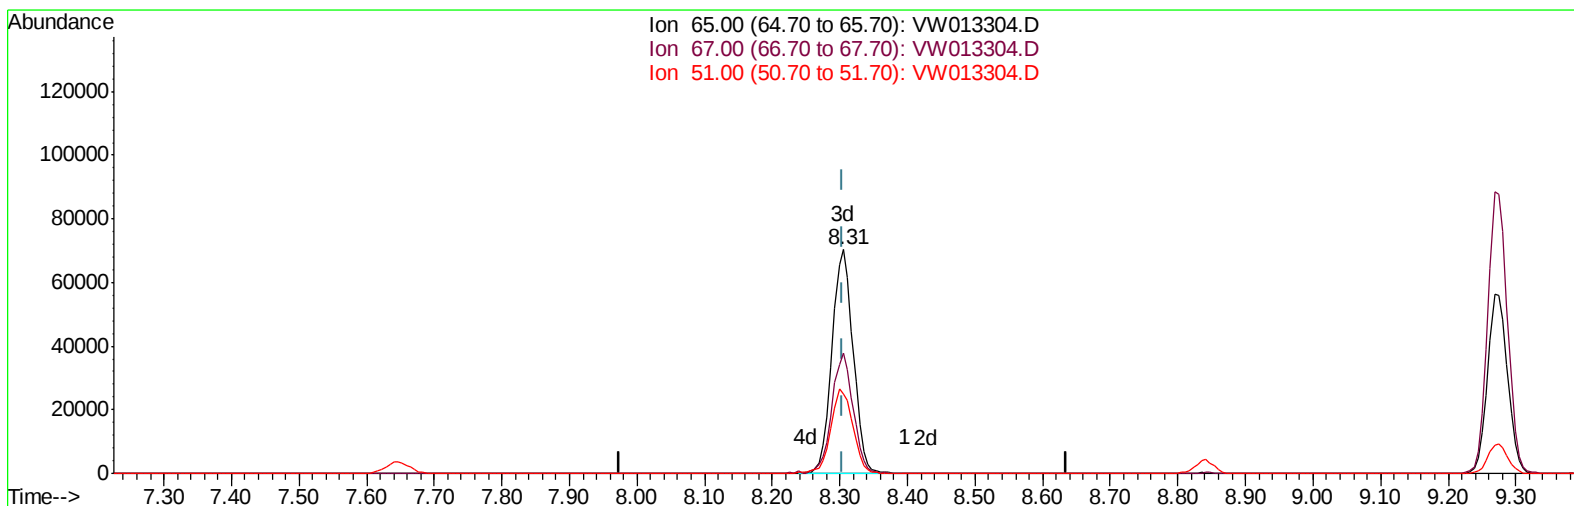

TIC: VW013304.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 25.29ug/L m

response 151918

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.06#
51.00	109.60	0.16#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092619\
 Data File : VW013304.D
 Acq On : 26 Sep 2019 13:46
 Operator : SY/VA
 Sample : VW0926SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK01

Manual Integrations
 APPROVED

MMDadoda
 10/9/2019 2:13:03 PM

Quant Time: Sep 26 19:16:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092619S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 12:57:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	493155	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	443177	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	216999	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	150114	25.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.12%
7) Chloroethane-d5	2.89	69	117674	24.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.72%
10) 1,1-Dichloroethene-d2	4.01	63	219031	18.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.68%
20) 2-Butanone-d5	7.08	46	102106	50.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.48%
24) Chloroform-d	7.65	84	271097	24.38	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.52%
26) 1,2-Dichloroethane-d4	8.31	65	151918m	25.29	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.16%
29) Benzene-d6	8.27	84	601042	24.98	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.92%
33) 1,2-Dichloropropane-d6	9.27	67	178511	24.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.56%
37) Toluene-d8	10.32	98	567383	25.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.16%
38) trans-1,3-Dichloropropene-	10.58	79	79152	24.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.28%
39) 2-Hexanone-d5	10.92	63	81275	51.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.60%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	154300	25.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	199498	25.74	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.96%

Target Compounds					Ovalue
16) Methylene chloride	4.92	84	15934	2.163 ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092619\
Data File : VW013304.D
Acq On : 26 Sep 2019 13:46
Operator : SY/VA
Sample : VW0926SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK01

Manual Integrations
APPROVED

MMDadoda
10/9/2019 2:13:03 PM

Quant Time: Sep 26 19:16:13 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092619S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 12:57:49 2019
Response via : Initial Calibration

