


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW092620\
 Data File : VW016650.D
 Acq On : 25 Sep 2020 08:44
 Operator : SY/VA
 Sample : BFB103
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB103

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM091820SMA.M
 Title : SFAM01.0
 Last Update : Sat Sep 26 00:13:39 2020

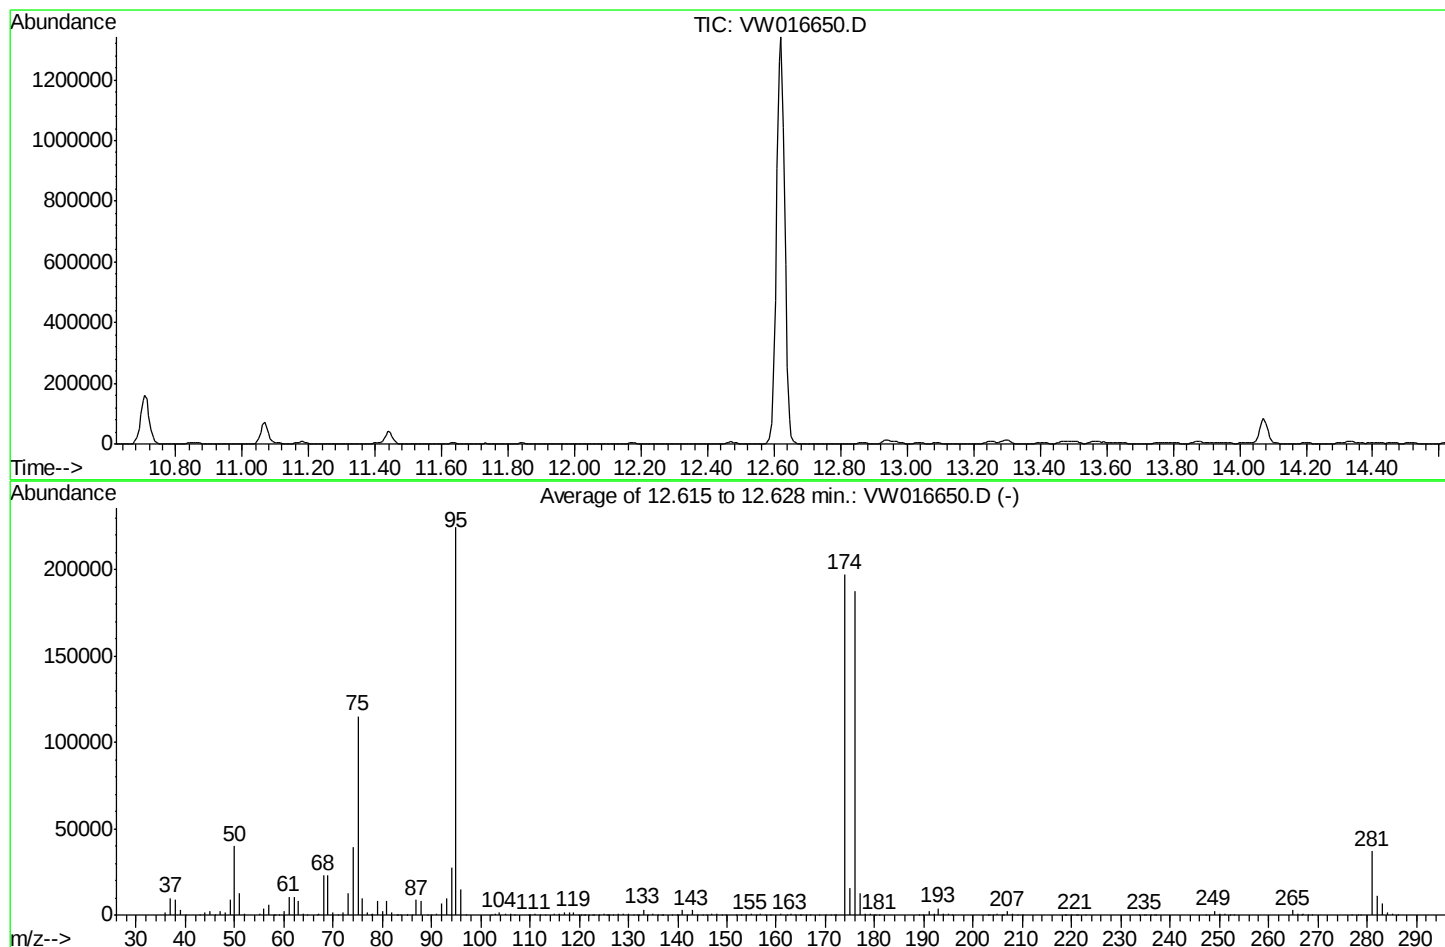

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	39933	PASS
75	95	30	80	51.2	115010	PASS
95	95	100	100	100.0	224448	PASS
96	95	5	9	6.7	14947	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.8	197098	PASS
175	174	5	9	7.8	15463	PASS
176	174	95	105	95.3	187797	PASS
177	176	5	10	6.9	12881	PASS

m/z	Abundance
36.00	2035.0
37.00	10732.0
38.00	9557.0
39.00	3398.0
40.10	281.0
41.10	102.0
43.10	302.0
44.00	1674.0
45.00	2390.0
46.00	226.0
47.10	1765.0
48.00	1552.0
49.00	9327.0
50.00	42032.0
51.00	13528.0
52.00	726.0
55.00	762.0
56.00	3720.0
57.00	6516.0
57.90	366.0
59.00	666.0
60.00	2174.0
61.00	11054.0
62.00	11254.0
63.00	8728.0
64.00	801.0
64.80	128.0
66.90	612.0
68.00	23968.0
69.00	24264.0
70.00	2012.0
71.10	143.0
72.00	1458.0
73.00	14008.0
74.00	40952.0
75.00	120544.0
76.00	10457.0
77.00	1418.0
78.00	1249.0
78.90	8199.0
80.00	2451.0
80.90	8510.0
81.90	1870.0
82.80	336.0
83.80	63.0
84.90	140.0
86.00	314.0
87.00	8489.0
87.90	8220.0
89.10	204.0
90.90	919.0
92.00	6533.0
93.00	9541.0
94.00	27592.0
95.00	224384.0
96.00	15703.0
97.10	429.0
103.00	1138.0
103.90	1416.0
104.90	559.0
105.90	1148.0
106.80	203.0
110.10	424.0
110.90	633.0
112.10	281.0
113.00	268.0
115.00	382.0
115.90	847.0
117.00	1904.0
117.90	1784.0
118.90	2150.0
119.90	133.0
120.30	125.0
120.90	239.0
123.90	229.0
125.00	1707.0
125.60	620.0
126.20	226.0
126.90	131.0
127.90	931.0
129.00	373.0
129.80	950.0
130.90	383.0
131.90	225.0
133.00	5228.0
133.80	1102.0
135.00	799.0
135.90	70.0
136.70	386.0
138.90	63.0
139.80	125.0
140.90	2736.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

142.00	333.0
142.90	2407.0
144.00	180.0
145.00	327.0
145.80	303.0
147.00	708.0
147.90	752.0
148.90	410.0
149.80	292.0
151.90	124.0
152.90	199.0
153.80	224.0
154.90	614.0
155.90	92.0
156.90	559.0
158.90	390.0
160.90	543.0
162.10	95.0
162.90	997.0
163.90	86.0
164.90	642.0
166.10	109.0
166.90	122.0
168.90	69.0
170.10	52.0
170.90	139.0
172.00	450.0
174.00	189760.0
175.10	14504.0
176.00	168704.0
176.90	12551.0
178.00	658.0
179.00	1212.0
179.90	249.0
181.10	200.0
189.00	456.0
189.80	176.0
191.00	4059.0
192.00	1080.0
193.00	5973.0
194.00	1206.0
195.00	749.0
195.80	69.0
202.90	648.0
204.00	92.0
204.90	1305.0
206.00	363.0
207.00	3571.0
208.00	810.0
208.90	372.0
210.00	77.0
218.70	169.0
219.90	97.0
220.90	284.0
222.90	76.0
234.90	703.0
236.10	166.0
237.10	119.0
247.20	95.0
249.00	3658.0
249.90	961.0
251.00	1367.0
252.10	370.0
252.90	219.0
265.00	3946.0
266.10	1195.0
267.10	996.0
268.00	268.0
268.80	105.0
276.80	76.0
278.20	146.0
278.70	169.0
281.00	54688.0
282.00	17528.0
283.00	10453.0
284.10	2104.0
285.10	717.0
286.10	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

m/z	Abundance
36.00	2033.0
37.00	10351.0
38.00	9617.0
39.00	3553.0
39.90	210.0
41.10	113.0
43.10	255.0
44.00	1741.0
45.00	2150.0
46.10	223.0
47.00	2514.0
48.00	1433.0
49.00	10118.0
50.00	44592.0
51.00	13824.0
52.00	690.0
55.10	705.0
56.00	3767.0
57.00	6733.0
58.10	309.0
59.00	386.0
60.00	2022.0
61.00	11581.0
62.00	11499.0
63.00	8878.0
64.00	875.0
64.90	131.0
67.10	645.0
68.00	25592.0
69.00	25208.0
70.00	2068.0
71.10	163.0
72.00	1354.0
73.00	13909.0
74.00	44536.0
75.00	126552.0
76.00	10908.0
77.00	1213.0
78.10	972.0
78.90	8933.0
79.90	2527.0
80.90	9050.0
81.90	1989.0
83.10	329.0
83.80	56.0
85.10	138.0
86.00	327.0
86.90	9480.0
87.90	9674.0
89.90	55.0
91.00	1040.0
92.00	7120.0
93.00	11089.0
94.00	30264.0
95.00	252480.0
96.00	16163.0
97.10	413.0
102.10	64.0
103.00	590.0
103.90	1248.0
105.00	519.0
105.90	1240.0
106.90	309.0
109.80	274.0
110.90	546.0
111.90	273.0
112.90	258.0
115.00	436.0
115.90	1100.0
116.90	1759.0
118.00	1103.0
118.90	1909.0
119.80	197.0
121.10	104.0
121.80	81.0
122.60	72.0
123.00	58.0
123.90	239.0
124.90	863.0
125.80	270.0
126.70	71.0
127.90	1024.0
129.00	530.0
129.90	1104.0
130.80	480.0
131.80	107.0
132.10	118.0
133.00	2588.0
134.90	856.0
135.90	134.0
136.90	466.0
138.90	98.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

140.00	311.0
141.00	2787.0
142.00	419.0
142.90	3160.0
143.80	223.0
144.90	355.0
145.90	482.0
146.90	532.0
148.00	728.0
149.00	338.0
149.90	435.0
151.80	144.0
152.90	168.0
153.90	168.0
154.90	660.0
155.80	112.0
156.80	506.0
157.70	54.0
159.00	341.0
160.80	383.0
162.90	596.0
164.00	87.0
165.10	442.0
165.90	85.0
167.00	89.0
170.10	54.0
170.90	113.0
171.70	433.0
173.90	212544.0
175.00	16808.0
175.90	218048.0
176.90	12642.0
178.00	633.0
179.00	766.0
180.00	103.0
180.90	76.0
189.00	406.0
190.90	2581.0
192.00	617.0
193.00	3848.0
193.90	578.0
195.00	446.0
202.90	334.0
203.90	154.0
205.00	804.0
206.20	305.0
207.00	2135.0
208.00	455.0
209.00	359.0
218.70	61.0
219.00	65.0
220.90	132.0
233.80	51.0
235.10	325.0
236.10	57.0
236.70	70.0
237.10	65.0
247.20	99.0
249.00	2204.0
250.00	542.0
251.00	972.0
252.00	268.0
253.00	101.0
265.00	3190.0
265.90	855.0
267.00	562.0
268.10	143.0
268.90	73.0
278.10	91.0
278.80	171.0
281.10	38520.0
282.10	10293.0
283.00	6139.0
284.10	1504.0
285.10	362.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

m/z	Abundance
36.00	1489.0
37.00	7938.0
38.00	7389.0
39.00	2480.0
40.00	370.0
41.20	53.0
43.10	188.0
43.90	1385.0
45.00	1577.0
46.10	153.0
46.90	1827.0
48.00	1058.0
49.00	7343.0
50.00	33176.0
51.00	10426.0
52.00	398.0
55.00	500.0
56.00	2821.0
57.00	5162.0
57.90	236.0
59.10	124.0
60.00	1711.0
61.00	8855.0
62.00	8968.0
63.00	6447.0
64.00	665.0
64.90	108.0
67.00	564.0
68.00	18568.0
69.00	19584.0
70.00	1469.0
71.00	182.0
72.00	1029.0
73.00	9182.0
74.00	32320.0
75.00	97936.0
76.00	8101.0
77.00	1374.0
77.80	754.0
78.90	6731.0
79.90	1928.0
80.90	7179.0
82.00	1549.0
82.90	239.0
85.90	279.0
87.00	7781.0
87.90	7549.0
91.00	895.0
92.00	6098.0
93.00	8848.0
94.00	24584.0
95.00	196480.0
96.00	13143.0
96.90	328.0
102.80	373.0
103.80	1020.0
104.90	364.0
106.00	963.0
107.00	279.0
110.00	213.0
110.80	237.0
111.80	202.0
113.00	303.0
114.90	395.0
115.90	722.0
116.90	1323.0
117.80	667.0
118.90	1270.0
119.90	68.0
122.60	72.0
123.00	55.0
123.90	191.0
125.00	353.0
125.50	248.0
126.00	167.0
127.90	963.0
128.90	418.0
129.90	713.0
131.00	298.0
132.90	1098.0
134.80	387.0
135.00	375.0
135.80	62.0
136.90	470.0
138.80	54.0
139.80	148.0
140.90	2572.0
142.00	331.0
143.00	2681.0
144.00	172.0
145.00	230.0
145.90	343.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

147.00	265.0
147.80	483.0
149.00	214.0
149.80	232.0
151.90	105.0
152.90	203.0
153.80	178.0
154.90	696.0
155.90	113.0
156.90	408.0
157.70	105.0
158.80	260.0
161.00	325.0
162.90	251.0
163.80	56.0
164.80	167.0
168.70	65.0
171.00	113.0
171.80	473.0
173.90	188992.0
174.90	15077.0
176.00	176640.0
176.90	13452.0
177.90	601.0
178.90	293.0
180.20	64.0
188.90	161.0
190.90	1023.0
192.00	214.0
193.00	1727.0
194.10	285.0
194.80	125.0
202.70	64.0
203.20	65.0
205.00	274.0
207.10	1000.0
207.90	233.0
209.10	133.0
220.70	72.0
221.10	59.0
234.70	131.0
235.10	122.0
247.00	55.0
249.00	1076.0
250.00	497.0
251.00	604.0
252.00	115.0
264.90	1249.0
266.00	505.0
266.80	239.0
268.00	63.0
278.80	67.0
281.10	17328.0
282.00	4688.0
283.10	2874.0
284.20	357.0
285.10	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

Scan 1749 (12.567 min): VW016650.D
BFB103

m/z	Abundance
38.80	61.0
39.90	250.0
41.20	108.0
42.90	145.0
44.00	433.0
54.90	72.0
55.90	57.0
57.00	162.0
68.90	71.0
69.90	62.0
95.90	56.0
207.10	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103