


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091919\
 Data File : VU034648.D
 Acq On : 19 Sep 2019 14:34
 Operator : JC/SP
 Sample : BFB34
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 28 02:29:26 2019

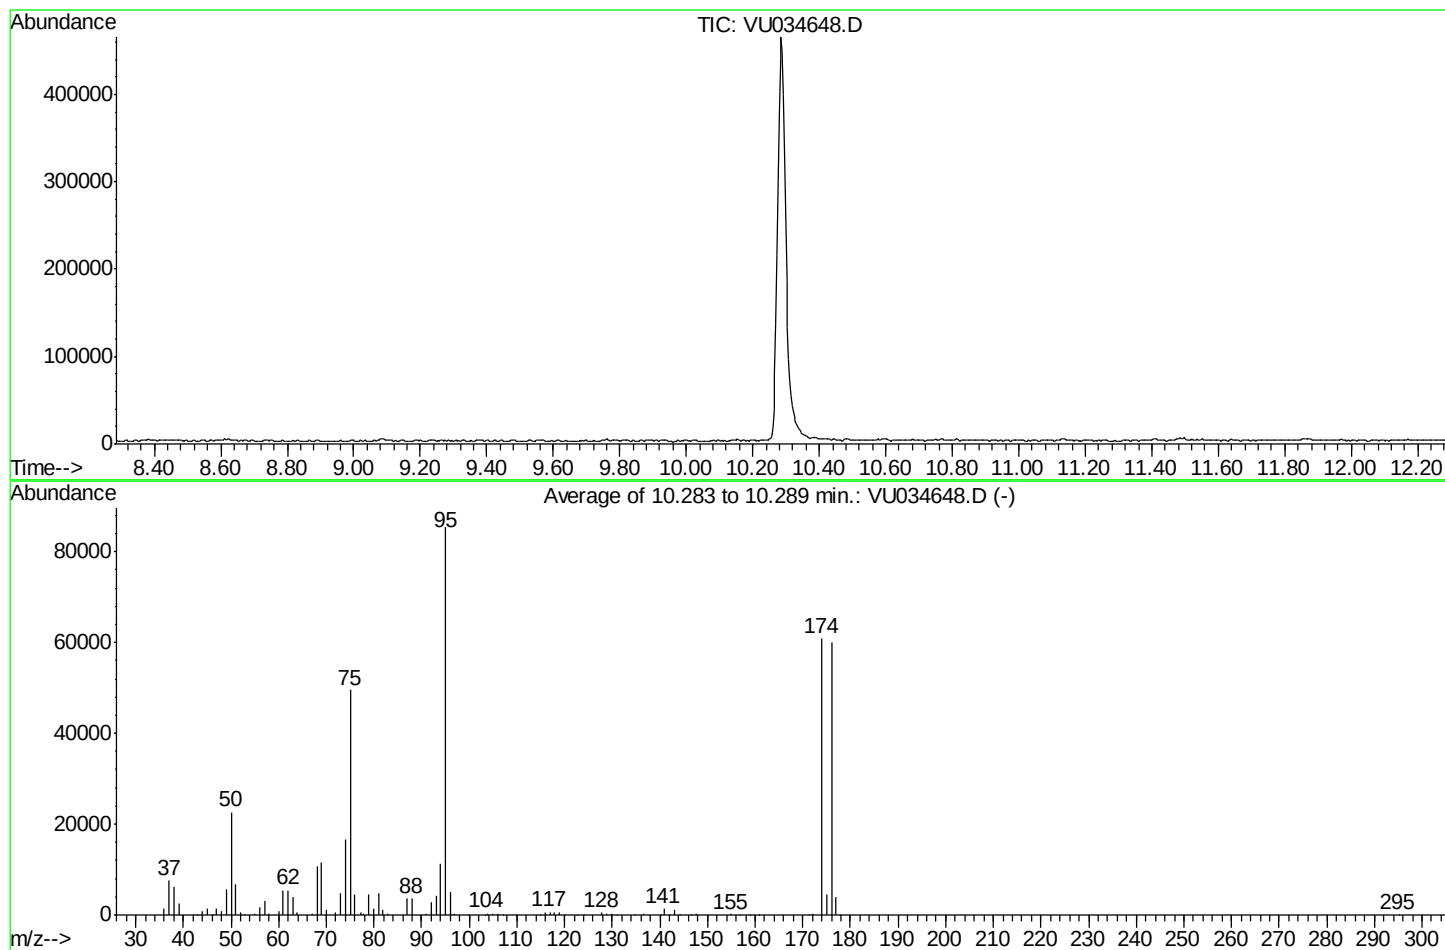

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.5	22624	PASS
75	95	30	80	58.0	49538	PASS
95	95	100	100	100.0	85354	PASS
96	95	5	9	5.9	5055	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.3	60834	PASS
175	174	5	9	7.2	4405	PASS
176	174	95	101	98.8	60082	PASS
177	176	5	9	6.7	4028	PASS