

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092818\
 Data File : VW005727.D
 Acq On : 28 Sep 2018 18:34
 Operator : SY/AP
 Sample : J5011-08
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK02

Quant Time: Sep 29 22:11:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 28 16:00:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	234540	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	225590	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	113510	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	66510	22.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.96%
7) Chloroethane-d5	2.90	69	52415	22.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.88%
10) 1,1-Dichloroethene-d2	4.01	63	112859	17.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.16%
20) 2-Butanone-d5	7.09	46	57676	60.09	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.18%
24) Chloroform-d	7.65	84	142661	23.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.72%
26) 1,2-Dichloroethane-d4	8.31	65	95890	26.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.12%
29) Benzene-d6	8.28	84	269446	24.13	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.52%
33) 1,2-Dichloropropane-d6	9.28	67	79857	24.74	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.96%
37) Toluene-d8	10.33	98	259131	23.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.00%
38) trans-1,3-Dichloropropene-	10.59	79	39737	23.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.76%
39) 2-Hexanone-d5	10.93	63	42432	56.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.28%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	84640	26.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	103587	25.79	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.16%


Target Compounds					Ovalue
13) Acetone	4.14	43	1911	1.912 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092818\
Data File : VW005727.D
Acq On : 28 Sep 2018 18:34
Operator : SY/AP
Sample : J5011-08
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK02

Quant Time: Sep 29 22:11:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 28 16:00:53 2018
Response via : Initial Calibration

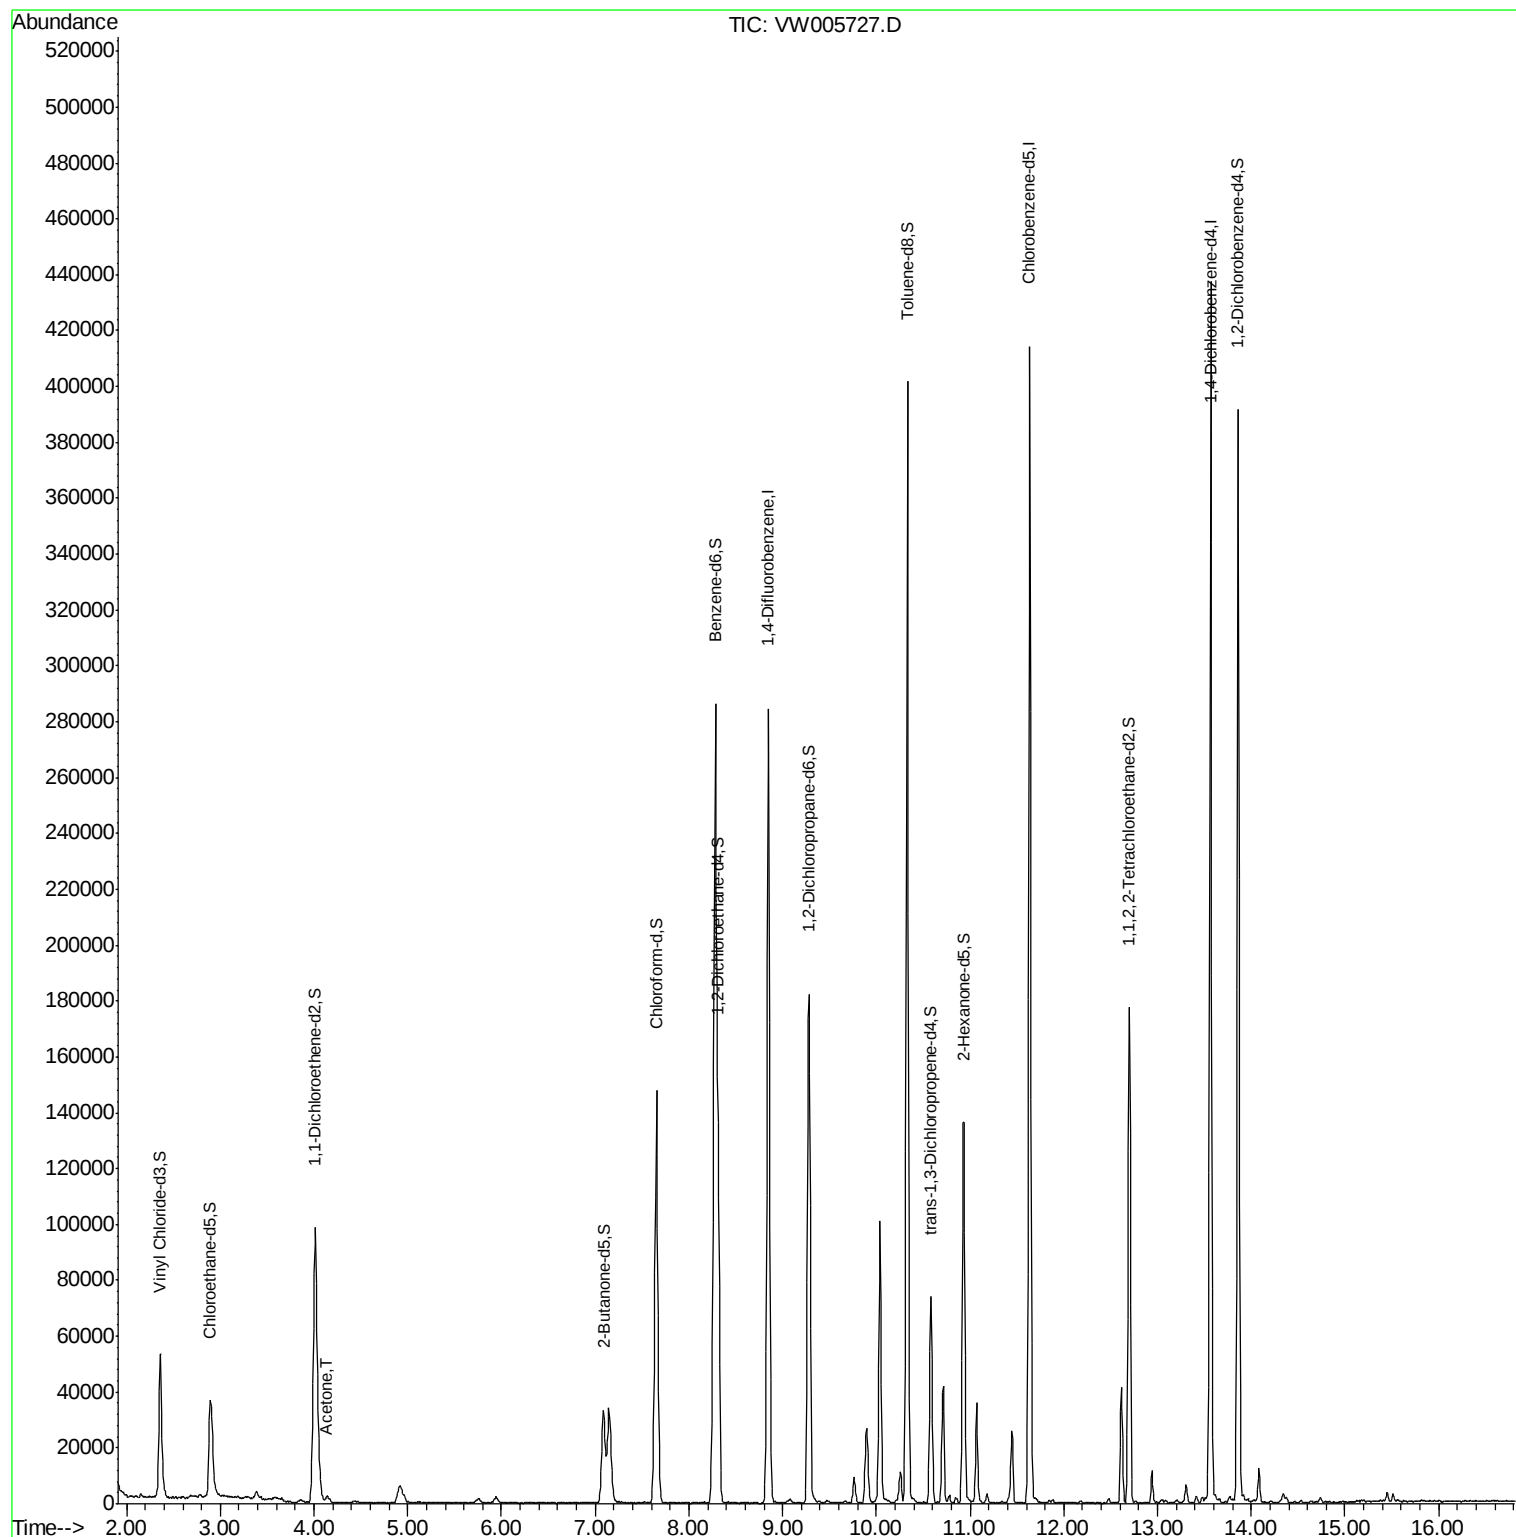

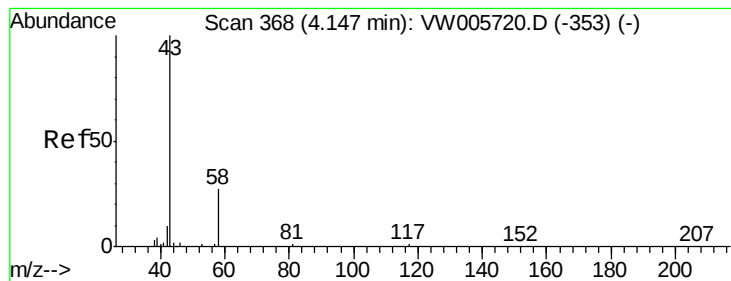

#13
 Acetone
 Concen: 1.912 ug/L
 RT: 4.14 min Scan# 366
 Delta R.T. -0.01 min
 Lab File: VW005727.D
 Acq: 28 Sep 2018 18:34

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK02

Tot Ion: 43 Resp: 1911
 Ion Ratio Lower Upper
 43 100
 58 16.2 0.0 31.8

