

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092820\
 Data File : VW016675.D
 Acq On : 28 Sep 2020 18:05
 Operator : SY/VA
 Sample : L4144-04
 Misc : 5.07G/10ML/MSVOA W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AM2

Manual Integrations
 APPROVED

SAM
 10/12/2020 6:08:55 PM

Quant Time: Sep 29 07:24:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 29 05:26:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	923996	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	830797	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	394948	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	128470	14.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.44%
7) Chloroethane-d5	2.91	69	117657	16.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.44%
10) 1,1-Dichloroethene-d2	4.03	63	213554	10.68	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.72%#
20) 2-Butanone-d5	7.08	46	85178	34.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.86%
24) Chloroform-d	7.65	84	337024	17.44	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.76%
26) 1,2-Dichloroethane-d4	8.31	65	181110	18.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.00%
29) Benzene-d6	8.28	84	645257	17.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.28%
33) 1,2-Dichloropropane-d6	9.28	67	184971	18.32	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.28%
37) Toluene-d8	10.33	98	616737	16.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.28%
38) trans-1,3-Dichloropropene-	10.59	79	80853	15.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	63.52%
39) 2-Hexanone-d5	10.93	63	67422	36.71	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	157361	18.32	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.28%
61) 1,2-Dichlorobenzene-d4	13.85	152	224593	17.80	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	71.20%#

Target Compounds					Ovalue
13) Acetone	4.15	43	2721m	1.425 ug/L	
16) Methylene chloride	4.93	84	28390	1.992 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092820\
Data File : VW016675.D
Acq On : 28 Sep 2020 18:05
Operator : SY/VA
Sample : L4144-04
Misc : 5.07G/10ML/MSVOA W/SOIL
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampled :
C0AM2

Manual Integrations
APPROVED

SAM
10/12/2020 6:08:55 PM

Quant Time: Sep 29 07:24:02 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 29 05:26:53 2020
Response via : Initial Calibration

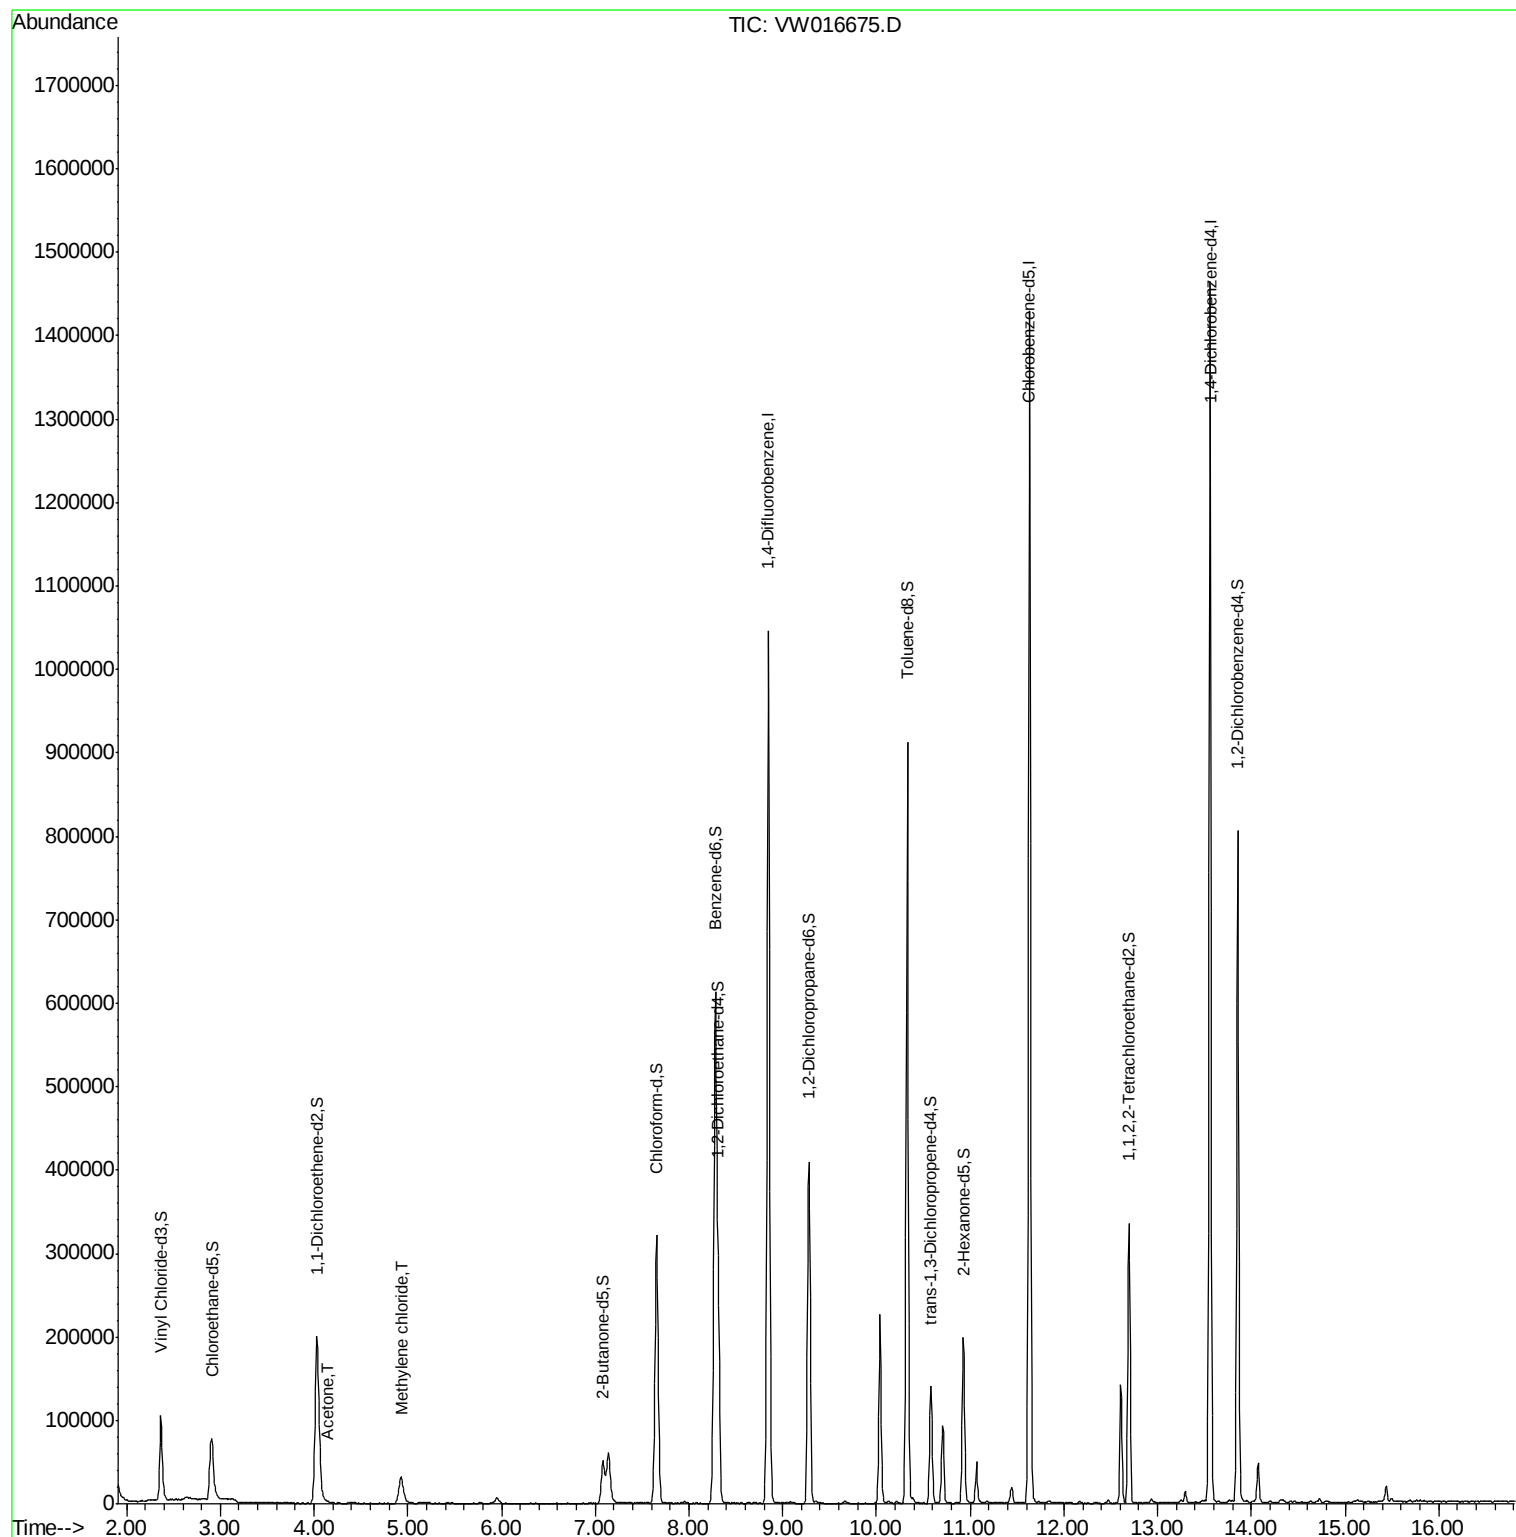

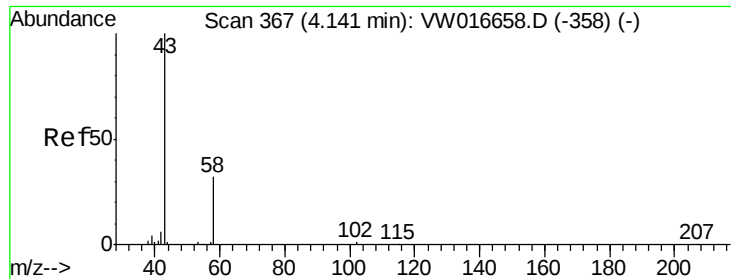





#13
Acetone
Concen: 1.425 ug/L m
RT: 4.15 min Scan# 368
Delta R.T. 0.01 min
Lab File: VW016675.D
Acq: 28 Sep 2020 18:05

Instrument :
MSVOA_W
ClientSampleId :
C0AM2

Tot Ion: 43 Resp: 2721
Ion Ratio Lower Upper
43 100
58 26.6 0.0 60.2

Manual Integrations
APPROVED

SAM
10/12/2020 6:08:55 PM

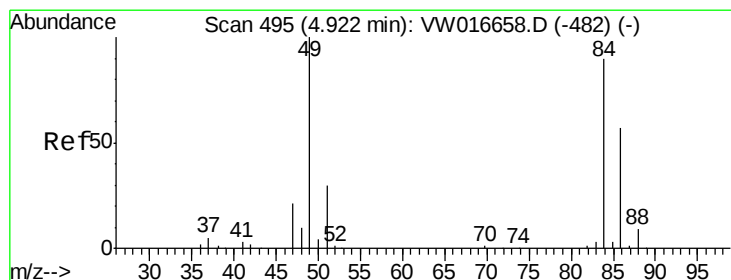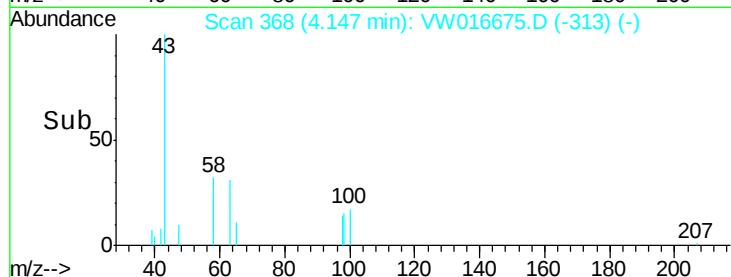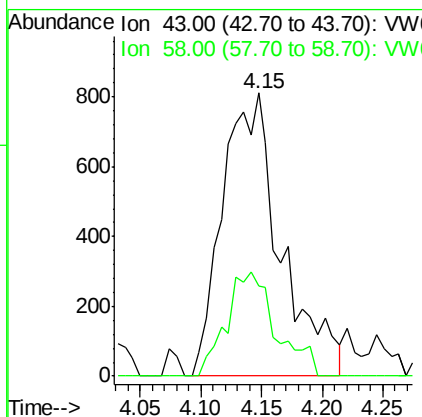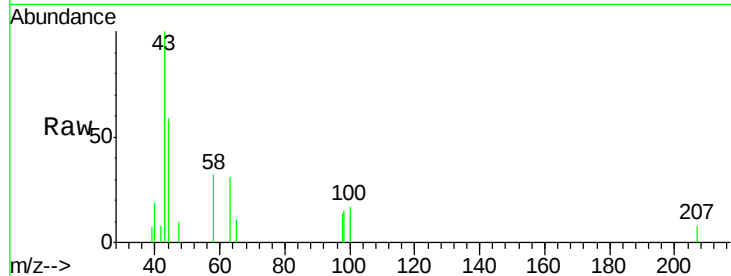

#16
Methylene chloride
Concen: 1.992 ug/L
RT: 4.93 min Scan# 496
Delta R.T. 0.01 min
Lab File: VW016675.D
Acq: 28 Sep 2020 18:05

Tgt Ion: 84 Resp: 28390
Ion Ratio Lower Upper
84 100
49 107.1 76.0 141.2
86 62.8 45.6 84.6

