
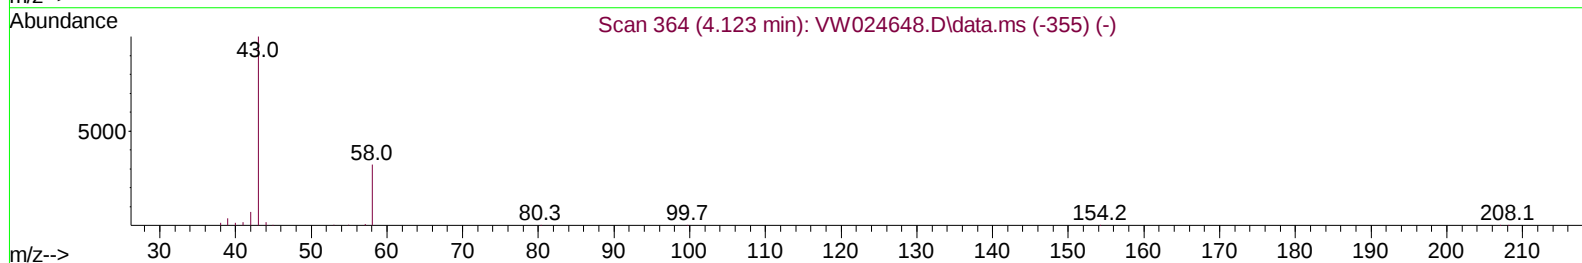
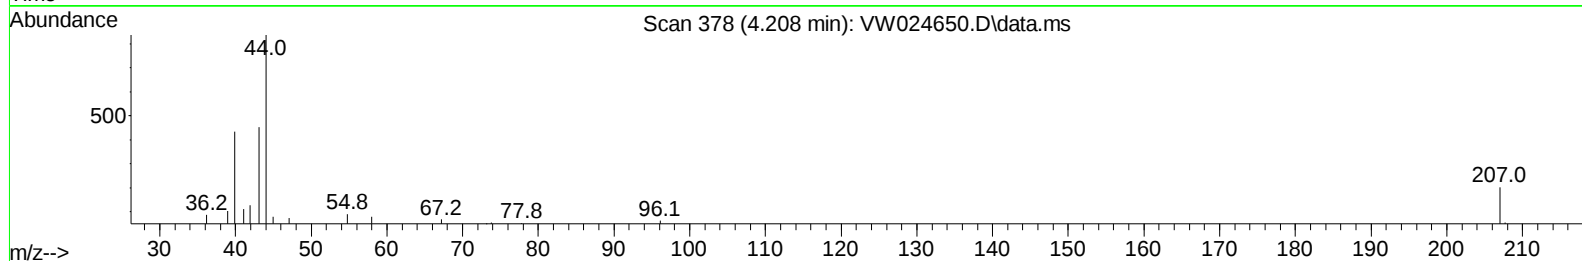


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092822\
Data File : VW024650.D
Acq On : 28 Sep 2022 11:10
Operator : SY/VA
Sample : N4858-01
Misc : 5.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:43:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 29 04:41:43 2022
Response via : Initial Calibration

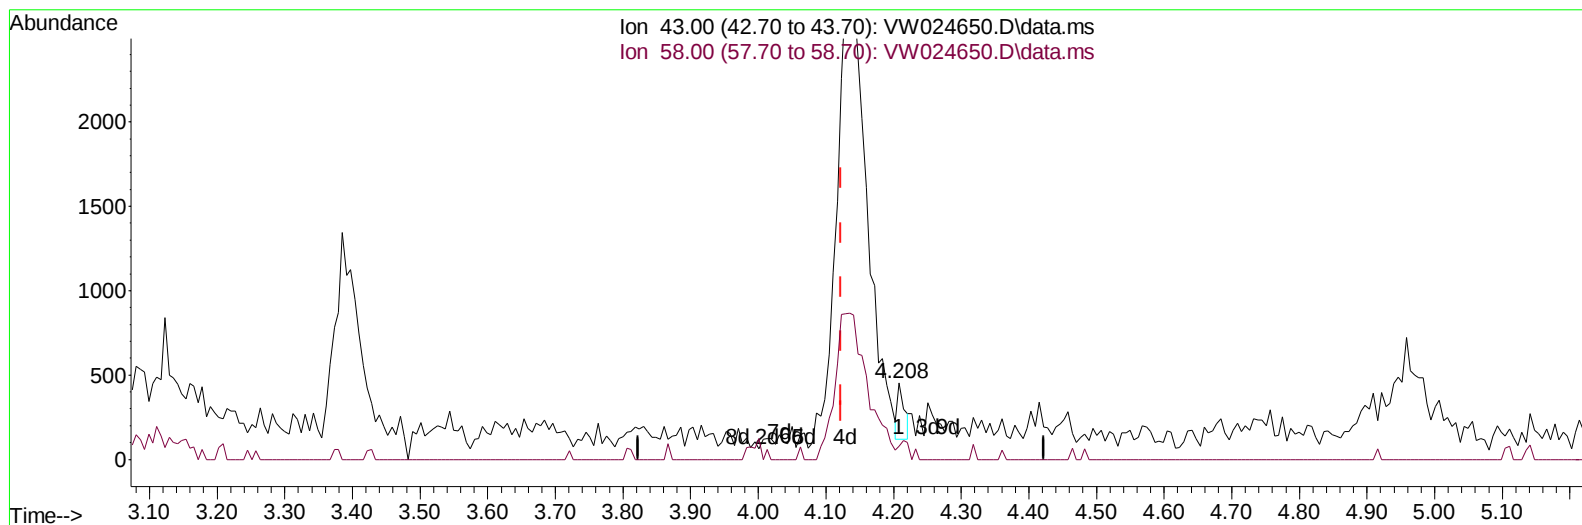

TIC: VW024650.D\data.ms

(13) Acetone (T)




4.208min (+ 0.086) 0.17 ug/L

response 242

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.80	44.63
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092822\
Data File : VW024650.D
Acq On : 28 Sep 2022 11:10
Operator : SY/VA
Sample : N4858-01
Misc : 5.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:43:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 29 04:41:43 2022
Response via : Initial Calibration

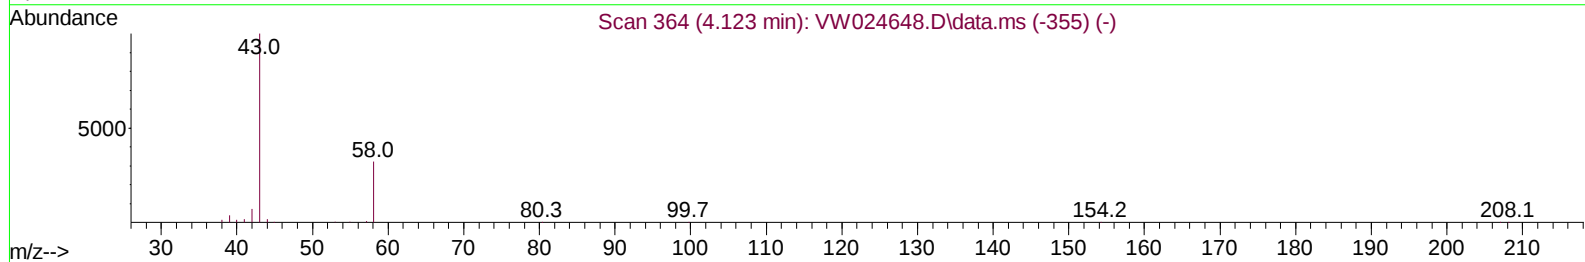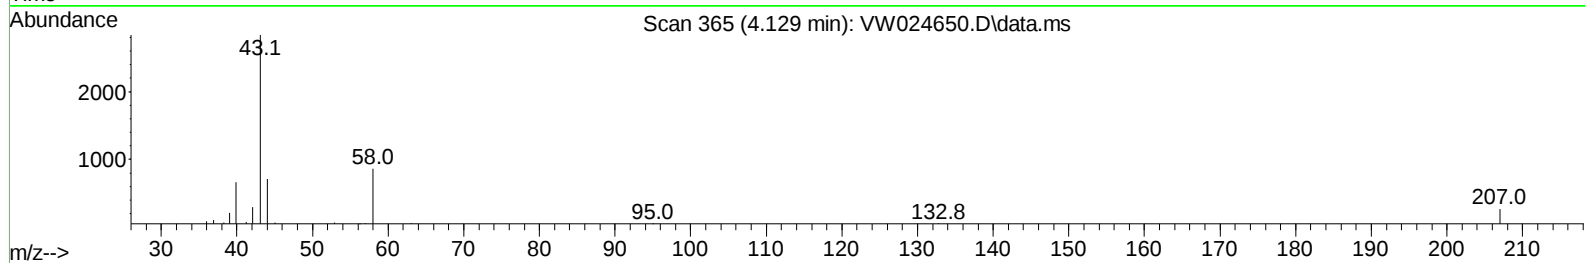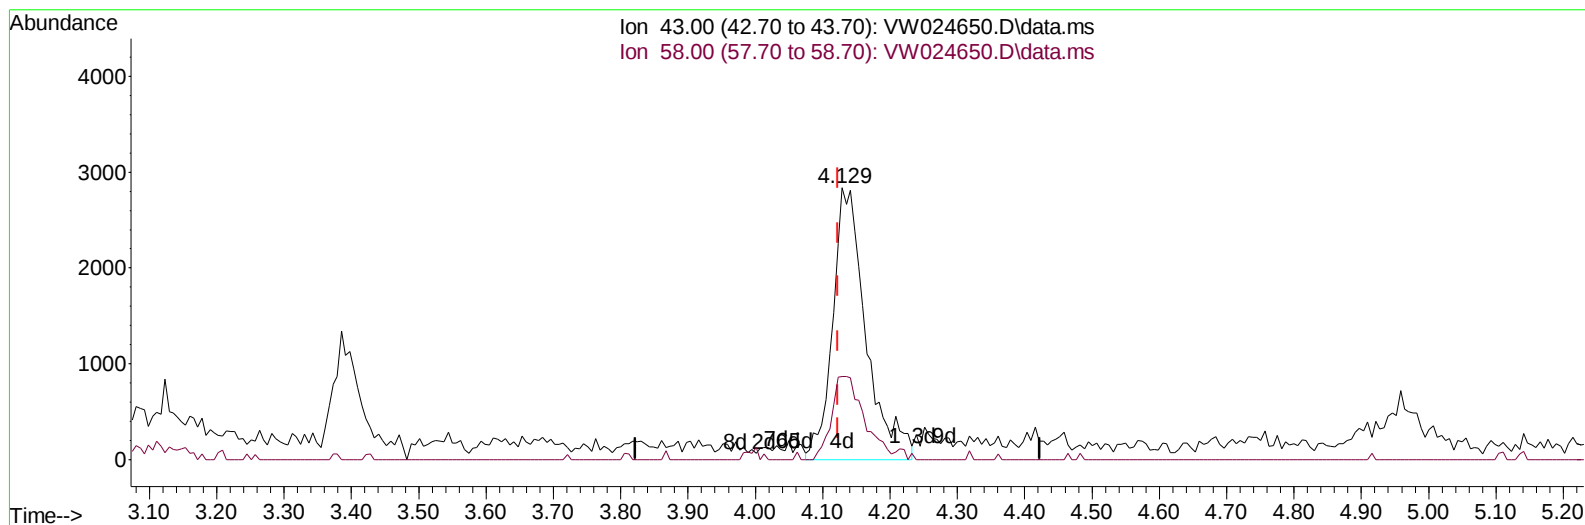

TIC: VW024650.D\data.ms

(13) Acetone (T)




4.129min (+ 0.006) 6.67 ug/L m

response 9719

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.80	1.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092822\
 Data File : VW024650.D
 Acq On : 28 Sep 2022 11:10
 Operator : SY/VA
 Sample : N4858-01
 Misc : 5.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:43:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 29 04:41:43 2022
 Response via : Initial Calibration

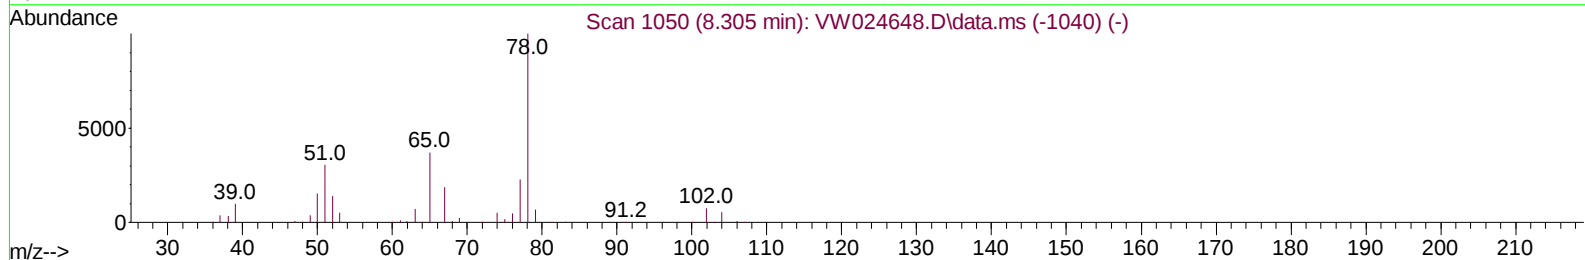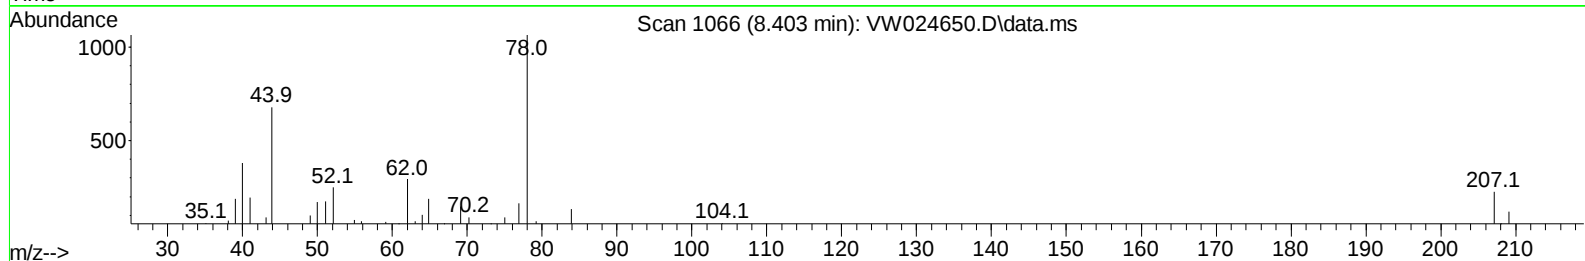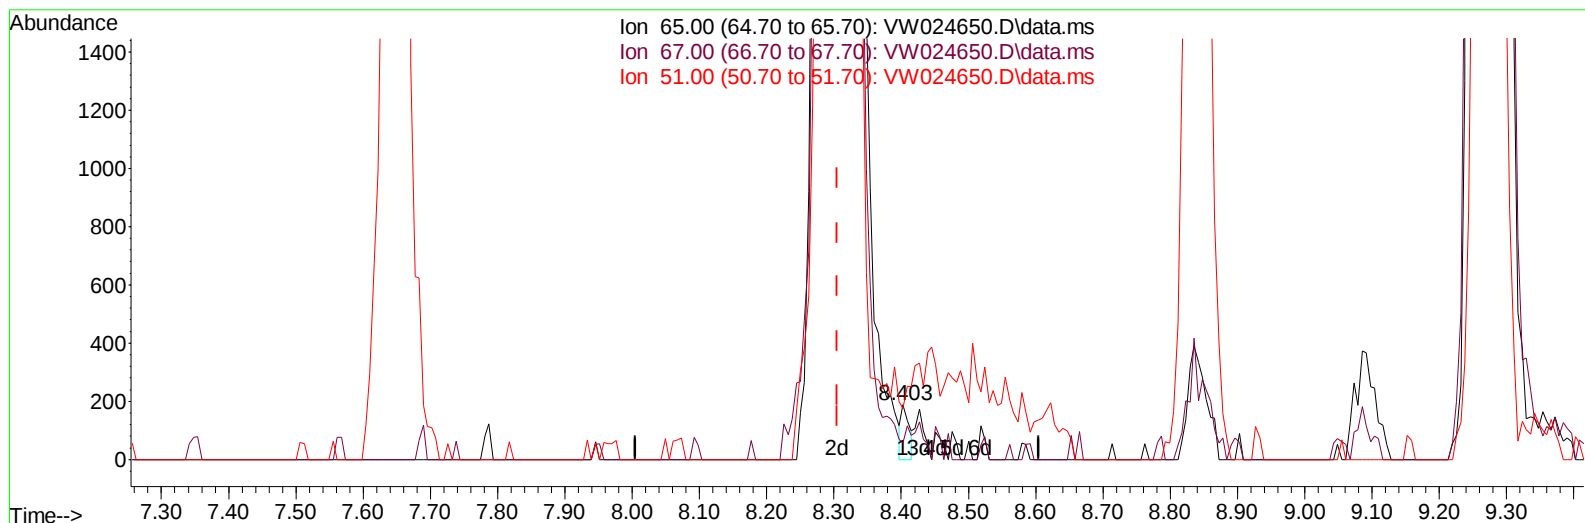

TIC: VW024650.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.403min (+ 0.098) 0.02 ug/L

response 154

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.90	46.75
51.00	118.70	122.08
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092822\
Data File : VW024650.D
Acq On : 28 Sep 2022 11:10
Operator : SY/VA
Sample : N4858-01
Misc : 5.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:43:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 29 04:41:43 2022
Response via : Initial Calibration

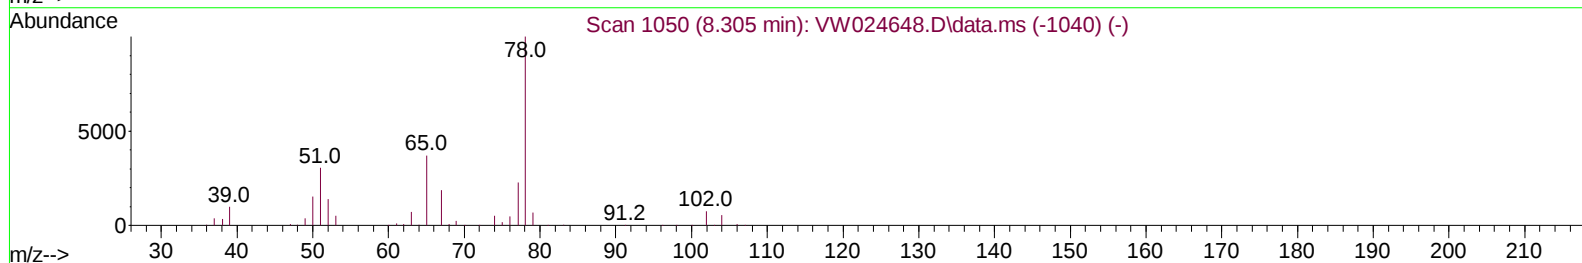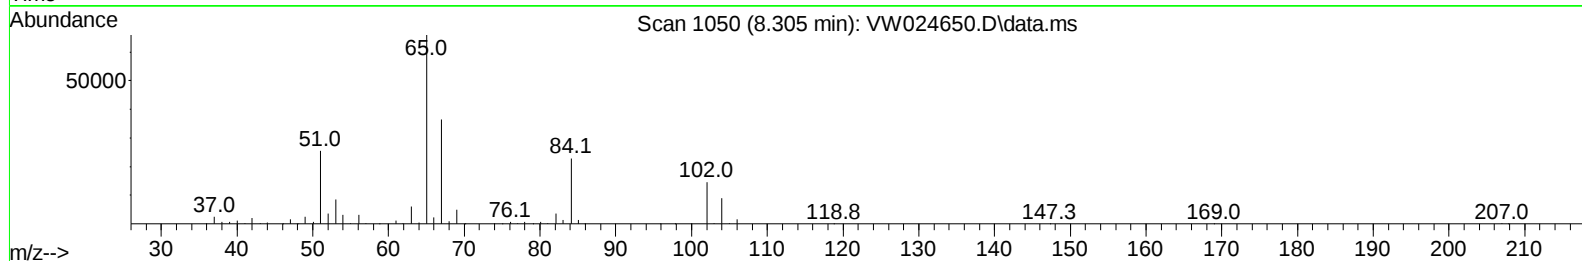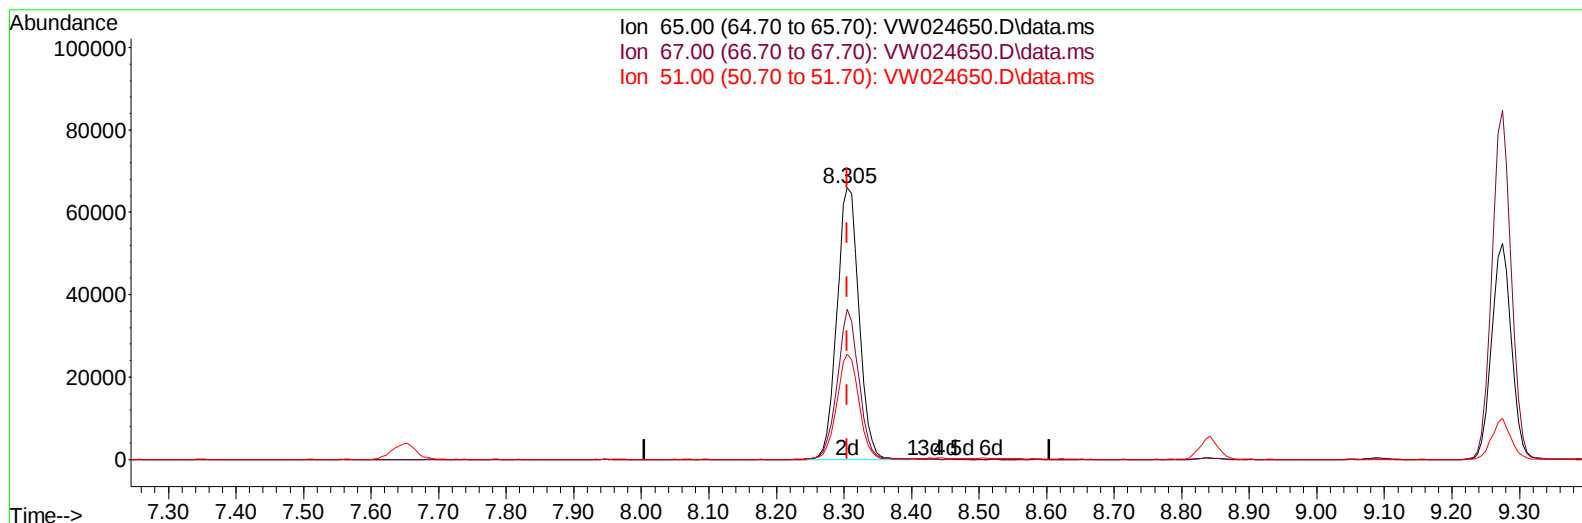

TIC: VW024650.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 20.36 ug/L m

response 149807

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.90	0.05#
51.00	118.70	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092822\
 Data File : VW024650.D
 Acq On : 28 Sep 2022 11:10
 Operator : SY/VA
 Sample : N4858-01
 Misc : 5.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:43:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 29 04:41:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	530679	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	288906	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	54066	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	84395	15.200	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.800%	
7) Chloroethane-d5	2.891	69	55311	17.143	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.560%	
11) 1,1-Dichloroethene-d2	4.019	63	144278	11.227	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	44.920%#	
21) 2-Butanone-d5	7.080	46	130101	65.175	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	130.340%	
24) Chloroform-d	7.647	84	264835	18.667	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	74.680%	
26) 1,2-Dichloroethane-d4	8.305	65	149807m	20.355	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	81.440%	
32) Benzene-d6	8.275	84	481195	26.059	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	104.240%	
36) 1,2-Dichloropropane-d6	9.274	67	168257	29.822	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	119.280%	
41) Toluene-d8	10.323	98	312917	18.960	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.840%	
43) trans-1,3-Dichloroprop...	10.579	79	58085	23.118	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	92.480%	
47) 2-Hexanone-d5	10.921	63	89605	92.824	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	185.640%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85157	21.183	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.720%	
66) 1,2-Dichlorobenzene-d4	13.853	152	30706	16.140	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	64.560%#	
Target Compounds						
					Qvalue	
13) Acetone	4.129	43	9719m	6.673	ug/L	
16) Methylene chloride	4.915	84	77720	7.457	ug/L	95
34) Trichloroethene	9.092	95	38384	7.489	ug/L	94
46) Tetrachloroethene	10.866	164	1348194	387.158	ug/L	94
62) 1,3,5-Trimethylbenzene	12.938	105	3008	0.393	ug/L	90
63) 1,2,4-Trimethylbenzene	13.243	105	8634	1.151	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092822\
Data File : VW024650.D
Acq On : 28 Sep 2022 11:10
Operator : SY/VA
Sample : N4858-01
Misc : 5.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:43:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 29 04:41:43 2022
Response via : Initial Calibration

