

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020234.D
 Acq On : 29 Sep 2021 15:45
 Operator : SY/VA
 Sample : M3973-14
 Misc : 7.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y0

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:18:16 PM

Quant Time: Sep 30 01:04:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 30 00:57:20 2021
 Response via : Initial Calibration

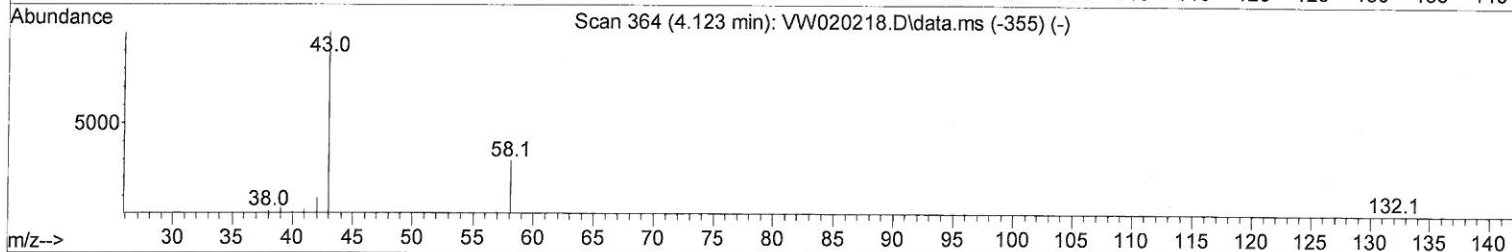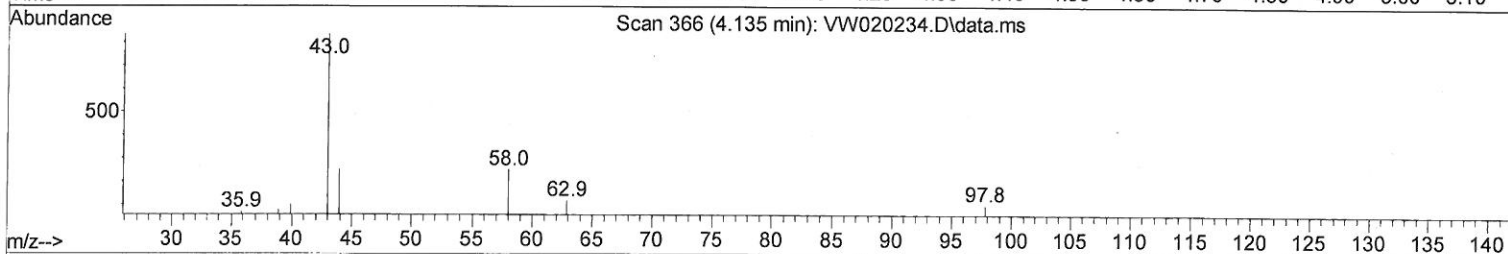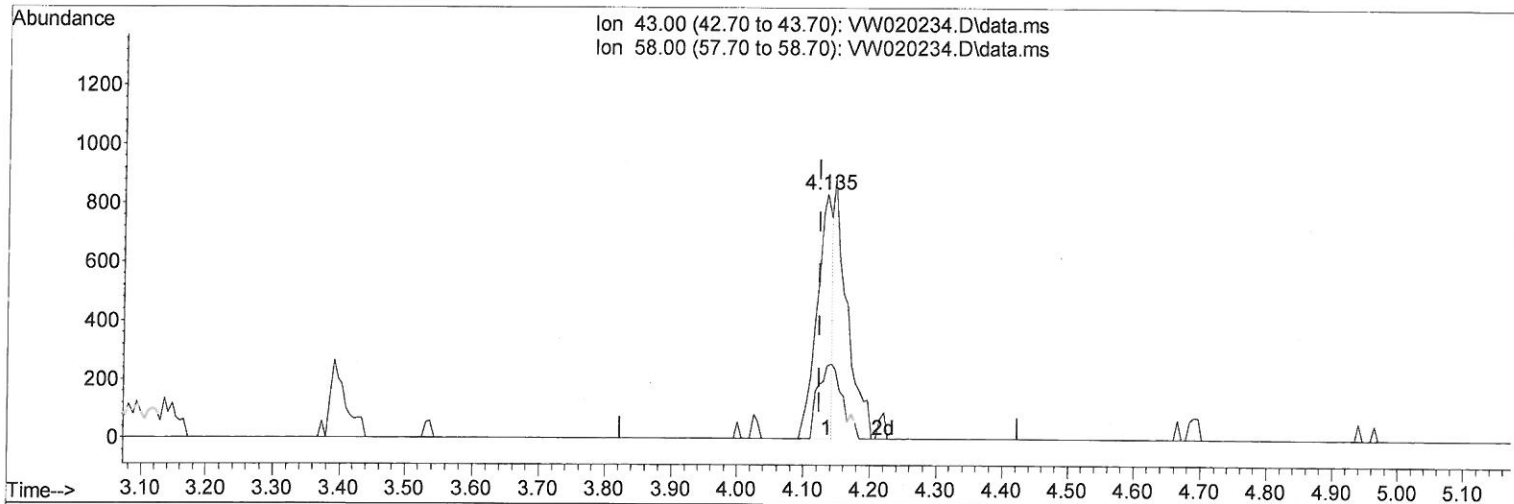

TIC: VW020234.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 2.20 ug/L

response 1353

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.80	44.64
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020234.D
 Acq On : 29 Sep 2021 15:45
 Operator : SY/VA
 Sample : M3973-14
 Misc : 7.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y0

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:18:16 PM

Quant Time: Sep 30 01:04:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 30 00:57:20 2021
 Response via : Initial Calibration

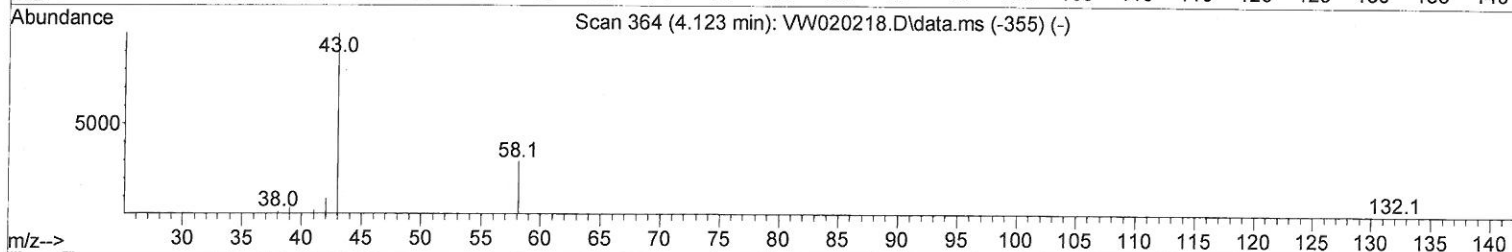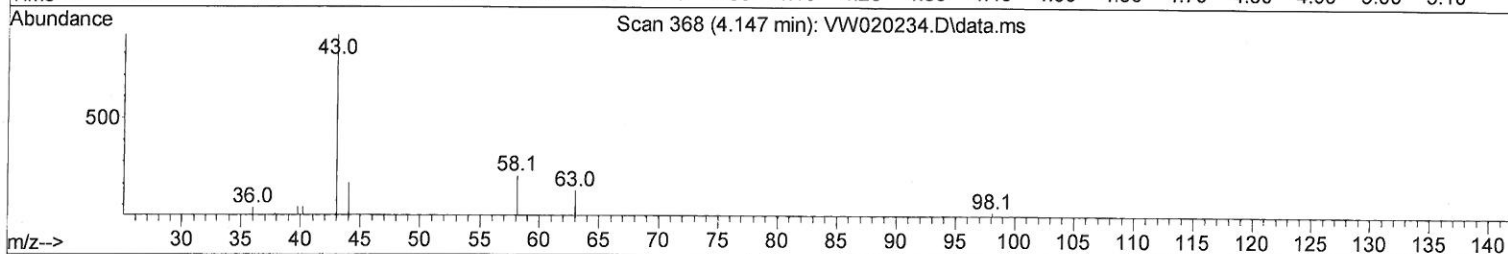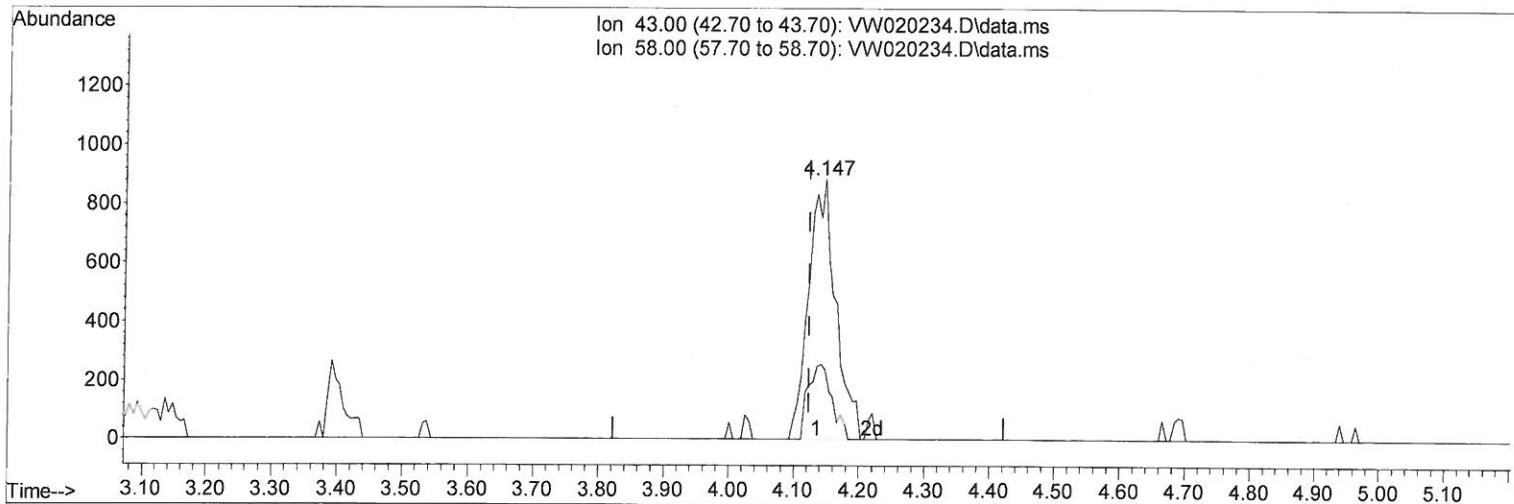

TIC: VW020234.D\data.ms

(13) Acetone (T)

4.147min (+ 0.024) 4.16 ug/L m

response 2565

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.80	23.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020234.D
 Acq On : 29 Sep 2021 15:45
 Operator : SY/VA
 Sample : M3973-14
 Misc : 7.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y0

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:18:16 PM

Quant Time: Sep 30 01:04:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 Qlast Update : Thu Sep 30 00:57:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	227791	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	119984	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	13503	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	109038	23.398	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	93.600%	
7) Chloroethane-d5	2.898	69	93559	26.650	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	106.600%	
11) 1,1-Dichloroethene-d2	4.025	63	110676	15.169	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	60.680%	
21) 2-Butanone-d5	7.080	46	28289	39.339	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	78.680%	
24) Chloroform-d	7.653	84	167400	23.367	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	93.480%	
26) 1,2-Dichloroethane-d4	8.311	65	84735	21.977	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	87.920%	
32) Benzene-d6	8.281	84	286449	37.421	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	149.680%#	
36) 1,2-Dichloropropane-d6	9.274	67	87280	39.398	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	157.600%#	
41) Toluene-d8	10.329	98	182006	26.131	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	104.520%	
43) trans-1,3-Dichloroprop...	10.579	79	22416	23.674	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	94.680%	
47) 2-Hexanone-d5	10.927	63	17261	56.303	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	112.600%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	48730	28.516	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	114.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	14927	29.481	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	117.920%	
Target Compounds						
13) Acetone	4.147	43	2565m	4.165	ug/L	Qvalue 10/04/21 Sy
34) Trichloroethene	9.098	95	3338	1.722	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
Data File : VW020234.D
Acq On : 29 Sep 2021 15:45
Operator : SY/VA
Sample : M3973-14
Misc : 7.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8Y0

Manual Integrations
APPROVED

MMDadoda
10/4/2021 3:18:16 PM

Quant Time: Sep 30 01:04:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 30 00:57:20 2021
Response via : Initial Calibration

