

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020247.D
 Acq On : 29 Sep 2021 22:31
 Operator : SY/VA
 Sample : M3973-17
 Misc : 8.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y3

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:19:43 PM

Quant Time: Sep 30 02:11:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 30 02:06:51 2021
 Response via : Initial Calibration

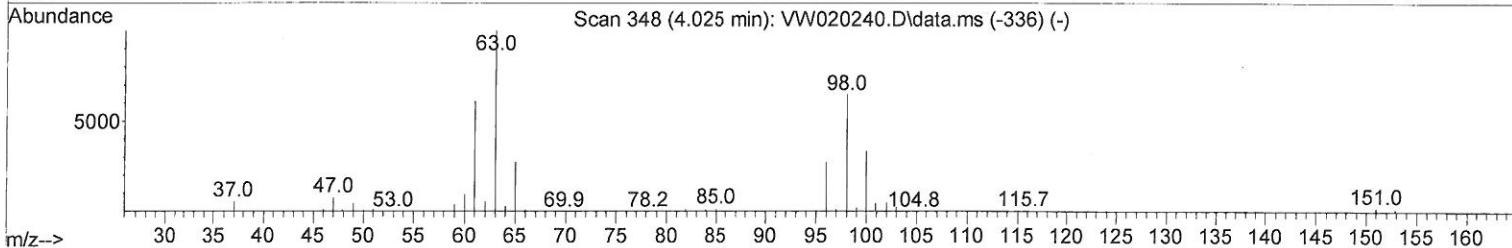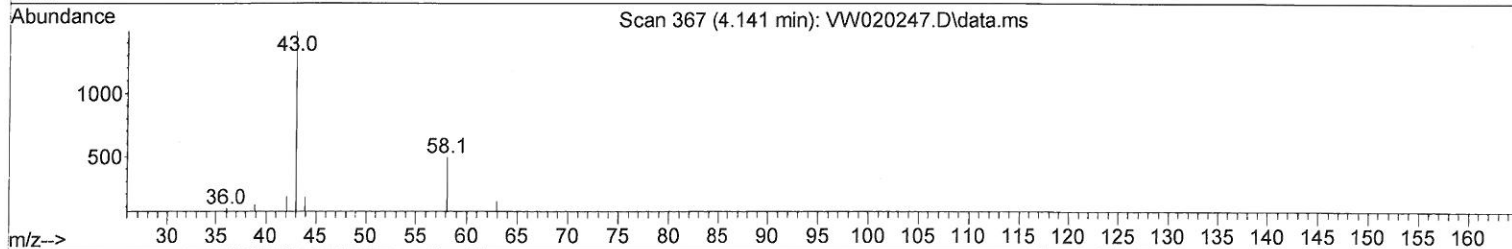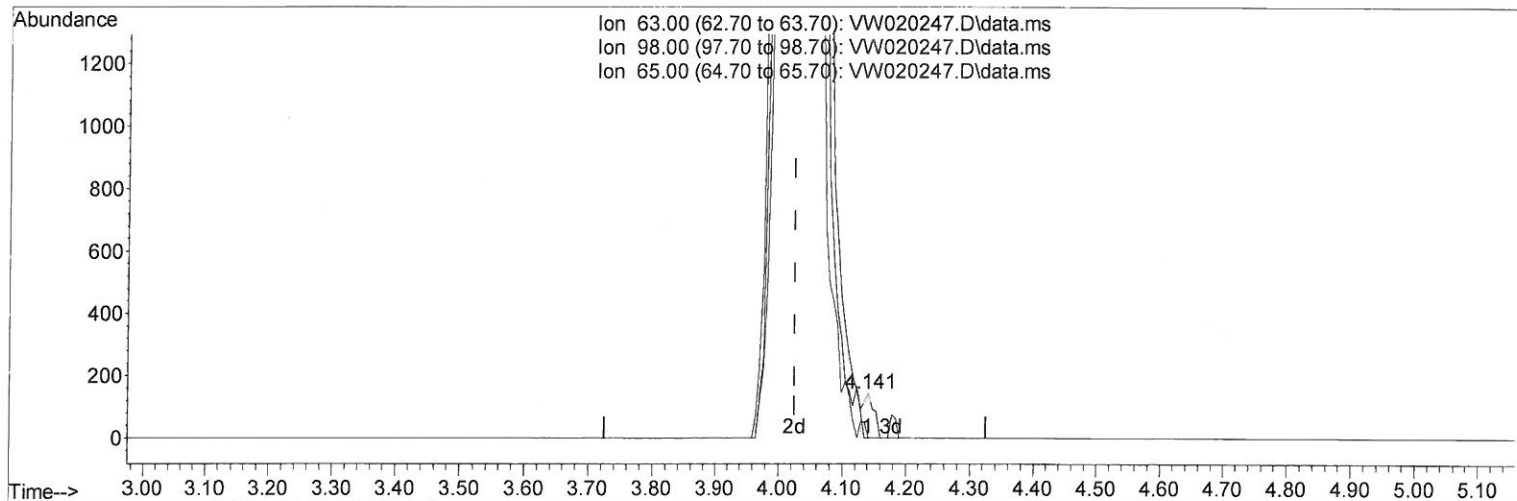

TIC: VW020247.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.141min (+ 0.116) 0.02 ug/L

response 160

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.60	56.88
65.00	23.90	23.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020247.D
 Acq On : 29 Sep 2021 22:31
 Operator : SY/VA
 Sample : M3973-17
 Misc : 8.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y3

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:19:43 PM

Quant Time: Sep 30 02:11:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 30 02:06:51 2021
 Response via : Initial Calibration

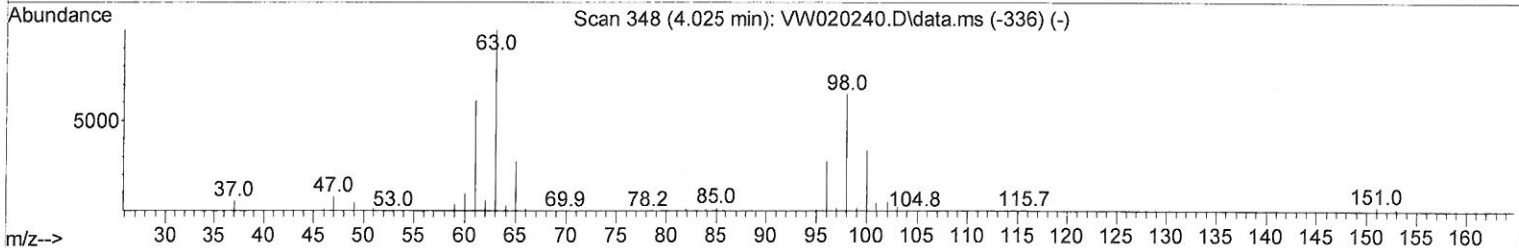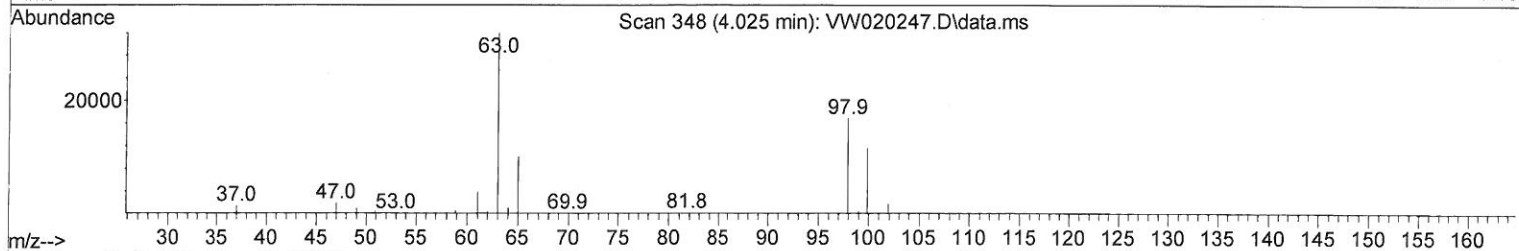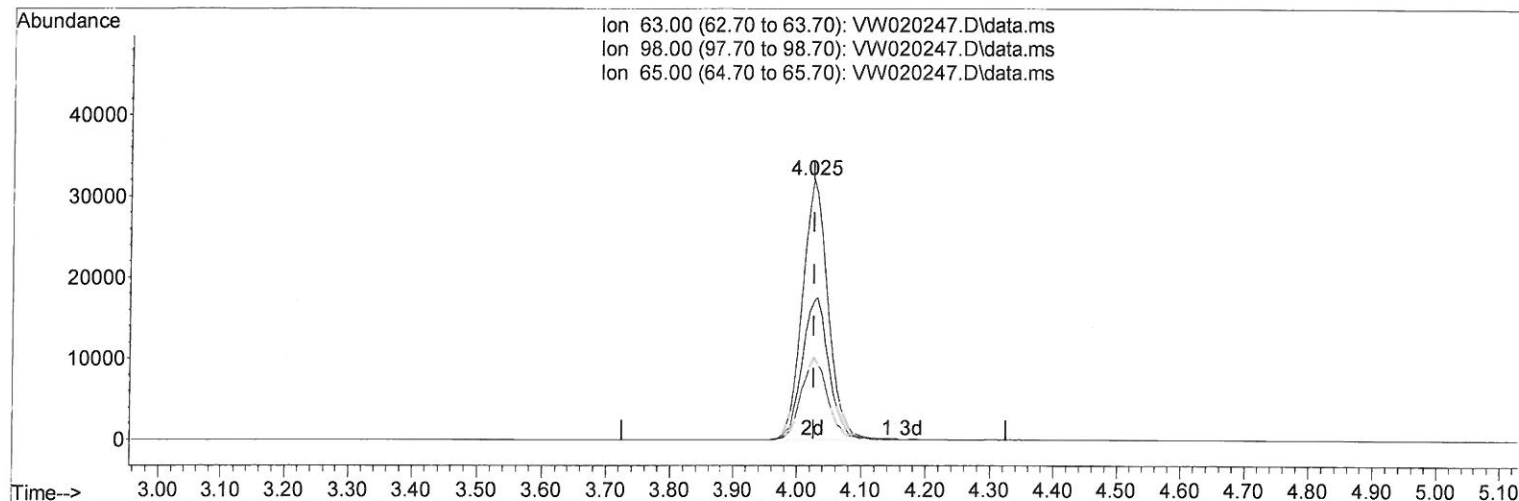

TIC: VW020247.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.025min (-0.000) 13.00 ug/L m

response 88913

Ion	Exp%	Act%
-----	------	------

63.00	100.00	100.00
-------	--------	--------

98.00	70.60	0.10#
-------	-------	-------

65.00	23.90	0.04#
-------	-------	-------

0.00	0.00	0.00
------	------	------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020247.D
 Acq On : 29 Sep 2021 22:31
 Operator : SY/VA
 Sample : M3973-17
 Misc : 8.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y3

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:19:43 PM

Quant Time: Sep 30 02:11:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 30 02:06:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	213463	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	159131	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	29893	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	88353	20.232	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.920%		
7) Chloroethane-d5	2.904	69	79346	24.119	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.480%		
11) 1,1-Dichloroethene-d2	4.025	63	88913m	13.004	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.000%		
21) 2-Butanone-d5	7.080	46	24859	36.889	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	73.780%		
24) Chloroform-d	7.653	84	147263	21.936	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.760%		
26) 1,2-Dichloroethane-d4	8.311	65	76157	21.078	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.320%		
32) Benzene-d6	8.281	84	254782	25.096	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	100.400%		
36) 1,2-Dichloropropane-d6	9.281	67	80016	27.234	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.920%		
41) Toluene-d8	10.329	98	188618	20.419	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.680%		
43) trans-1,3-Dichloroprop...	10.579	79	25718	20.479	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.920%		
47) 2-Hexanone-d5	10.927	63	17578	43.232	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.460%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	51294	22.633	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	90.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	30123	26.874	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.480%		
Target Compounds						
13) Acetone	4.135	43	4775	8.273	ug/L	98
34) Trichloroethene	9.092	95	3461	1.346	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

10/04/21 6y

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
Data File : VW020247.D
Acq On : 29 Sep 2021 22:31
Operator : SY/VA
Sample : M3973-17
Misc : 8.10g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8Y3

Manual Integrations
APPROVED

MMDadoda
10/4/2021 3:19:43 PM

Quant Time: Sep 30 02:11:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 30 02:06:51 2021
Response via : Initial Calibration

