

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020251.D
 Acq On : 30 Sep 2021 00:19
 Operator : SY/VA
 Sample : M3974-02
 Misc : 7.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Y8

Quant Time: Sep 30 02:12:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 30 02:06:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	289979	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	211216	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	62010	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	106092	17.884	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.520%
7) Chloroethane-d5	2.897	69	89146	19.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.800%
11) 1,1-Dichloroethene-d2	4.025	63	127326	13.708	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.840%
21) 2-Butanone-d5	7.086	46	32479	35.479	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.960%
24) Chloroform-d	7.653	84	169803	18.619	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.480%
26) 1,2-Dichloroethane-d4	8.311	65	87011	17.727	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	70.920%
32) Benzene-d6	8.280	84	316191	23.465	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.840%
36) 1,2-Dichloropropane-d6	9.280	67	93511	23.978	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.920%
41) Toluene-d8	10.329	98	263093	21.458	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.840%
43) trans-1,3-Dichloroprop...	10.579	79	32757	19.652	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.600%
47) 2-Hexanone-d5	10.926	63	29838	55.288	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.580%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	62008	20.613	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	55856	24.022	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.080%
Target Compounds					Qvalue	
13) Acetone	4.123	43	5949	7.588	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
Data File : VW020251.D
Acq On : 30 Sep 2021 00:19
Operator : SY/VA
Sample : M3974-02
Misc : 7.10g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8Y8

Quant Time: Sep 30 02:12:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 30 02:06:51 2021
Response via : Initial Calibration

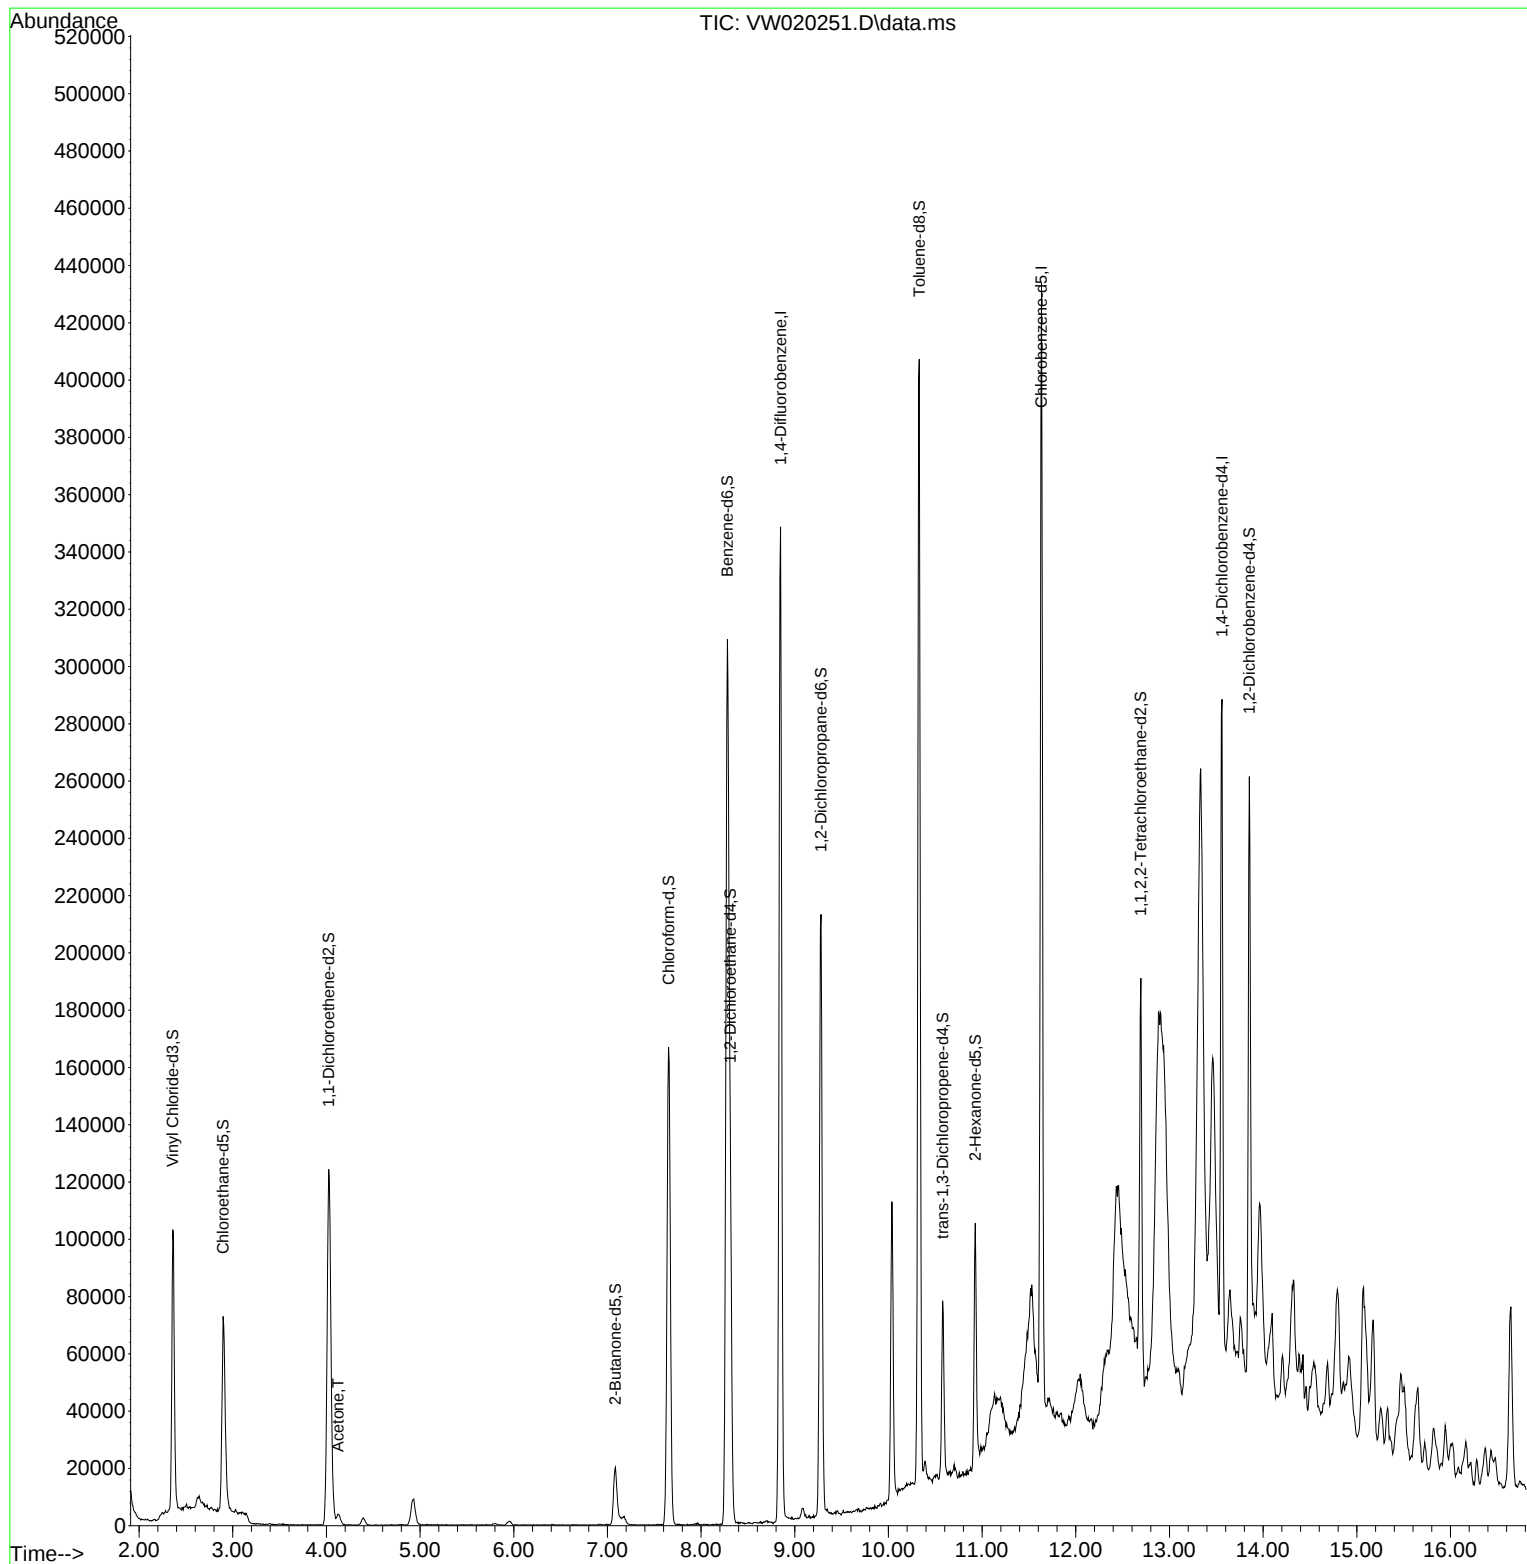

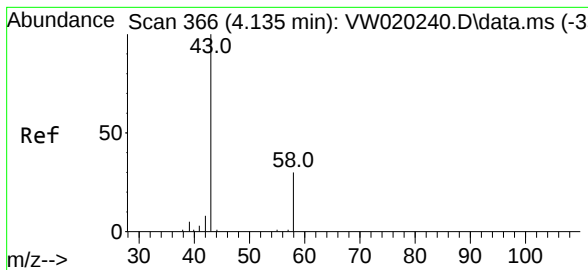

#13

Acetone

Concen: 7.588 ug/L

RT: 4.123 min Scan# 364

Delta R.T. -0.013 min

Lab File: VW020251.D




Acq: 30 Sep 2021 00:19

Tgt Ion: 43 Resp: 5949

Ion Ratio Lower Upper

43 100

58 31.3 0.0 61.6

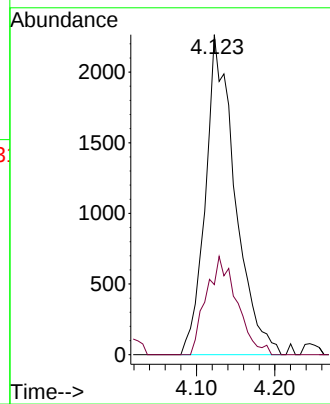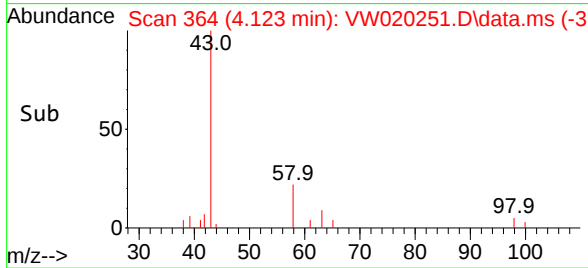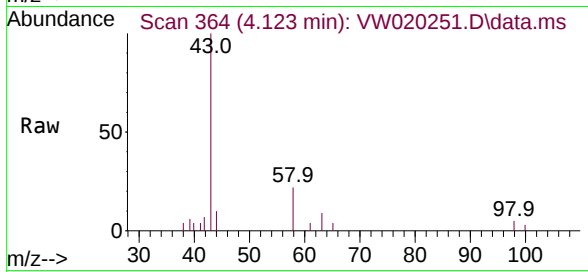

Instrument :
MSVOA_W
ClientSampleId :
EW8Y8