
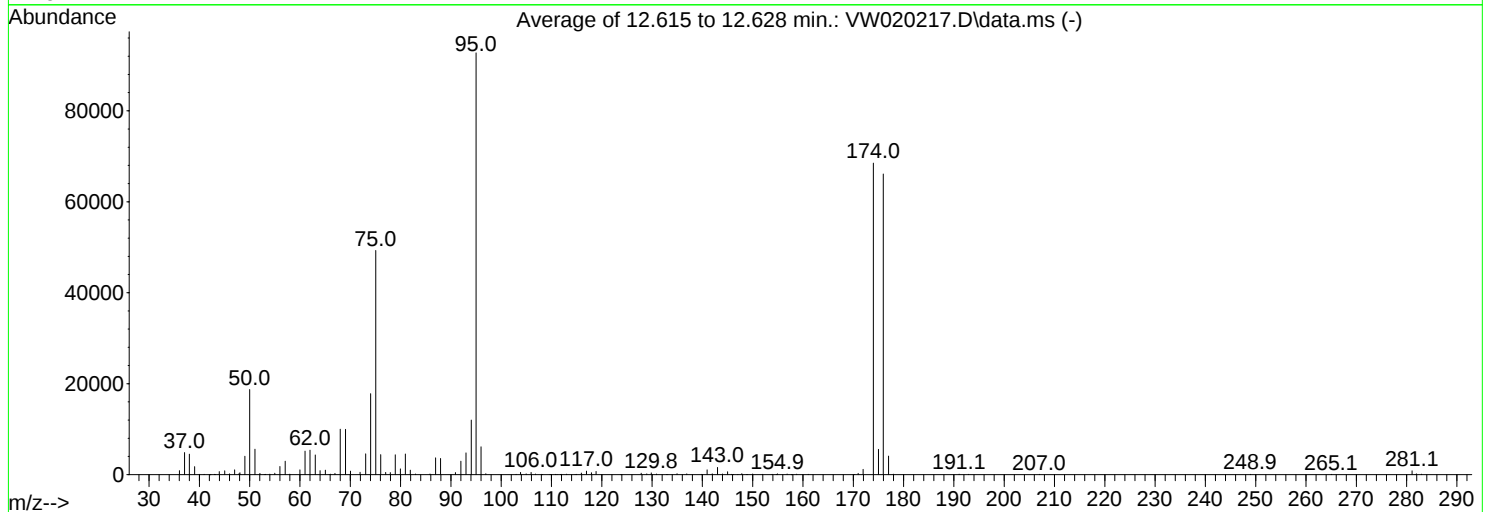


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092921\
 Data File : VW020217.D
 Acq On : 29 Sep 2021 07:48
 Operator : SY/VA
 Sample : BFB442
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB442

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Title : SFAM01.0
 Last Update : Fri Oct 01 01:03:15 2021

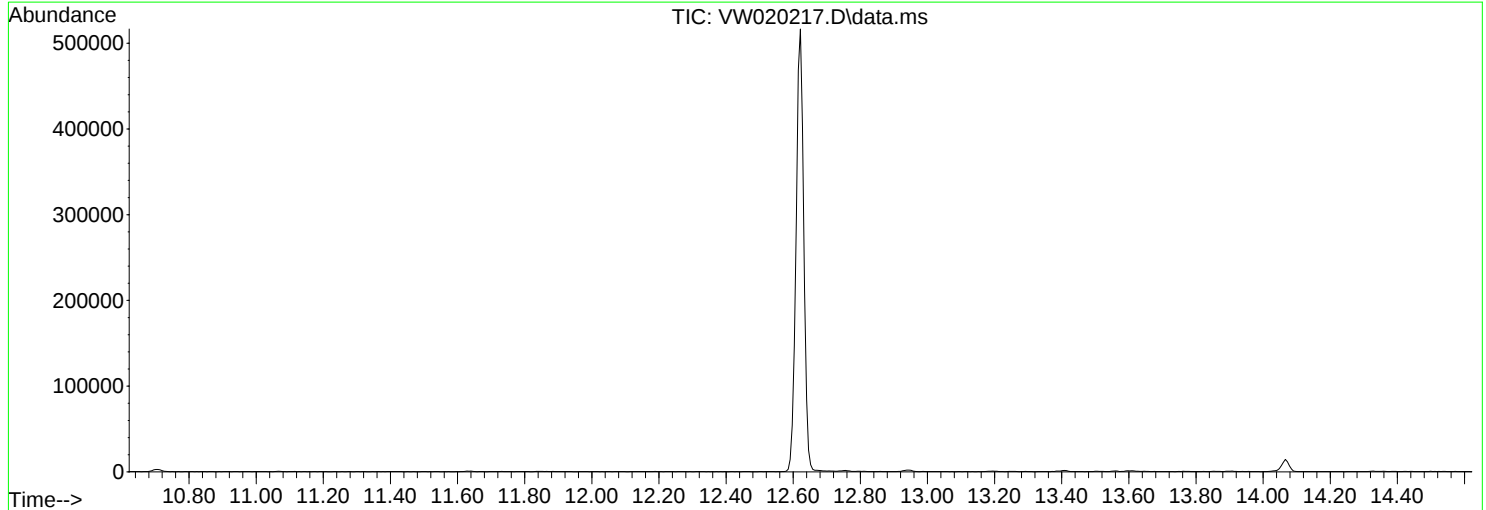

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	18728	PASS
75	95	30	80	53.1	49293	PASS
95	95	100	100	100.0	92749	PASS
96	95	5	9	6.6	6113	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	68491	PASS
175	174	5	9	8.1	5558	PASS
176	174	95	105	96.5	66123	PASS
177	176	5	10	6.2	4091	PASS

m/z	Abundance
40.00	140.0
43.90	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442

m/z	Abundance
36.10	1006.0
37.10	5099.0
38.00	5219.0
39.10	1967.0
40.10	224.0
41.00	81.0
42.10	52.0
43.00	113.0
44.00	915.0
45.00	932.0
46.00	232.0
47.00	1062.0
47.90	742.0
49.00	4505.0
50.00	19696.0
51.00	6038.0
52.10	316.0
52.90	157.0
54.10	116.0
54.90	341.0
56.00	1916.0
57.00	3124.0
58.10	82.0
60.00	1147.0
61.00	5597.0
62.00	5558.0
63.00	4782.0
64.00	1084.0
65.00	1002.0
66.10	173.0
66.90	287.0
68.00	10365.0
69.10	9867.0
70.10	818.0
72.00	578.0
73.10	4487.0
74.00	18728.0
75.00	51024.0
76.00	5023.0
77.10	605.0
78.00	407.0
79.00	4709.0
80.00	1466.0
80.90	4576.0
82.00	1064.0
83.00	109.0
85.80	133.0
86.90	3840.0
87.90	3540.0
91.00	532.0
92.00	3019.0
93.00	5087.0
94.00	12354.0
95.00	93928.0
96.00	6322.0
97.00	217.0
102.90	108.0
103.90	555.0
105.10	154.0
106.00	519.0
106.80	139.0
108.00	97.0
109.70	65.0
111.10	135.0
111.80	99.0
113.00	124.0
114.70	82.0
115.90	315.0
116.90	947.0
118.00	345.0
118.90	694.0
127.90	398.0
129.00	163.0
129.90	333.0
130.80	146.0
132.90	146.0
135.10	191.0
136.90	164.0
141.00	1044.0
141.90	152.0
143.00	1742.0
144.00	197.0
145.00	763.0
146.20	118.0
148.00	166.0
148.80	63.0
150.10	80.0
152.00	70.0
153.80	61.0
154.70	236.0
156.80	124.0
158.80	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442

161.00	59.0
170.20	59.0
171.00	291.0
171.90	1040.0
174.00	66520.0
175.00	5461.0
176.00	61008.0
177.00	3919.0
178.00	113.0
191.00	122.0
192.90	206.0
207.10	121.0
248.90	124.0
265.00	142.0
281.10	1502.0
282.00	351.0
282.90	248.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442

m/z	Abundance
36.00	916.0
37.00	5708.0
38.00	5071.0
39.00	2071.0
40.00	255.0
40.90	120.0
43.20	86.0
44.00	838.0
45.10	907.0
46.00	188.0
47.00	1169.0
48.10	780.0
49.00	4518.0
50.00	21384.0
51.10	6384.0
52.10	304.0
53.20	162.0
54.00	97.0
55.00	308.0
56.00	2207.0
57.10	3252.0
58.00	100.0
60.00	1248.0
61.00	5753.0
62.00	5929.0
63.10	4822.0
64.10	941.0
65.00	1075.0
66.10	159.0
67.00	410.0
68.00	11543.0
69.00	11566.0
70.00	885.0
71.90	534.0
73.00	5385.0
74.00	20248.0
75.10	55168.0
76.10	4653.0
77.10	474.0
77.80	362.0
78.10	364.0
78.90	4836.0
80.00	1320.0
81.00	4966.0
81.90	1044.0
83.00	141.0
85.90	148.0
87.00	4200.0
87.90	4106.0
90.80	535.0
92.00	3298.0
93.00	5353.0
94.00	13724.0
95.00	105576.0
96.00	7050.0
96.90	282.0
103.00	74.0
103.90	557.0
104.90	183.0
105.90	537.0
106.90	116.0
108.20	61.0
109.90	59.0
110.80	182.0
112.00	140.0
113.00	112.0
115.00	122.0
116.00	366.0
117.00	849.0
117.90	524.0
118.80	772.0
127.90	316.0
128.90	201.0
129.80	507.0
130.90	127.0
133.10	122.0
134.90	215.0
136.90	169.0
139.90	114.0
141.00	1139.0
142.00	200.0
143.00	1636.0
144.00	163.0
145.00	710.0
145.90	137.0
147.00	67.0
147.80	252.0
149.00	121.0
150.00	174.0
151.90	101.0
153.80	56.0
154.90	278.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442

156.80	156.0
158.70	85.0
161.10	70.0
170.90	325.0
172.00	1536.0
174.00	71656.0
175.00	6017.0
176.00	74336.0
177.00	4614.0
177.90	128.0
191.10	92.0
192.90	50.0
206.90	85.0
249.00	101.0
265.10	65.0
281.10	633.0
281.80	186.0
283.00	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442

m/z	Abundance
36.00	718.0
37.00	3766.0
38.00	3228.0
39.00	1288.0
39.90	169.0
43.00	61.0
44.00	719.0
45.10	645.0
45.90	127.0
47.00	919.0
48.00	496.0
49.10	3094.0
50.00	15104.0
51.00	4367.0
52.00	235.0
53.10	108.0
53.90	90.0
55.10	326.0
56.00	1297.0
57.00	2538.0
57.90	115.0
60.10	732.0
61.00	4119.0
62.00	4623.0
63.00	3371.0
63.90	653.0
65.10	898.0
65.80	92.0
67.00	205.0
68.00	8117.0
69.00	8452.0
70.10	615.0
72.00	477.0
73.00	3844.0
74.10	14394.0
75.00	41688.0
76.10	3493.0
76.90	415.0
78.00	275.0
79.00	3502.0
79.90	1055.0
80.90	4044.0
82.00	830.0
83.00	147.0
85.90	119.0
86.90	3058.0
88.00	2987.0
90.90	307.0
92.00	2564.0
93.00	3893.0
94.10	9885.0
95.00	78744.0
96.00	4966.0
97.00	161.0
103.00	67.0
103.80	395.0
104.90	155.0
106.00	455.0
106.80	139.0
108.00	102.0
109.70	78.0
110.80	68.0
111.90	93.0
113.10	69.0
114.90	89.0
115.90	380.0
117.00	574.0
118.00	375.0
118.90	611.0
123.80	50.0
127.70	221.0
128.90	172.0
129.90	332.0
131.00	111.0
134.90	205.0
136.90	215.0
139.90	85.0
140.90	964.0
142.00	135.0
143.00	1400.0
143.90	77.0
145.00	416.0
145.80	123.0
147.10	52.0
147.80	245.0
149.90	133.0
151.80	51.0
153.90	88.0
155.00	212.0
156.90	180.0
157.70	58.0
158.70	123.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442

161.00	102.0
171.00	287.0
172.00	901.0
174.00	67296.0
175.00	5196.0
175.90	63024.0
177.00	3739.0
178.00	107.0
191.10	63.0
281.00	393.0
281.70	77.0

Instrument :
MSVOA_W
ClientSampleId :
BFB442