

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW093020\
 Data File : VW016710.D
 Acq On : 30 Sep 2020 14:28
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Manual Integrations
 APPROVED

MMDadoda
 10/5/2020 4:10:16 PM

Quant Time: Oct 01 06:05:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 01 05:05:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	579318	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	519528	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	260046	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	83742	14.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.72%
7) Chloroethane-d5	2.90	69	78927	17.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.96%
10) 1,1-Dichloroethene-d2	4.03	63	147330	11.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.00%
20) 2-Butanone-d5	7.09	46	65501	42.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.68%
24) Chloroform-d	7.65	84	281152	23.20	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.80%
26) 1,2-Dichloroethane-d4	8.31	65	145727	23.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.68%
29) Benzene-d6	8.28	84	487046	20.90	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.60%
33) 1,2-Dichloropropane-d6	9.28	67	144243	22.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.36%
37) Toluene-d8	10.33	98	443905	19.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.48%
38) trans-1,3-Dichloropropene-	10.58	79	62211	19.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.16%
39) 2-Hexanone-d5	10.93	63	51225	44.60	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.20%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128097	23.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	203129	24.45	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.80%

Target Compounds					Ovalue
13) Acetone	4.14	43	2920m	2.438 ug/L	
16) Methylene chloride	4.93	84	16103	1.802 ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW093020\
Data File : VW016710.D
Acq On : 30 Sep 2020 14:28
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Manual Integrations
APPROVED

MMDadoda
10/5/2020 4:10:16 PM

Quant Time: Oct 01 06:05:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 01 05:05:13 2020
Response via : Initial Calibration

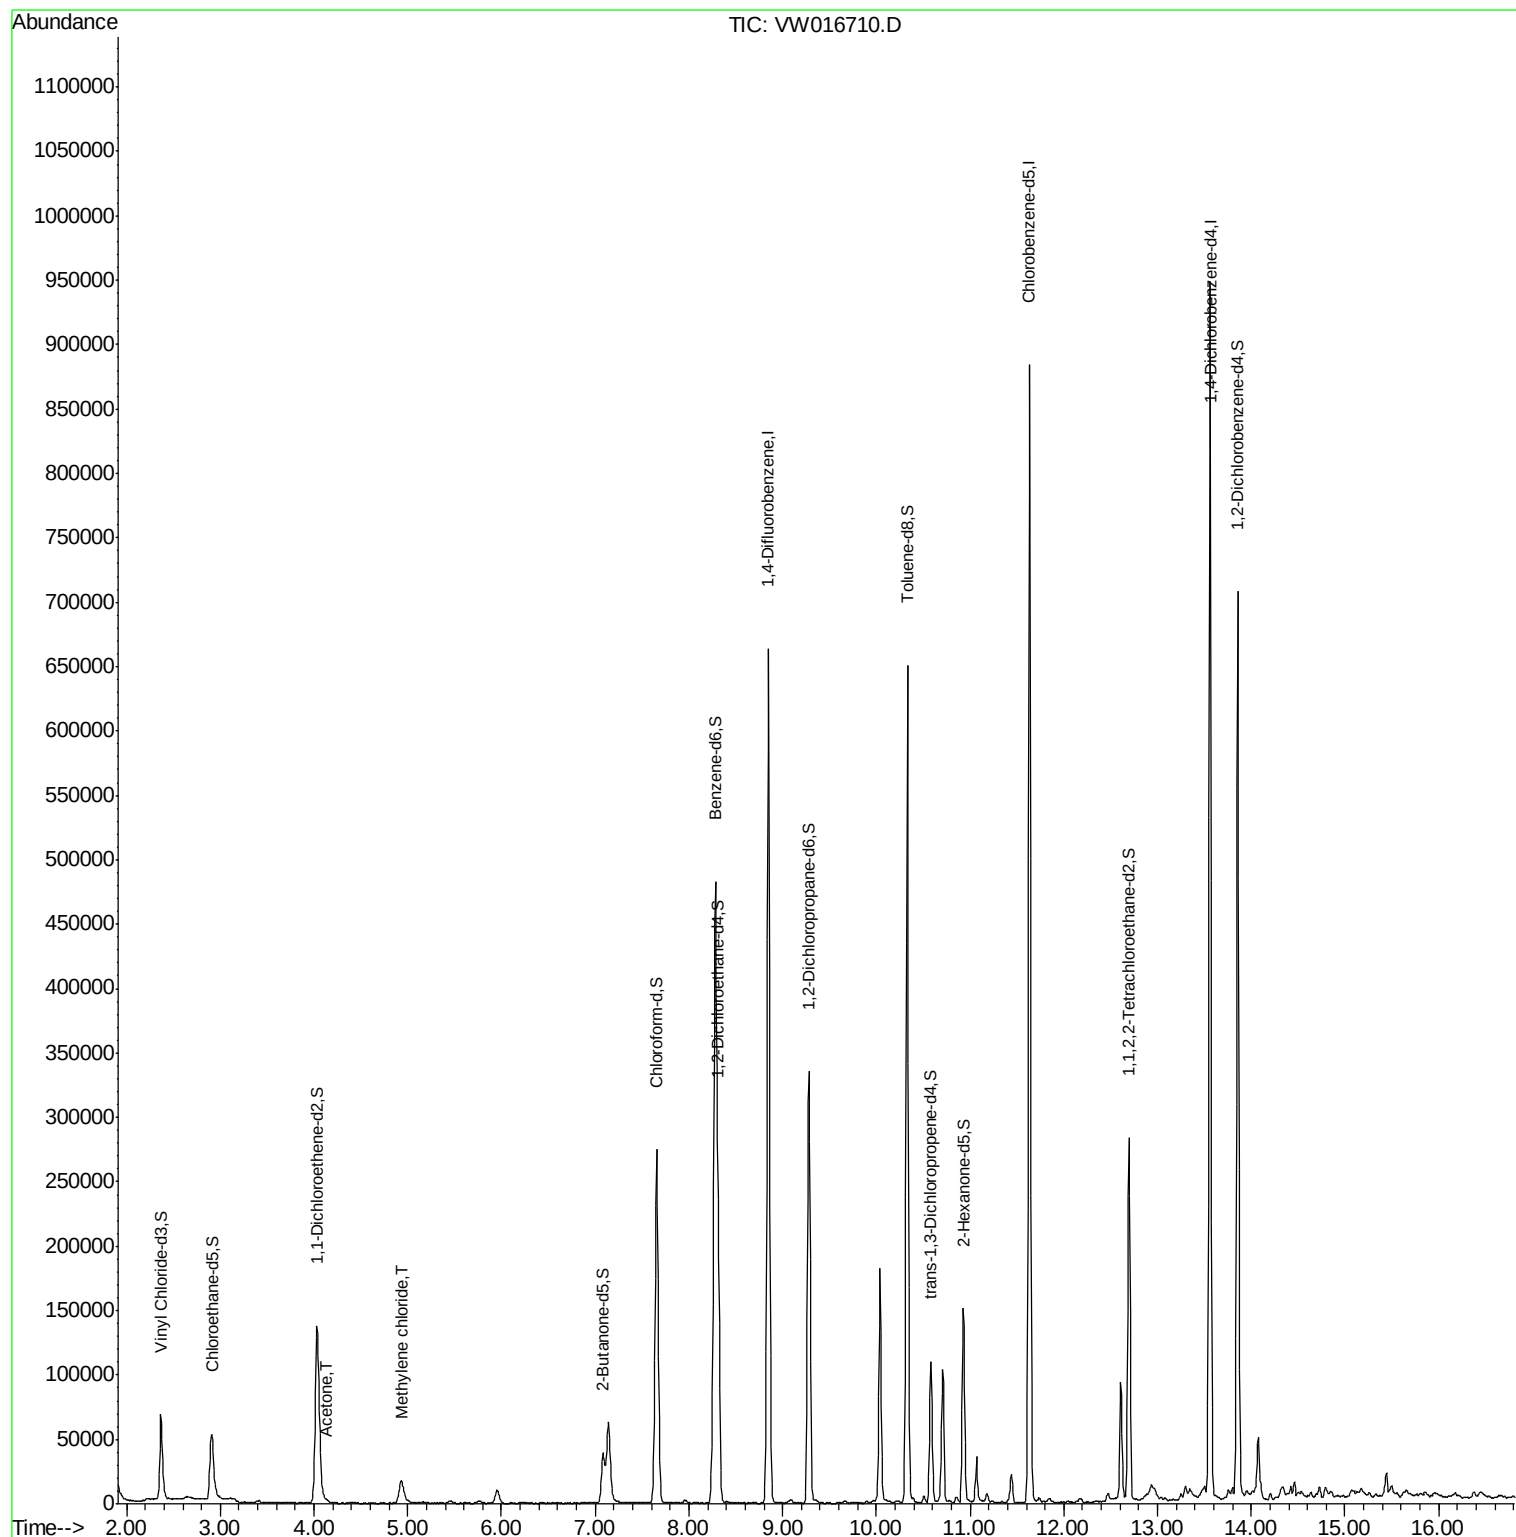

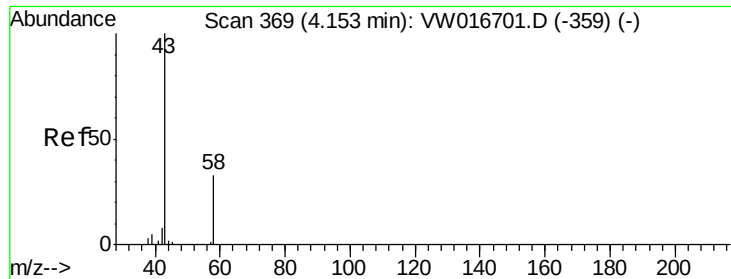





#13
Acetone
Concen: 2.438 ug/L m
RT: 4.14 min Scan# 366
Delta R.T. -0.02 min
Lab File: VW016710.D
Acq: 30 Sep 2020 14:28

Instrument :
MSVOA_W
ClientSampled :
VIBLK

Tot Ion: 43 Resp: 2920
Ion Ratio Lower Upper
43 100
58 8.9 0.0 60.2

Manual Integrations
APPROVED

MMDadoda
10/5/2020 4:10:16 PM

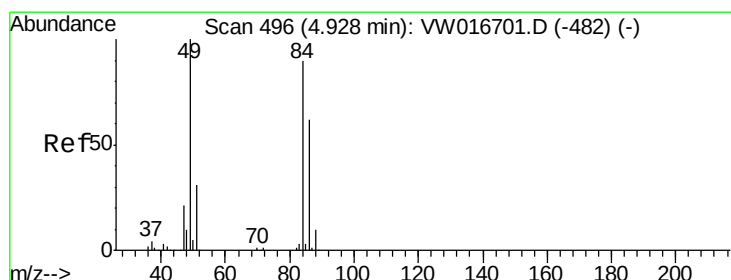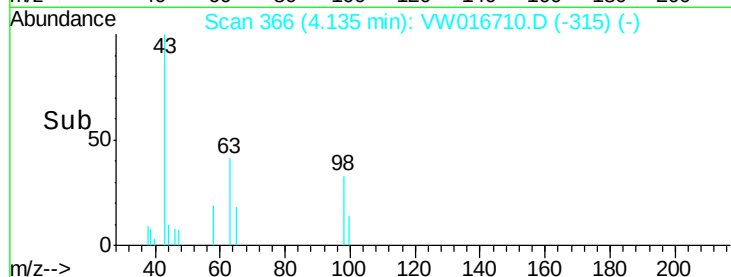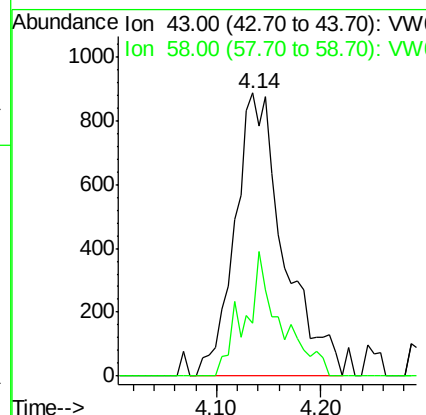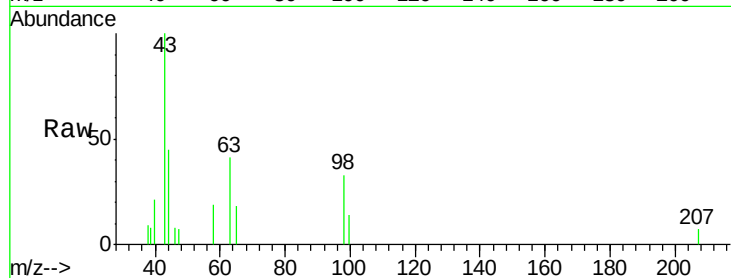

#16
Methylene chloride
Concen: 1.802 ug/L
RT: 4.93 min Scan# 497
Delta R.T. 0.01 min
Lab File: VW016710.D
Acq: 30 Sep 2020 14:28

Tgt Ion: 84 Resp: 16103
Ion Ratio Lower Upper
84 100
49 101.4 76.0 141.2
86 60.6 45.6 84.6

