

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020266.D
 Acq On : 30 Sep 2021 13:43
 Operator : SY/VA
 Sample : M3973-11RE
 Misc : 7.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X7RE

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:16:01 PM

Quant Time: Oct 01 01:05:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 01 01:03:15 2021
 Response via : Initial Calibration

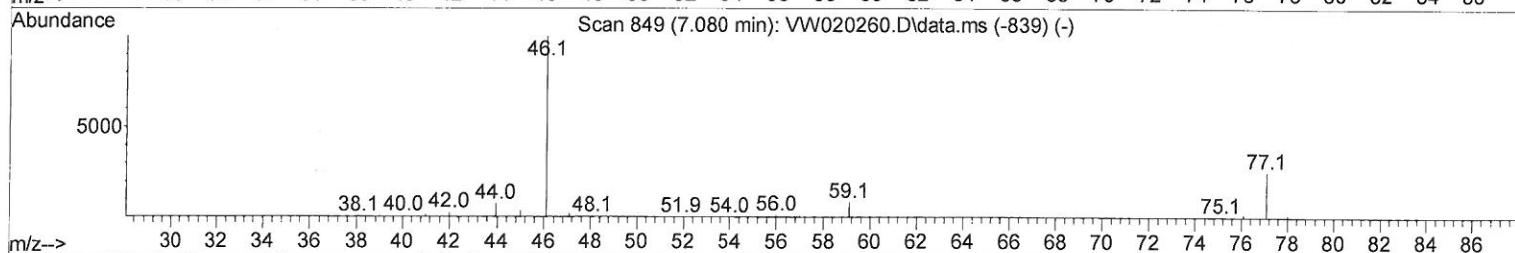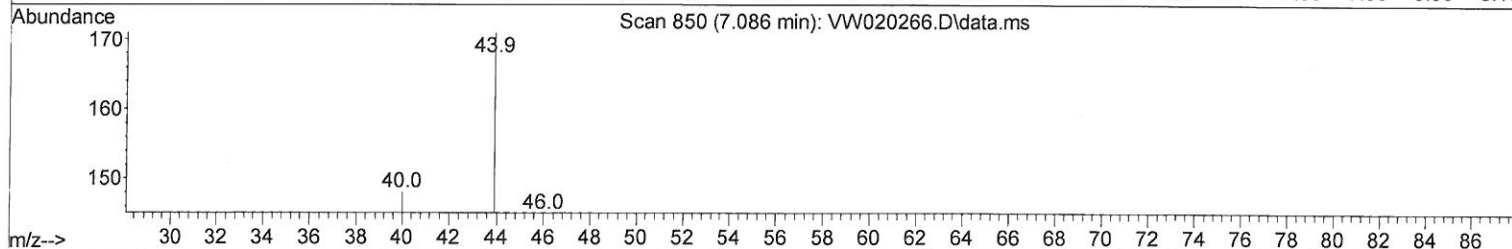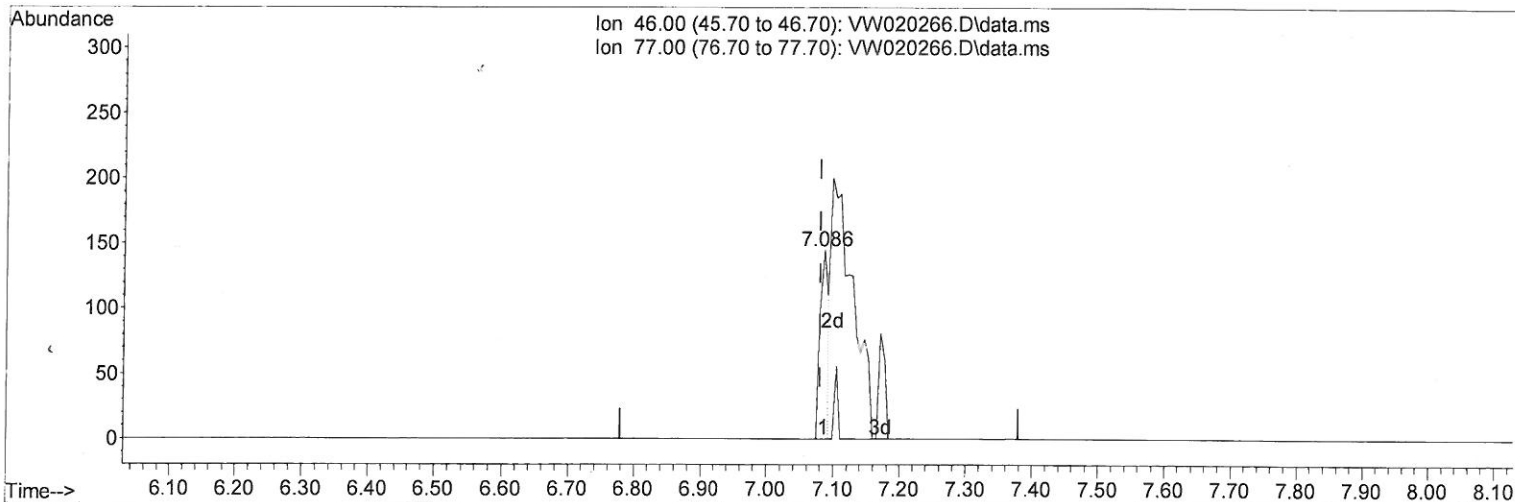

TIC: VW020266.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 2.07 ug/L

response 130

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.00	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020266.D
 Acq On : 30 Sep 2021 13:43
 Operator : SY/VA
 Sample : M3973-11RE
 Misc : 7.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X7RE

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:16:01 PM

Quant Time: Oct 01 01:05:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 01 01:03:15 2021
 Response via : Initial Calibration

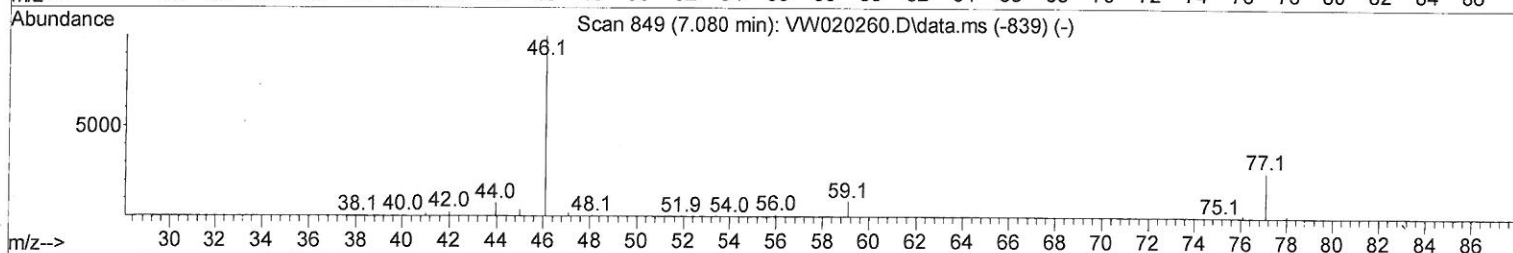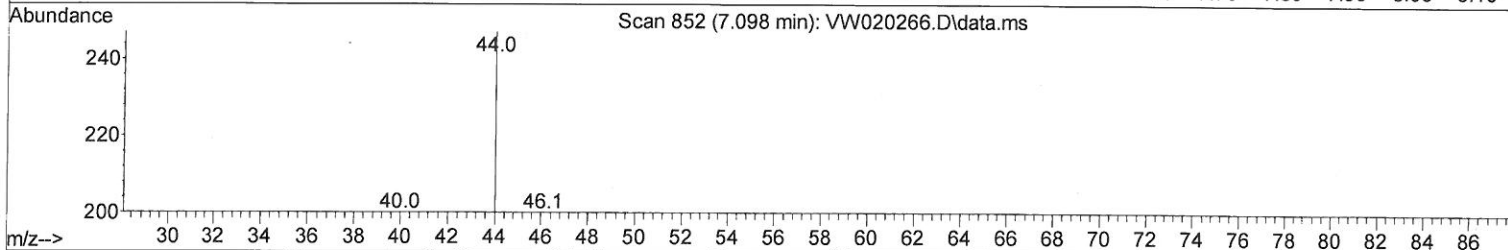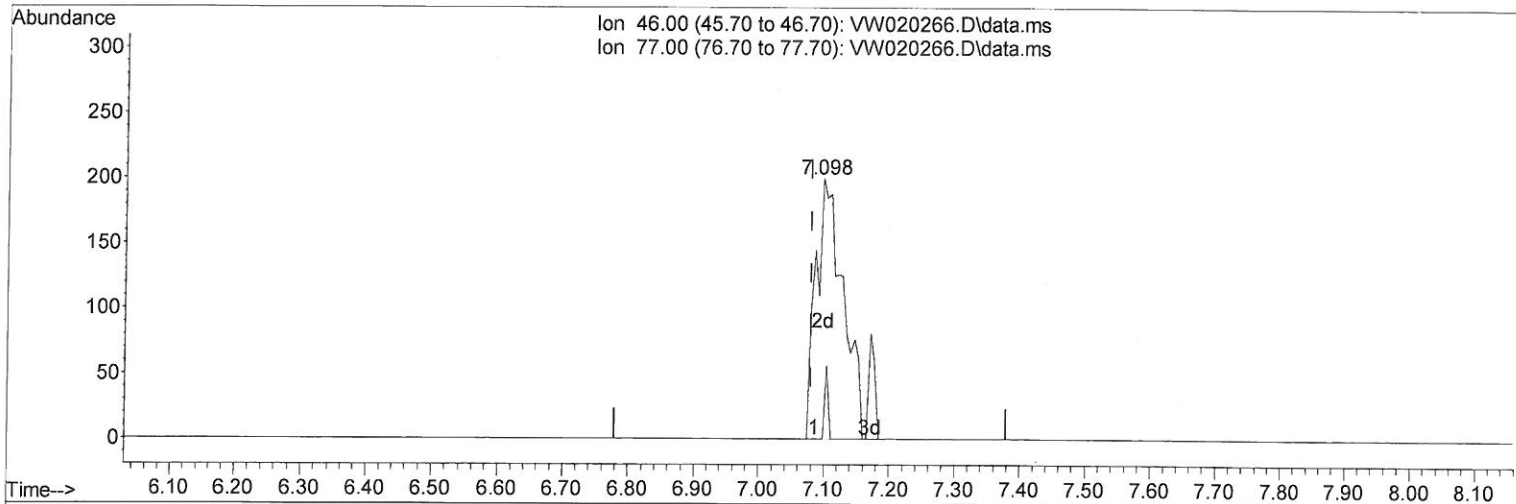

TIC: VW020266.D\data.ms

(21) 2-Butanone-d5 (S)

7.098min (+ 0.019) 9.24 ug/L m

response 580

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.00	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

> 10/04/2021 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020266.D
 Acq On : 30 Sep 2021 13:43
 Operator : SY/VA
 Sample : M3973-11RE
 Misc : 7.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X7RE

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:16:01 PM

Quant Time: Oct 01 01:05:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 01 01:03:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	19879	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.640	117	10921	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	2738	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	17850	43.892	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 175.560%#			
7) Chloroethane-d5	2.904	69	11091	36.202	ug/L	0.01
Spiked Amount 25.000	Range 30 - 150		Recovery = 144.800%			
11) 1,1-Dichloroethene-d2	4.032	63	23528	36.950	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 147.800%#			
21) 2-Butanone-d5	7.098	46	580m	9.242	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery = 18.480%#			
24) Chloroform-d	7.653	84	10892	17.422	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 69.680%			
26) 1,2-Dichloroethane-d4	8.311	65	3776	11.222	ug/L	0.01
Spiked Amount 25.000	Range 70 - 130		Recovery = 44.880%#			
32) Benzene-d6	8.281	84	22327	32.045	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 128.160%			
36) 1,2-Dichloropropane-d6	9.275	67	4463	22.133	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 88.520%			
41) Toluene-d8	10.329	98	16421	25.902	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 103.600%			
43) trans-1,3-Dichloroprop...	10.579	79	759	8.807	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 35.240%			
47) 2-Hexanone-d5	10.933	63	114	4.085	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery = 8.180%#			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	1263	8.120	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 32.480%#			
66) 1,2-Dichlorobenzene-d4	13.853	152	1803	17.562	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 70.240%#			
Target Compounds						
34) Trichloroethene	9.104	95	111414	631.464	ug/L	Qvalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
Data File : VW020266.D
Acq On : 30 Sep 2021 13:43
Operator : SY/VA
Sample : M3973-11RE
Misc : 7.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8X7RE

Manual Integrations
APPROVED

MMDadoda
10/4/2021 3:16:01 PM

Quant Time: Oct 01 01:05:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 01 01:03:15 2021
Response via : Initial Calibration

