

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020268.D
 Acq On : 30 Sep 2021 14:30
 Operator : SY/VA
 Sample : M3973-13RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X9RE

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:16:13 PM

Quant Time: Oct 01 01:05:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 01 01:03:15 2021
 Response via : Initial Calibration

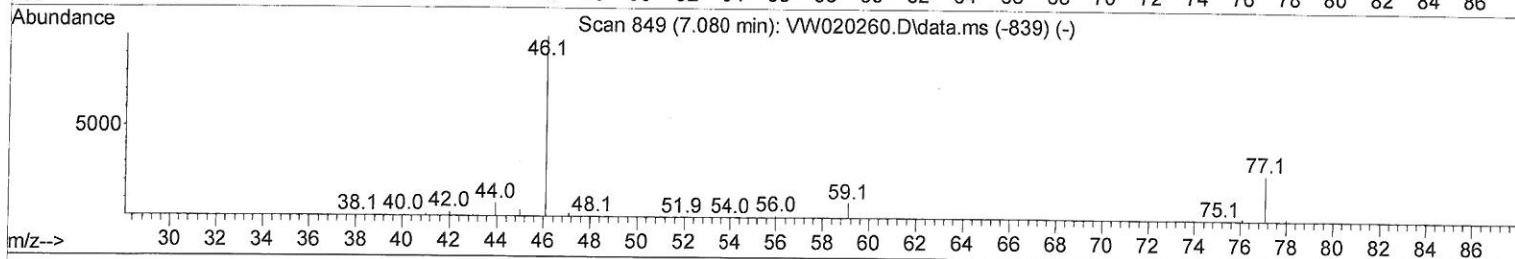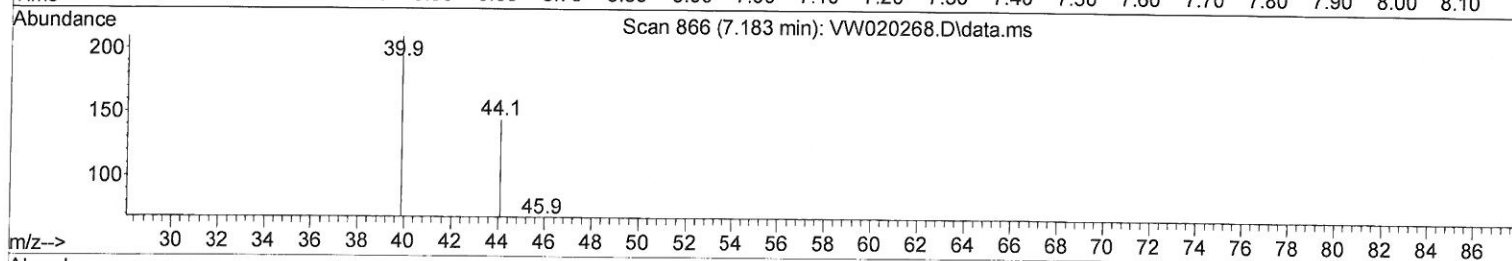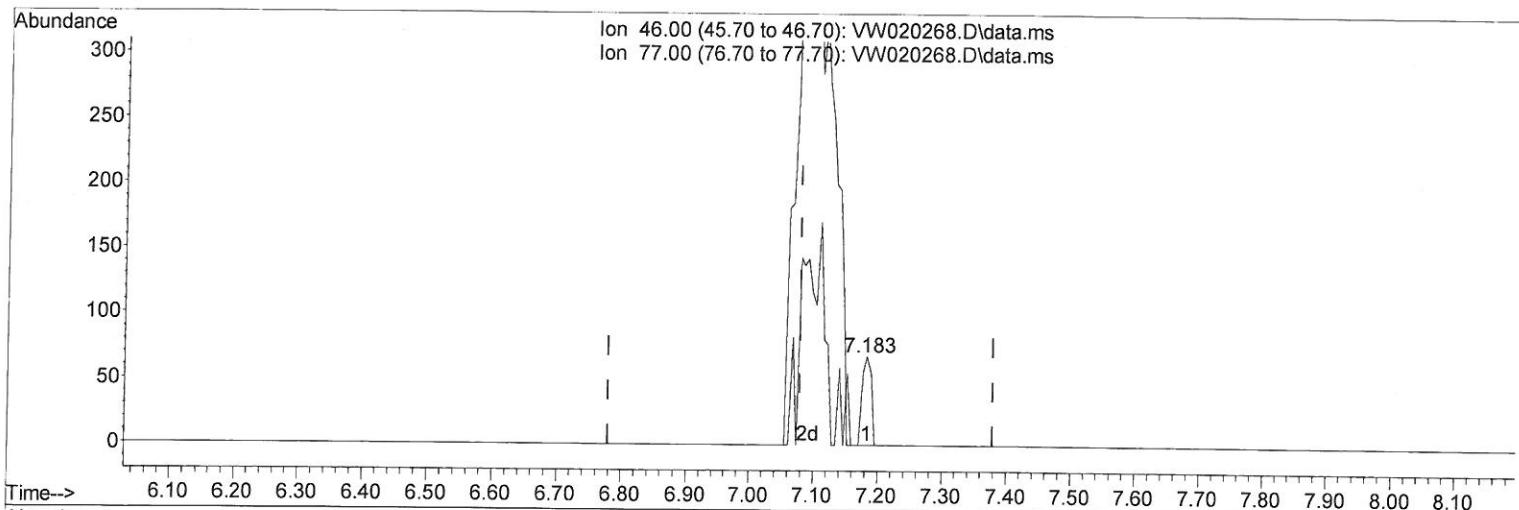

TIC: VW020268.D\data.ms

(21) 2-Butanone-d5 (S)

7.183min (+ 0.104) 0.57 ug/L

response 65

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.00	33.85
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020268.D
 Acq On : 30 Sep 2021 14:30
 Operator : SY/VA
 Sample : M3973-13RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X9RE

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:16:13 PM

Quant Time: Oct 01 01:05:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 01 01:03:15 2021
 Response via : Initial Calibration

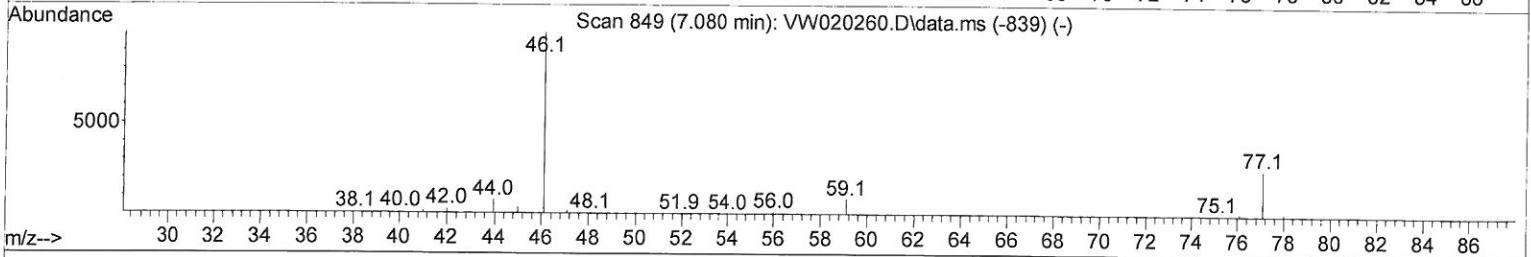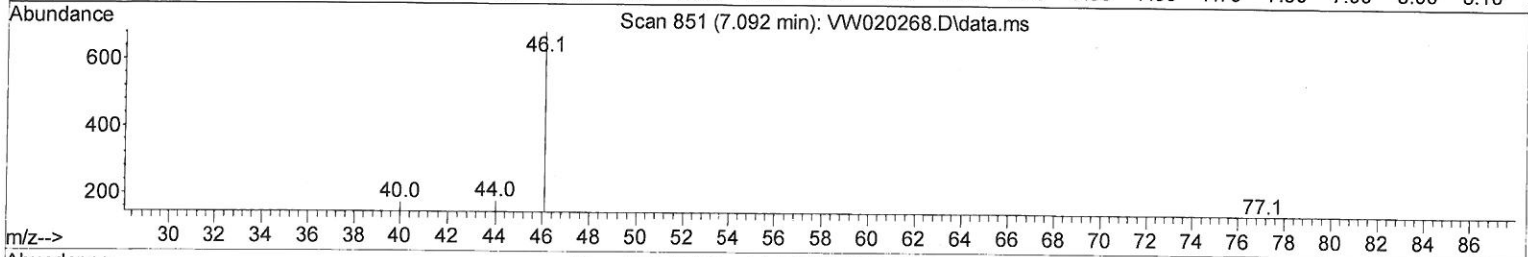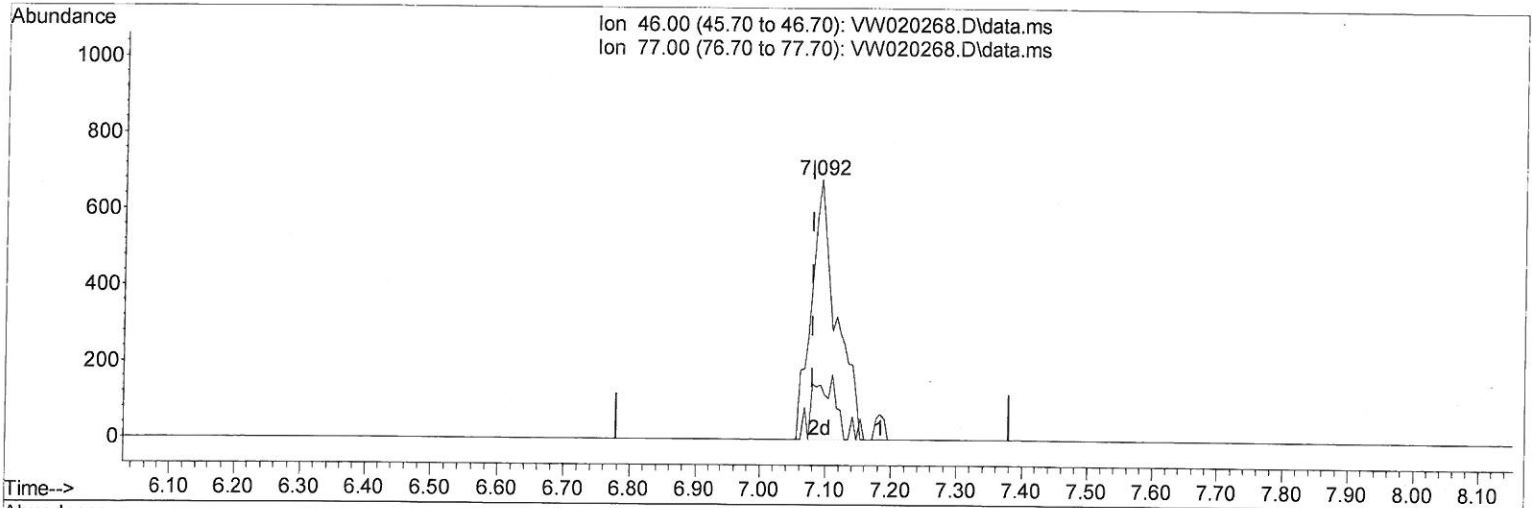

TIC: VW020268.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 15.76 ug/L m

response 1808

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.00	1.22#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020268.D
 Acq On : 30 Sep 2021 14:30
 Operator : SY/VA
 Sample : M3973-13RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X9RE

Manual Integrations
 APPROVED

MMDadoda
 10/4/2021 3:16:13 PM

Quant Time: Oct 01 01:05:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 01 01:03:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	36343	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	20154	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	3713	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	27732	37.299	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 149.200%			
7) Chloroethane-d5	2.898	69	14314	25.556	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.240%			
11) 1,1-Dichloroethene-d2	4.031	63	35380	30.392	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 121.560%#			
21) 2-Butanone-d5	7.092	46	1808m	15.759	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery = 31.520%			
24) Chloroform-d	7.653	84	22932	20.064	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 80.240%			
26) 1,2-Dichloroethane-d4	8.317	65	6030	9.802	ug/L	0.02
Spiked Amount 25.000	Range 70 - 130		Recovery = 39.200%#			
32) Benzene-d6	8.281	84	41532	32.301	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 129.200%			
36) 1,2-Dichloropropane-d6	9.281	67	8931	24.001	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 96.000%			
41) Toluene-d8	10.323	98	29695	25.382	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 101.520%			
43) trans-1,3-Dichloroprop...	10.579	79	1863	11.713	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 46.840%			
47) 2-Hexanone-d5	10.933	63	651	12.642	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery = 25.280%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	4342	15.127	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 60.520%			
66) 1,2-Dichlorobenzene-d4	13.853	152	3193	22.934	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 91.720%			
Target Compounds						
34) Trichloroethene	9.098	95	511	1.569	ug/L	89

10/04/2021

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
Data File : VW020268.D
Acq On : 30 Sep 2021 14:30
Operator : SY/VA
Sample : M3973-13RE
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8X9RE

Manual Integrations
APPROVED

MMDadoda
10/4/2021 3:16:13 PM

Quant Time: Oct 01 01:05:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 01 01:03:15 2021
Response via : Initial Calibration

