
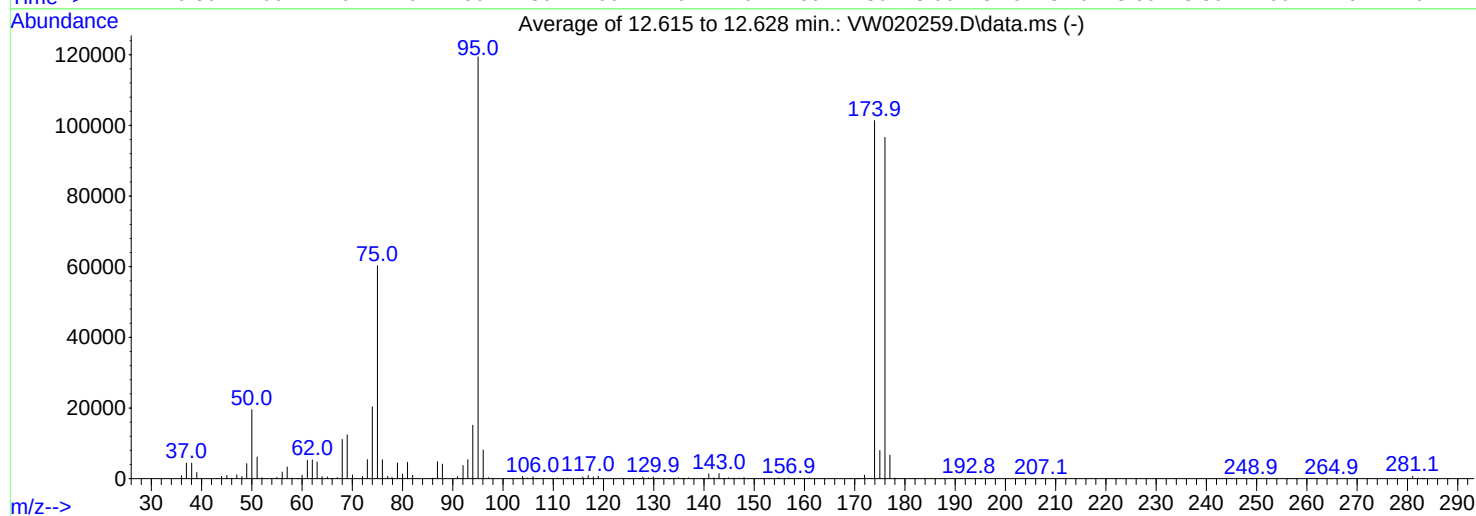


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093021\
 Data File : VW020259.D
 Acq On : 30 Sep 2021 08:12
 Operator : SY/VA
 Sample : BFB443
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB443

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Title : SFAM01.0
 Last Update : Fri Oct 01 01:03:15 2021

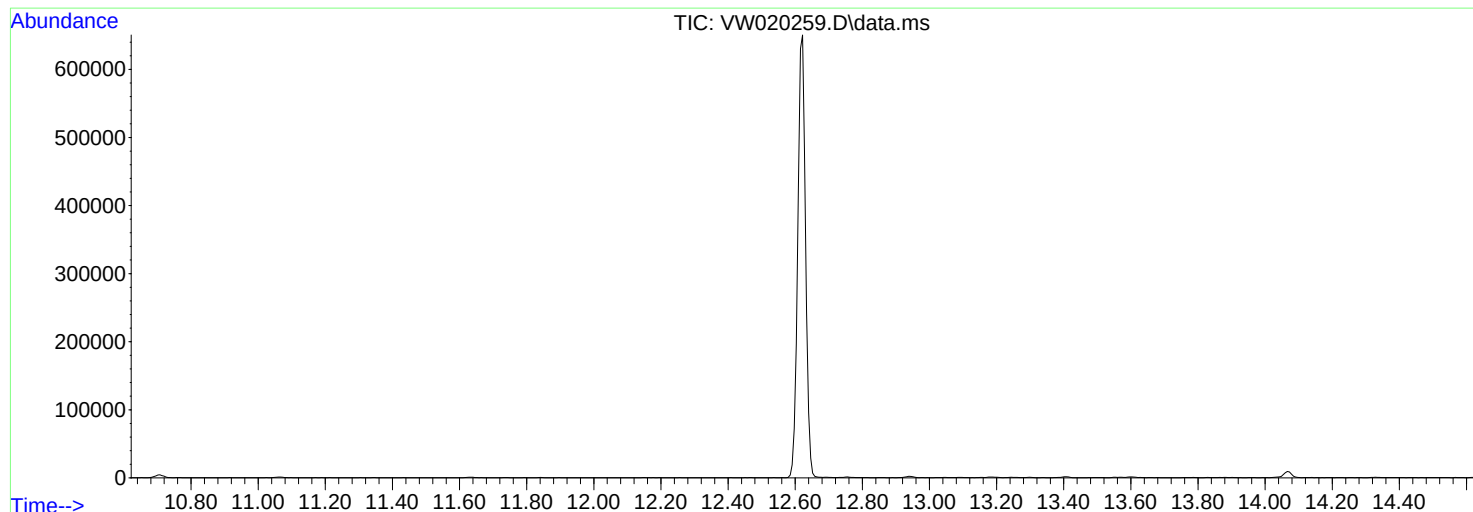

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	19531	PASS
75	95	30	80	50.5	60293	PASS
95	95	100	100	100.0	119416	PASS
96	95	5	9	6.8	8109	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.9	101365	PASS
175	174	5	9	7.9	7959	PASS
176	174	95	105	95.3	96632	PASS
177	176	5	10	6.9	6642	PASS

m/z	Abundance
36.10	574.0
37.00	3203.0
38.00	3559.0
39.00	1255.0
39.90	109.0
43.00	61.0
44.00	646.0
45.00	648.0
46.00	94.0
47.00	876.0
48.00	559.0
49.00	3267.0
50.00	14210.0
51.00	4485.0
52.00	202.0
53.00	57.0
54.90	248.0
56.00	1419.0
57.10	2517.0
58.10	182.0
60.00	730.0
61.00	3866.0
62.00	4146.0
63.00	3654.0
64.00	502.0
65.10	442.0
67.10	189.0
68.00	8772.0
69.00	9433.0
70.00	862.0
71.90	416.0
73.00	3929.0
74.00	15313.0
75.00	47904.0
76.00	4029.0
77.00	411.0
77.90	320.0
79.00	3459.0
80.00	1142.0
80.90	3442.0
81.90	670.0
83.10	89.0
86.10	160.0
87.00	3418.0
88.00	3416.0
90.90	459.0
92.00	2904.0
93.00	4392.0
94.00	11807.0
95.10	94856.0
96.00	6264.0
97.20	145.0
104.00	537.0
104.90	149.0
106.00	416.0
106.90	126.0
109.80	71.0
111.00	92.0
111.90	88.0
112.90	126.0
114.80	196.0
115.80	319.0
117.00	847.0
117.90	403.0
119.00	642.0
123.90	68.0
127.90	473.0
128.90	267.0
129.90	476.0
131.00	149.0
132.90	57.0
134.90	186.0
137.00	218.0
141.00	1150.0
142.00	162.0
143.00	1230.0
144.00	91.0
144.90	150.0
145.70	93.0
146.90	95.0
147.90	187.0
148.80	72.0
150.10	146.0
152.90	90.0
154.80	195.0
156.90	121.0
158.70	114.0
160.90	154.0
169.20	61.0
170.40	99.0
171.00	135.0
171.90	875.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

174.00	89504.0
175.00	6638.0
176.00	86760.0
177.00	5394.0
178.10	157.0
281.10	350.0
282.80	60.0
283.20	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

Scan 1749 (12.567 min): VW020259.D\data.ms
BFB443

m/z	Abundance
40.10	117.0
44.00	235.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

m/z	Abundance
36.00	1020.0
37.00	5205.0
38.10	4968.0
39.10	2032.0
40.20	155.0
43.00	77.0
44.00	1071.0
45.00	1076.0
46.00	134.0
47.00	1267.0
48.10	744.0
49.00	5108.0
50.00	22984.0
51.00	7314.0
52.00	237.0
52.90	56.0
55.00	363.0
56.00	2050.0
57.00	3757.0
57.90	238.0
59.10	72.0
60.10	1222.0
61.00	6036.0
62.10	5938.0
63.00	5361.0
64.00	676.0
65.10	547.0
66.00	73.0
67.10	371.0
68.00	12439.0
69.00	14368.0
70.00	1257.0
72.00	759.0
73.00	6416.0
74.00	23304.0
75.00	65272.0
76.00	6105.0
77.00	905.0
77.90	350.0
79.00	5084.0
80.00	1395.0
81.00	5205.0
82.00	1065.0
83.10	81.0
86.00	109.0
87.00	5644.0
88.00	4822.0
90.90	594.0
92.00	4332.0
93.00	6022.0
94.00	17224.0
95.00	128992.0
96.10	9132.0
97.00	292.0
102.80	85.0
103.80	642.0
104.80	201.0
105.90	660.0
106.70	124.0
110.00	132.0
110.90	166.0
112.00	93.0
112.90	184.0
115.20	171.0
115.90	490.0
116.90	862.0
118.00	615.0
119.00	695.0
123.80	69.0
125.00	70.0
125.80	53.0
127.10	75.0
127.90	497.0
129.00	174.0
129.90	464.0
130.80	116.0
132.80	119.0
133.90	79.0
134.90	264.0
136.90	236.0
139.80	74.0
140.90	1412.0
141.90	202.0
143.00	1570.0
144.00	102.0
144.90	411.0
146.00	144.0
147.00	189.0
147.90	320.0
148.90	102.0
149.80	157.0
152.90	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

154.80	289.0
156.90	204.0
158.80	154.0
161.00	130.0
169.10	52.0
170.70	165.0
172.00	1123.0
173.90	97520.0
175.00	8692.0
176.00	99888.0
177.00	6300.0
177.90	279.0
191.10	109.0
192.80	196.0
195.10	62.0
207.10	114.0
248.90	75.0
264.90	135.0
281.00	953.0
282.10	242.0
283.10	149.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

m/z	Abundance
36.00	886.0
37.00	4760.0
38.00	4616.0
39.00	1836.0
39.90	224.0
43.10	56.0
44.10	908.0
45.10	1009.0
45.90	127.0
47.00	1097.0
48.10	652.0
49.00	4448.0
50.00	21400.0
51.10	6500.0
52.00	359.0
55.00	449.0
56.10	2070.0
57.00	3597.0
58.00	145.0
59.90	1053.0
61.10	5696.0
62.00	5840.0
63.00	5091.0
64.00	548.0
65.00	484.0
65.90	58.0
66.90	365.0
68.00	12125.0
69.00	13382.0
70.10	1012.0
72.00	684.0
73.00	5887.0
74.00	22472.0
75.00	67704.0
76.00	5952.0
77.10	608.0
77.90	422.0
79.00	4780.0
80.00	1466.0
81.00	5253.0
82.00	1109.0
82.90	116.0
86.10	137.0
86.90	5414.0
87.90	4178.0
91.00	669.0
92.10	3865.0
93.00	5749.0
94.00	16363.0
95.00	134400.0
96.10	8930.0
97.10	388.0
102.90	96.0
103.90	763.0
104.80	238.0
105.90	572.0
107.00	121.0
109.90	101.0
110.80	153.0
112.00	107.0
112.90	115.0
115.00	118.0
115.90	497.0
116.90	908.0
117.90	492.0
118.90	747.0
123.90	137.0
125.80	50.0
127.80	445.0
128.90	281.0
129.90	553.0
130.90	153.0
133.10	67.0
134.00	67.0
135.00	363.0
135.80	54.0
136.80	238.0
140.90	1498.0
141.90	377.0
143.00	1567.0
144.00	75.0
144.90	277.0
145.80	210.0
147.00	118.0
148.00	414.0
148.90	104.0
150.00	179.0
151.80	71.0
153.00	100.0
155.00	365.0
156.90	238.0
158.80	203.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

161.00	204.0
169.10	70.0
170.80	149.0
171.90	949.0
174.00	117072.0
175.00	8548.0
176.00	103248.0
177.00	8231.0
177.90	209.0
192.70	97.0
249.10	67.0
265.00	70.0
281.10	650.0
282.20	259.0
282.90	93.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443