

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093022\
 Data File : VW024689.D
 Acq On : 30 Sep 2022 09:49
 Operator : SY/VA
 Sample : VW0930SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK413

Quant Time: Sep 30 22:13:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 22:12:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	573832	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	514188	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	240560	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	148404	24.718	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.880%
7) Chloroethane-d5	2.885	69	80420	23.051	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	4.019	63	218665	15.736	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.960%
21) 2-Butanone-d5	7.080	46	111888	51.836	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.680%
24) Chloroform-d	7.647	84	367536	23.958	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.840%
26) 1,2-Dichloroethane-d4	8.305	65	194815	24.480	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.920%
32) Benzene-d6	8.274	84	783681	23.845	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	9.274	67	240271	23.928	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.720%
41) Toluene-d8	10.323	98	672757	22.903	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	10.579	79	97799	21.870	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.480%
47) 2-Hexanone-d5	10.920	63	88131	51.297	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.600%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	184690	25.813	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.240%
66) 1,2-Dichlorobenzene-d4	13.847	152	204419	24.149	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.600%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	7024	0.500	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093022\
Data File : VW024689.D
Acq On : 30 Sep 2022 09:49
Operator : SY/VA
Sample : VW0930SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK413

Quant Time: Sep 30 22:13:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 22:12:13 2022
Response via : Initial Calibration

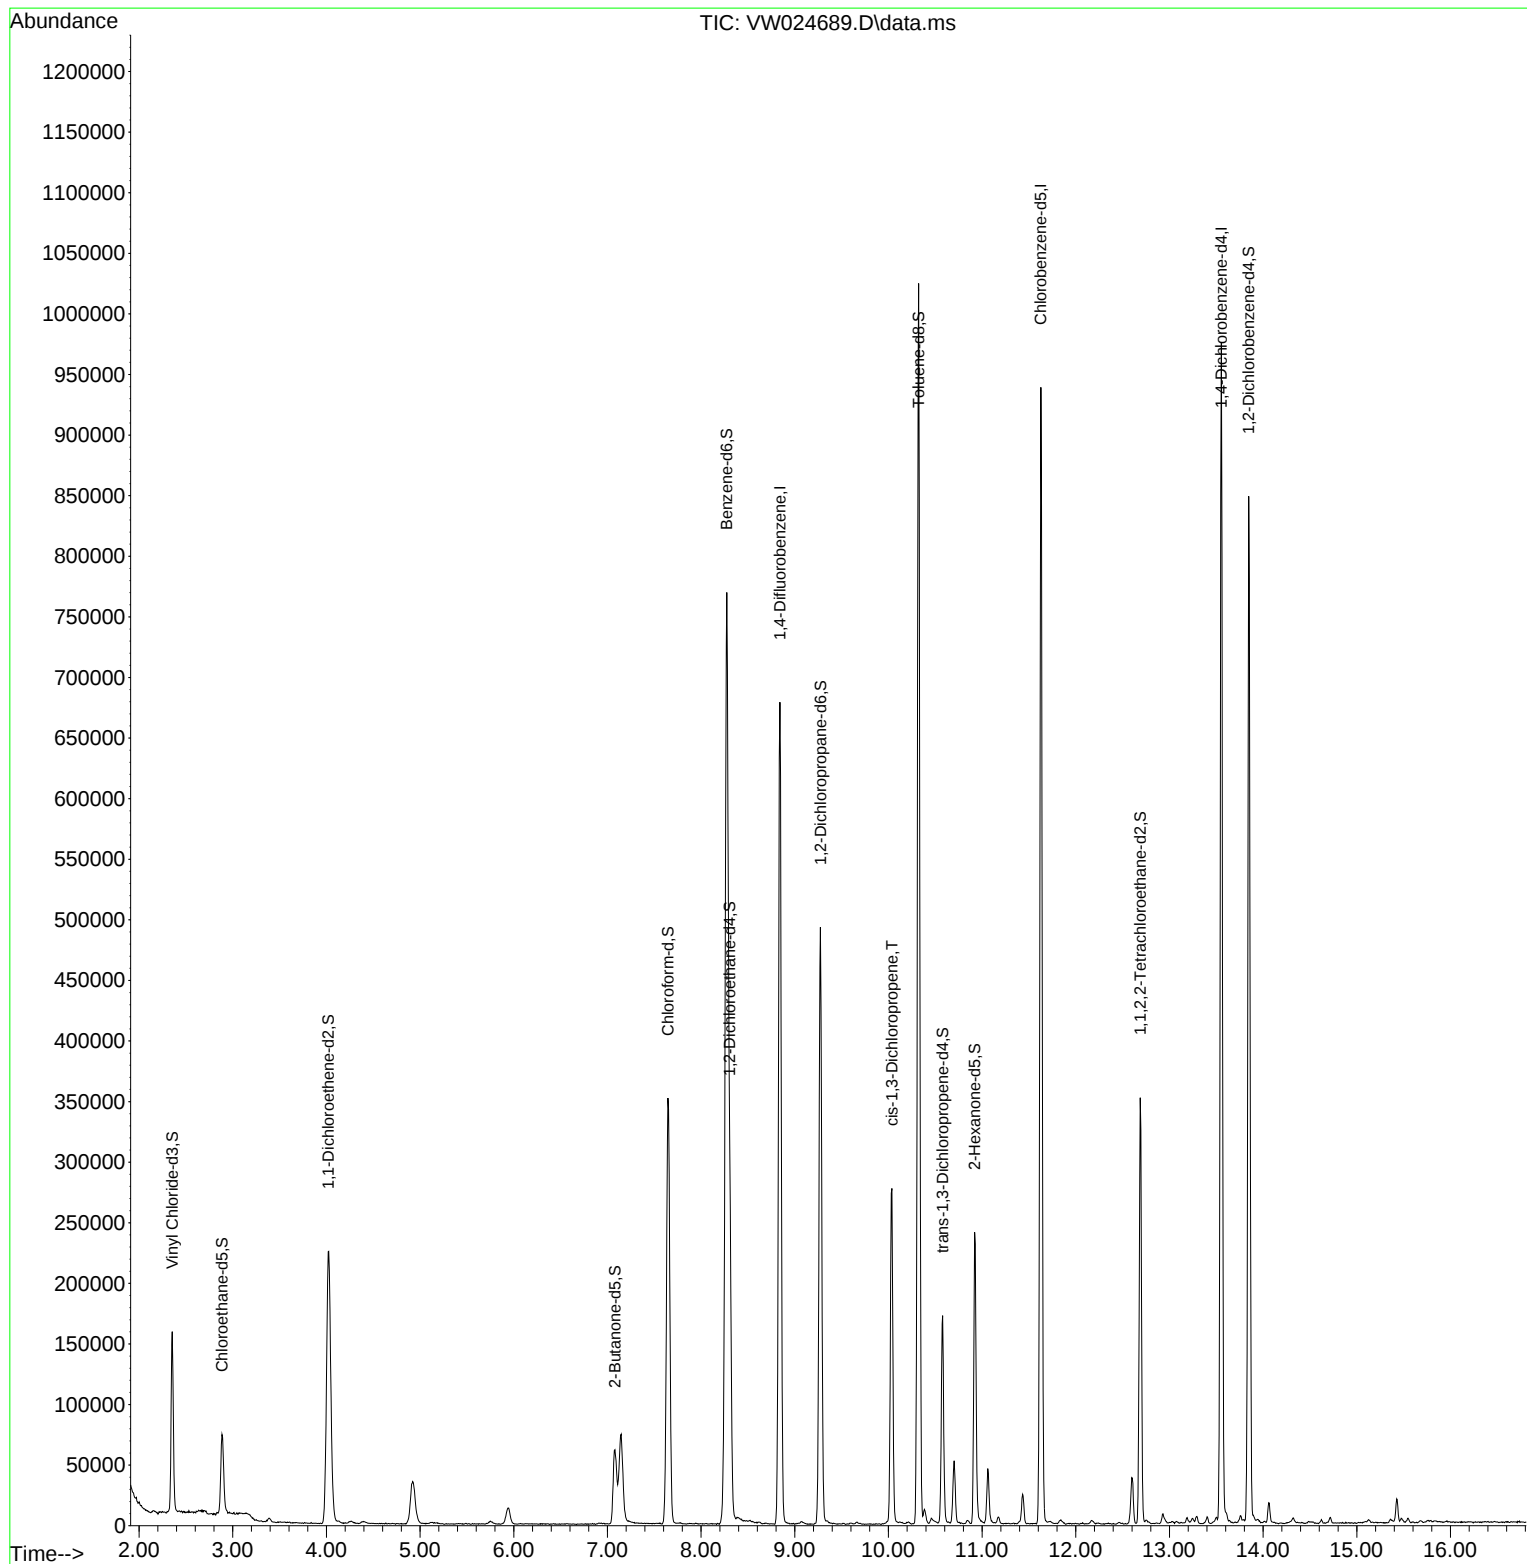

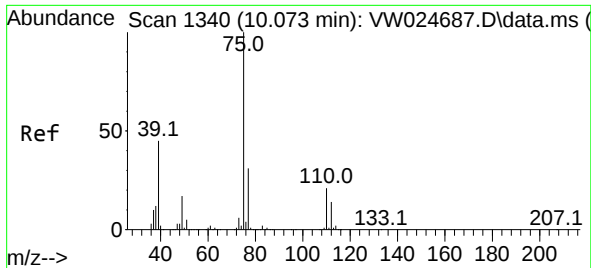

#39
 cis-1,3-Dichloropropene
 Concen: 0.500 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024689.D
 Acq: 30 Sep 2022 09:49

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK413

Tgt Ion: 75 Resp: 7024
 Ion Ratio Lower Upper
 75 100
 77 51.0 22.4 41.6#

