

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093022\
 Data File : VW024699.D
 Acq On : 30 Sep 2022 17:50
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK561

Quant Time: Sep 30 22:15:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 22:12:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	597488	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	537500	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	259973	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	140980	22.552	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.200%
7) Chloroethane-d5	2.892	69	77657	21.377	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.520%
11) 1,1-Dichloroethene-d2	4.019	63	222301	15.364	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.440%
21) 2-Butanone-d5	7.086	46	96078	42.749	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.500%
24) Chloroform-d	7.653	84	336711	21.080	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.320%
26) 1,2-Dichloroethane-d4	8.305	65	175763	21.212	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.840%
32) Benzene-d6	8.275	84	701169	20.409	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.640%
36) 1,2-Dichloropropane-d6	9.275	67	217467	20.718	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.880%
41) Toluene-d8	10.323	98	607310	19.779	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.120%
43) trans-1,3-Dichloroprop...	10.579	79	88385	18.908	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.640%
47) 2-Hexanone-d5	10.921	63	77759	43.297	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.600%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	165584	22.139	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	193610	21.164	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.640%
Target Compounds						Qvalue
35) Methylcyclohexane	9.275	83	52506	3.004	ug/L	# 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093022\
Data File : VW024699.D
Acq On : 30 Sep 2022 17:50
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK561

Quant Time: Sep 30 22:15:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 22:12:13 2022
Response via : Initial Calibration

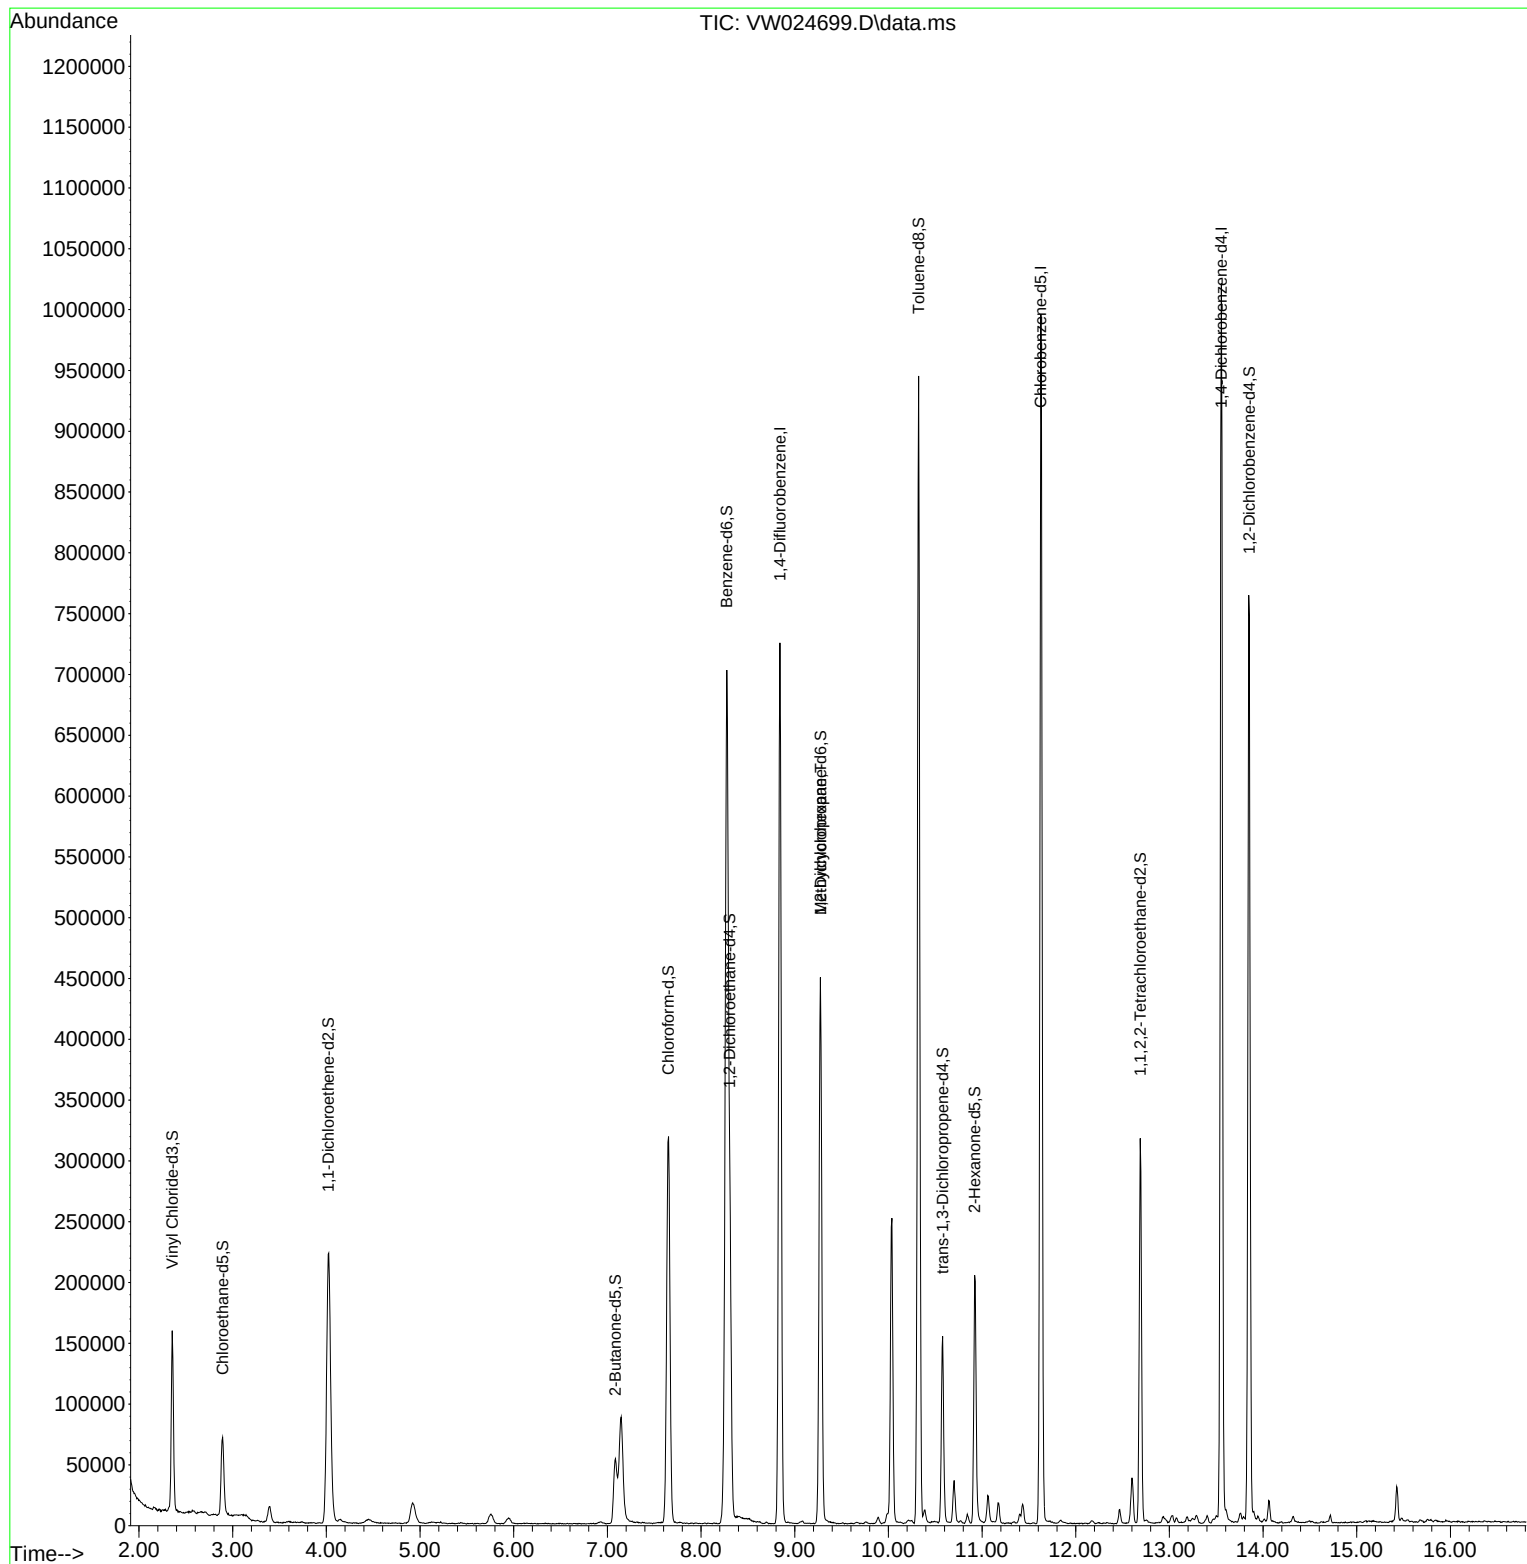

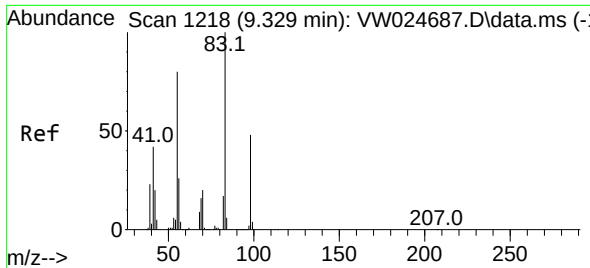

#35
Methylcyclohexane
Concen: 3.004 ug/L
RT: 9.275 min Scan# 11
Delta R.T. -0.055 min
Lab File: VW024699.D
Acq: 30 Sep 2022 17:50

Instrument :
MSVOA_W
ClientSampleId :
VIBLK561

Tgt Ion	Ratio	Lower	Upper
83	100		
55	0.6	63.1	94.7#
98	1.9	38.3	57.5#

