

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093022\
 Data File : VW024695.D
 Acq On : 30 Sep 2022 12:52
 Operator : SY/VA
 Sample : VIBLK560
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK560

Quant Time: Sep 30 22:14:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 22:12:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	607468	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	532593	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	259645	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	148450	23.357	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.440%
7) Chloroethane-d5	2.885	69	79061	21.406	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.640%
11) 1,1-Dichloroethene-d2	4.013	63	224679	15.273	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.080%
21) 2-Butanone-d5	7.080	46	105871	46.332	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.660%
24) Chloroform-d	7.647	84	366505	22.568	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.280%
26) 1,2-Dichloroethane-d4	8.305	65	192807	22.887	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.560%
32) Benzene-d6	8.275	84	770352	22.630	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.520%
36) 1,2-Dichloropropane-d6	9.268	67	238014	22.884	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.520%
41) Toluene-d8	10.323	98	673233	22.127	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.520%
43) trans-1,3-Dichloroprop...	10.573	79	95181	20.549	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.200%
47) 2-Hexanone-d5	10.921	63	82543	46.384	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.760%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	179056	24.161	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	202146	22.125	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.480%
Target Compounds					Qvalue	
13) Acetone	4.129	43	6616	3.968	ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093022\
Data File : VW024695.D
Acq On : 30 Sep 2022 12:52
Operator : SY/VA
Sample : VIBLK560
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK560

Quant Time: Sep 30 22:14:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 22:12:13 2022
Response via : Initial Calibration

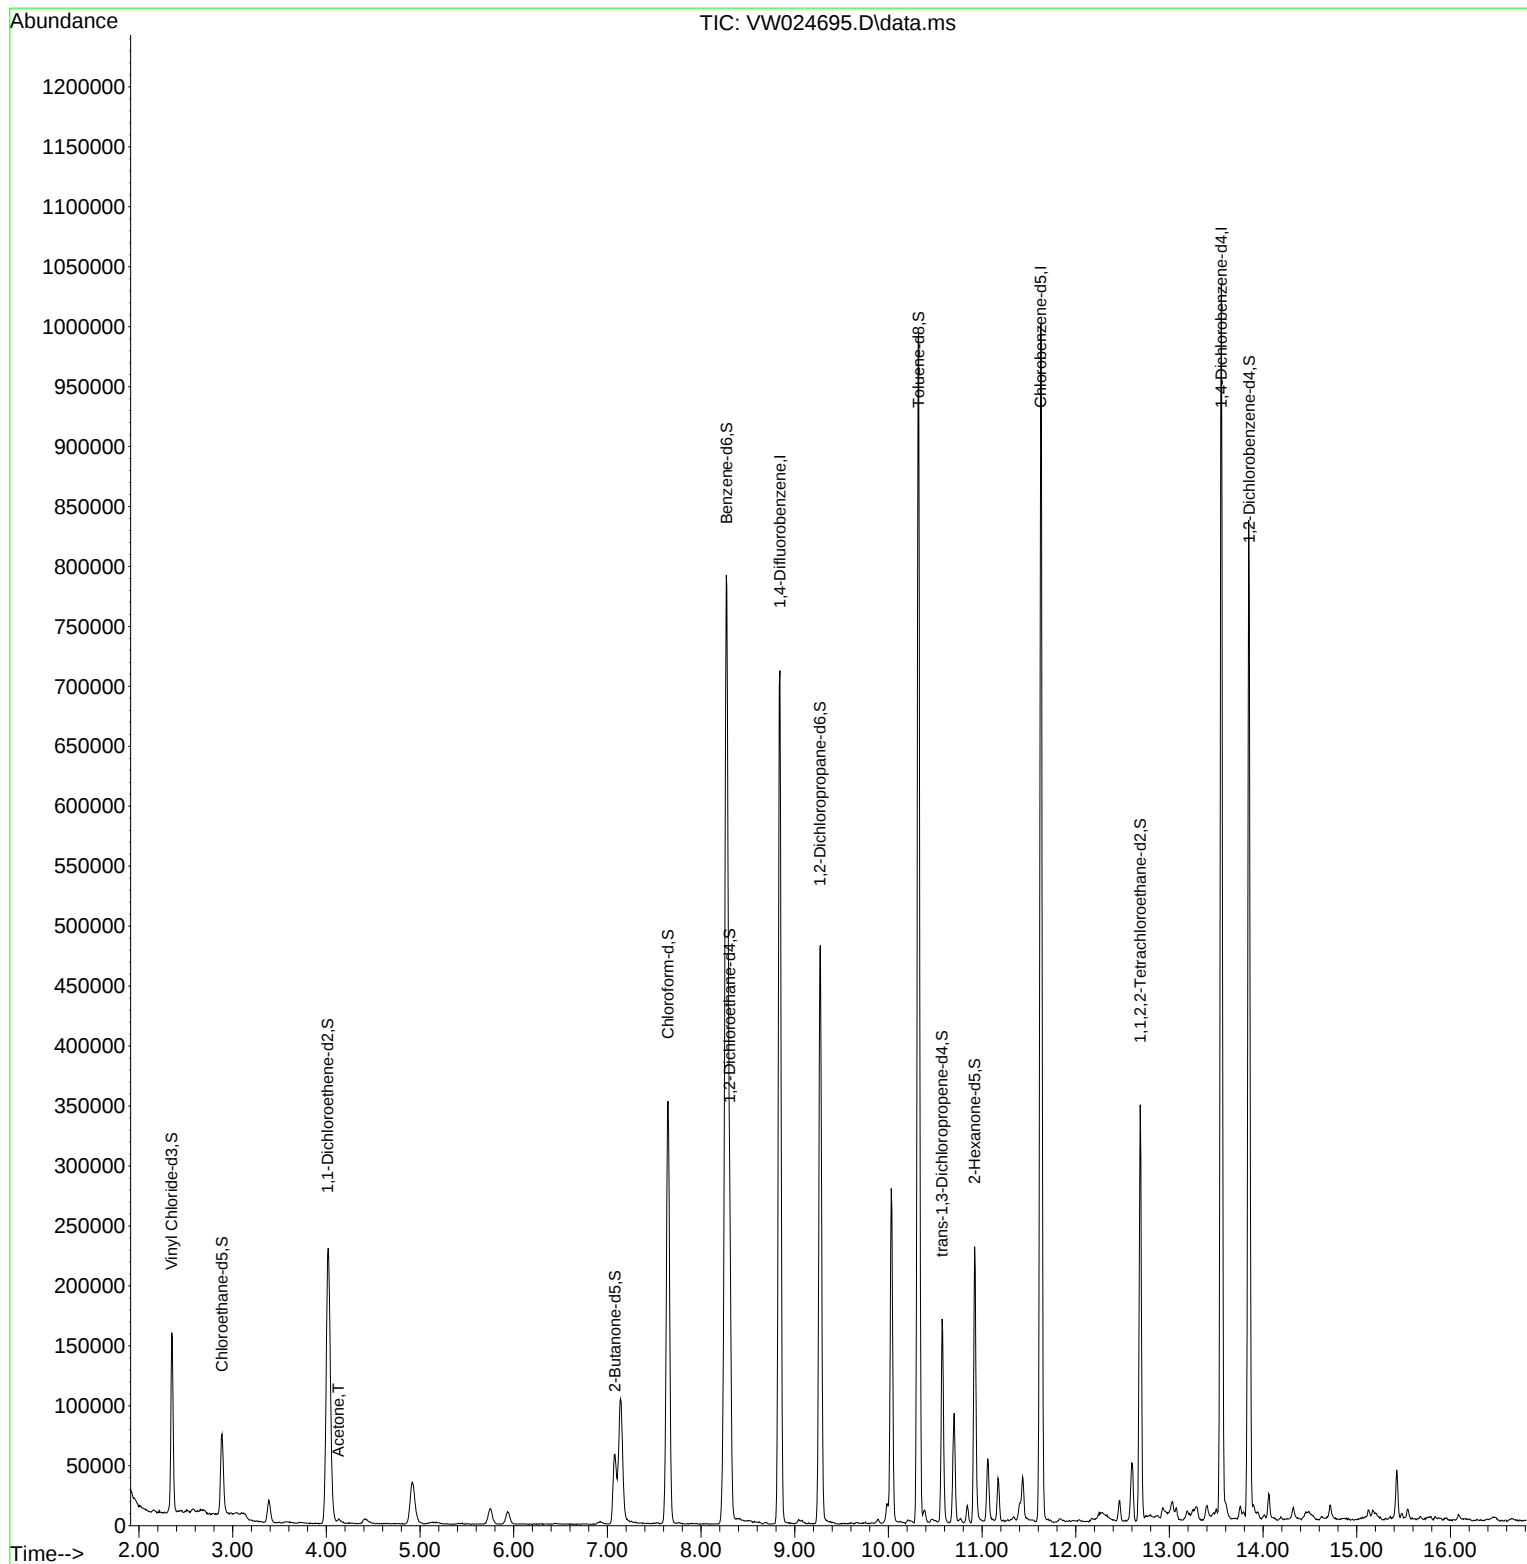

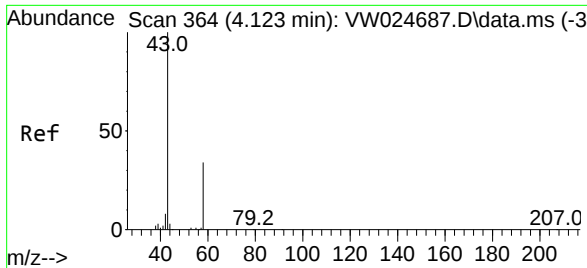

#13
 Acetone
 Concen: 3.968 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024695.D
 Acq: 30 Sep 2022 12:52

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK560

Tgt Ion: 43 Resp: 6616
 Ion Ratio Lower Upper
 43 100
 58 18.6 0.0 67.6

