

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100118\
 Data File : VW005751.D
 Acq On : 01 Oct 2018 23:21
 Operator : SY/AP
 Sample : J5180-18
 Misc : 3.12G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JLC27

Quant Time: Oct 02 07:27:39 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 02 07:19:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	142258	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	149752	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	67238	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	21942	12.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.40%
7) Chloroethane-d5	2.89	69	21453	15.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.64%
10) 1,1-Dichloroethene-d2	4.01	63	42772	10.80	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.20%#
20) 2-Butanone-d5	7.09	46	31481	54.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.14%
24) Chloroform-d	7.65	84	85190	23.31	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.24%
26) 1,2-Dichloroethane-d4	8.31	65	58892	26.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.44%
29) Benzene-d6	8.27	84	138318	18.66	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.64%
33) 1,2-Dichloropropane-d6	9.28	67	49485	23.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.36%
37) Toluene-d8	10.33	98	120831	16.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.04%
38) trans-1,3-Dichloropropene-	10.58	79	21942	19.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.00%
39) 2-Hexanone-d5	10.93	63	21917	43.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.36%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	52957	25.44	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.76%
61) 1,2-Dichlorobenzene-d4	13.86	152	53927	22.67	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.68%


Target Compounds					Ovalue
13) Acetone	4.12	43	4786	7.894 ug/L	97
16) Methylene chloride	4.90	84	8297	3.537 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100118\
Data File : VW005751.D
Acq On : 01 Oct 2018 23:21
Operator : SY/AP
Sample : J5180-18
Misc : 3.12G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLC27

Quant Time: Oct 02 07:27:39 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 02 07:19:35 2018
Response via : Initial Calibration

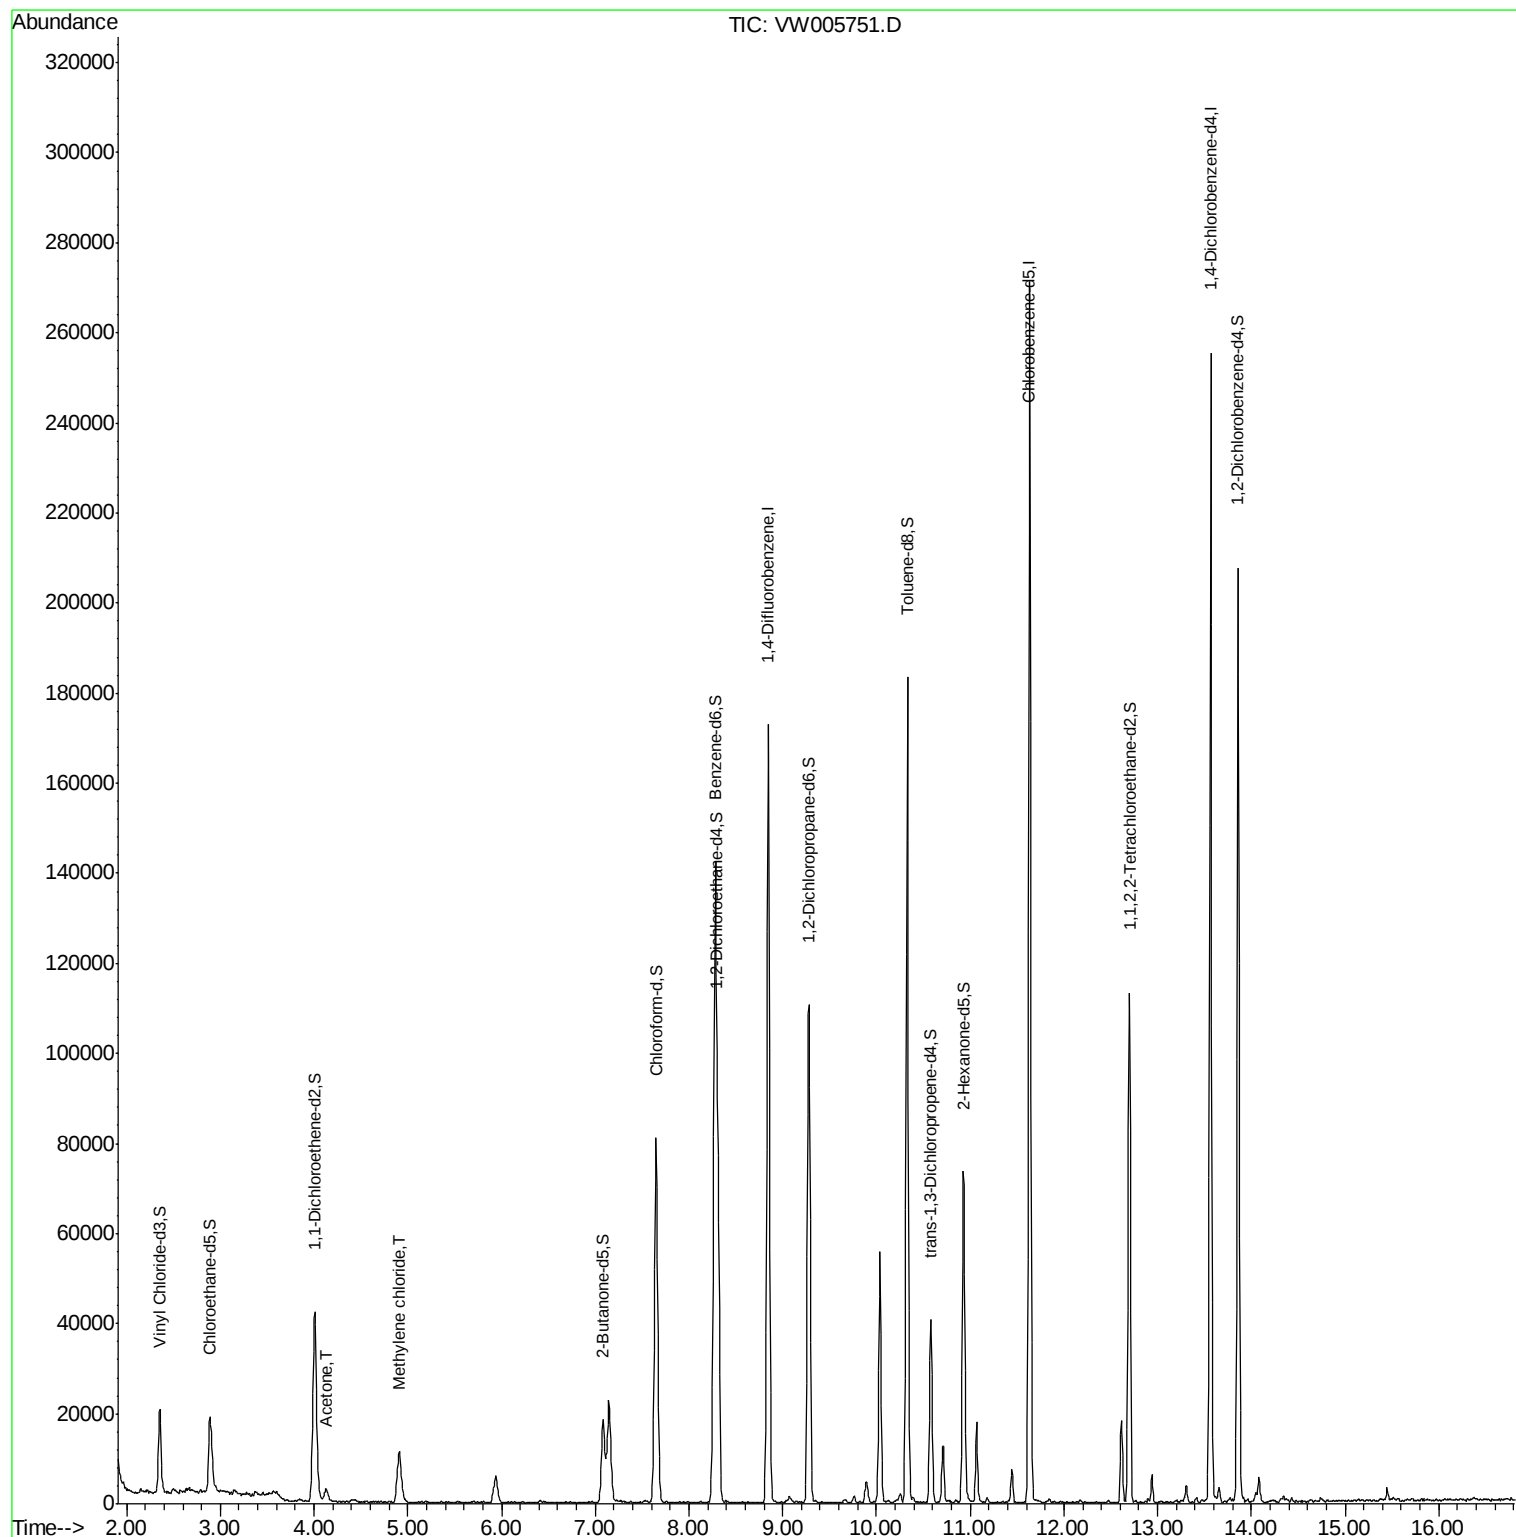

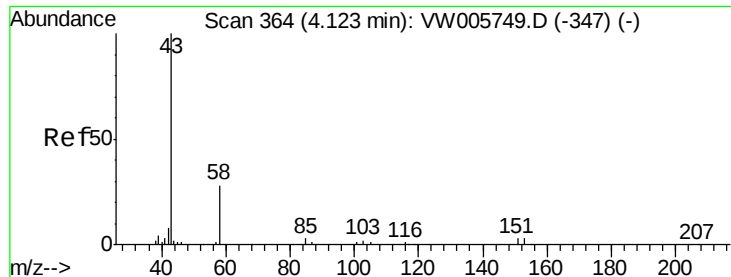

#13

Acetone

Concen: 7.894 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.00 min

Lab File: VW005751.D

Acq: 01 Oct 2018 23:21

Instrument :

MSVOA_W

ClientSampleId :





JLC27

Tot Ion: 43 Resp: 4786

Ion Ratio Lower Upper

43 100

58 14.6 0.0 31.8

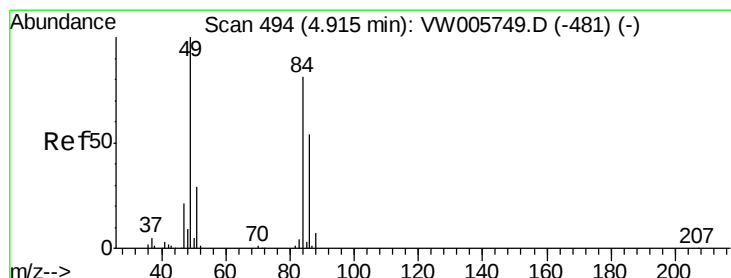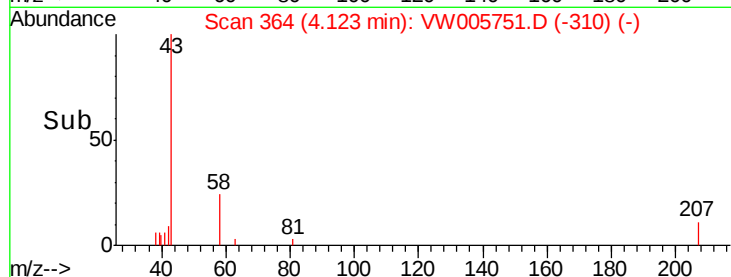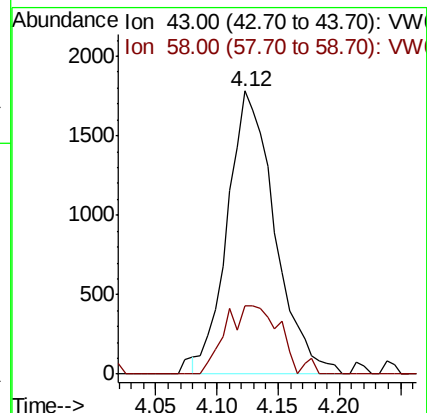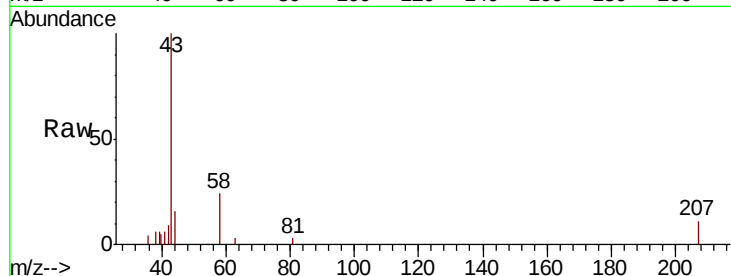

#16

Methylene chloride

Concen: 3.537 ug/L

RT: 4.90 min Scan# 492

Delta R.T. -0.01 min

Lab File: VW005751.D

Acq: 01 Oct 2018 23:21

Tgt Ion: 84 Resp: 8297

Ion Ratio Lower Upper

84 100

49 134.4 87.2 162.0

86 59.7 43.2 80.2

