



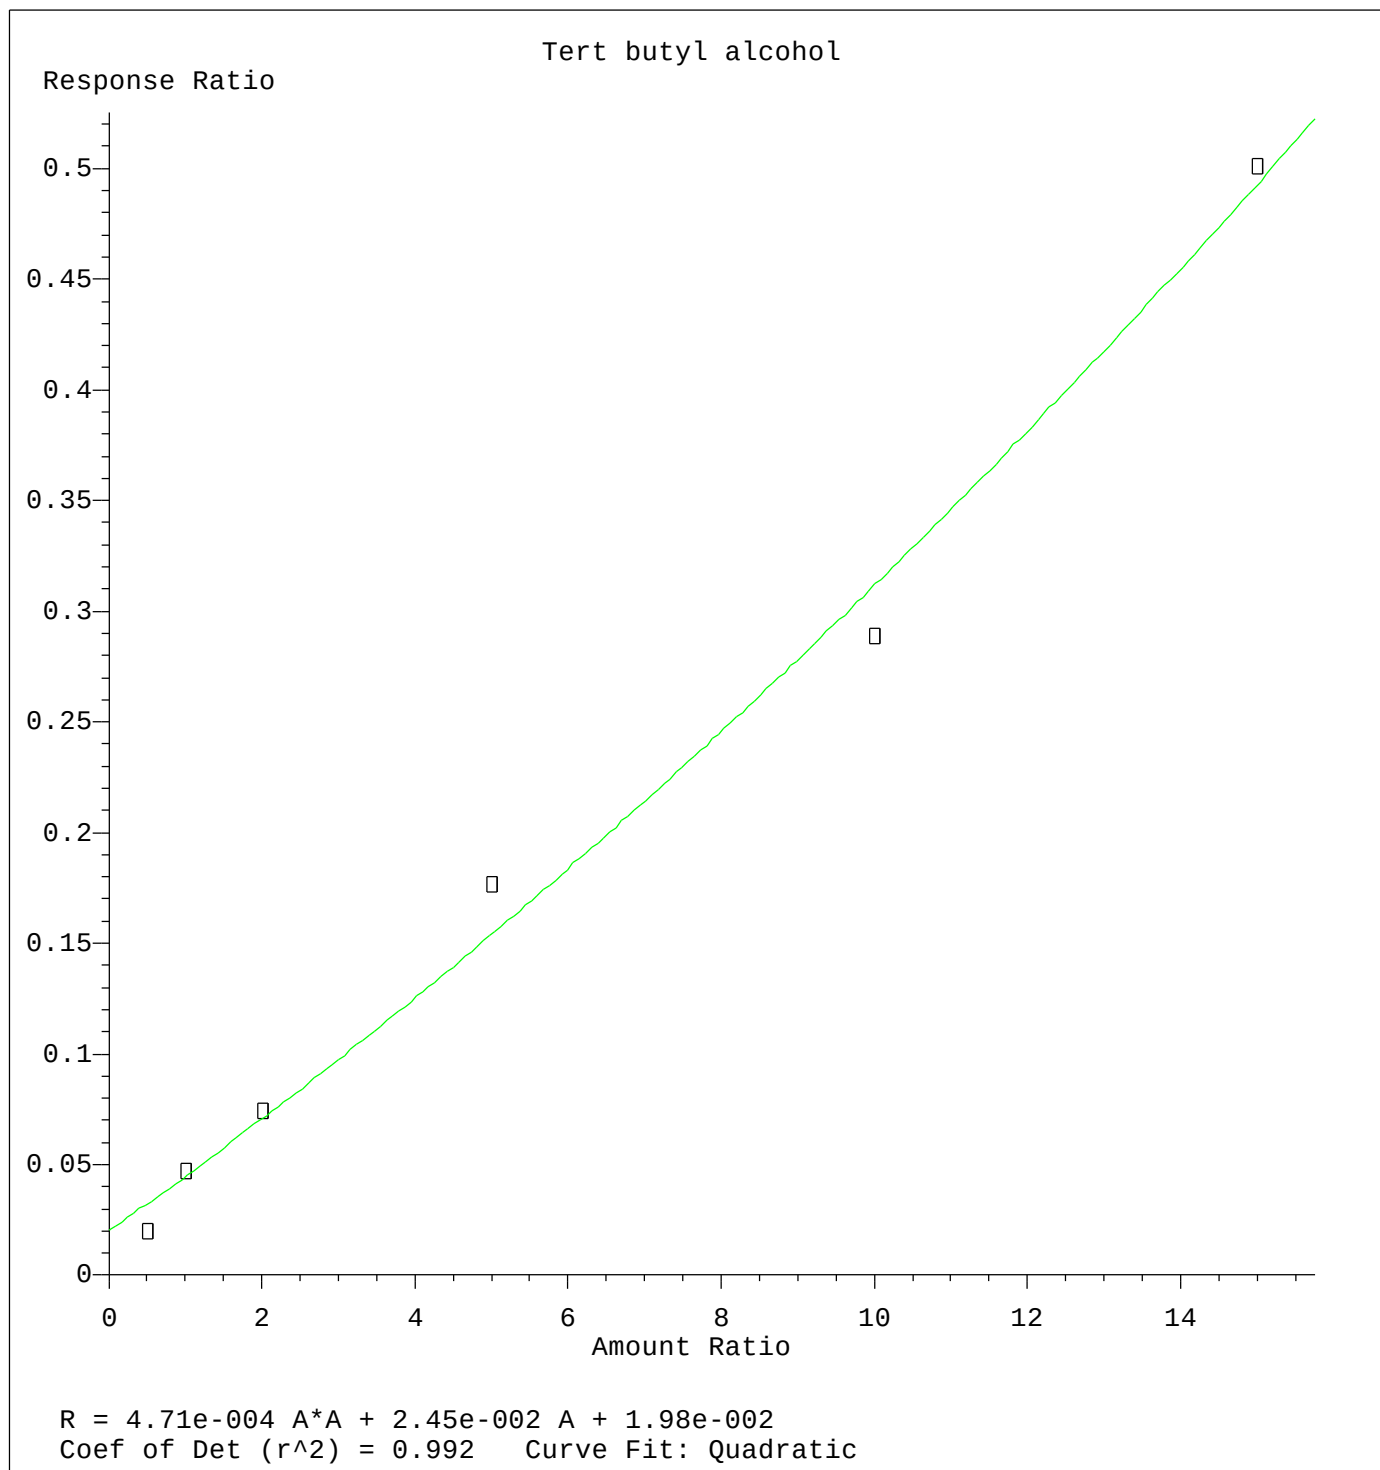


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019

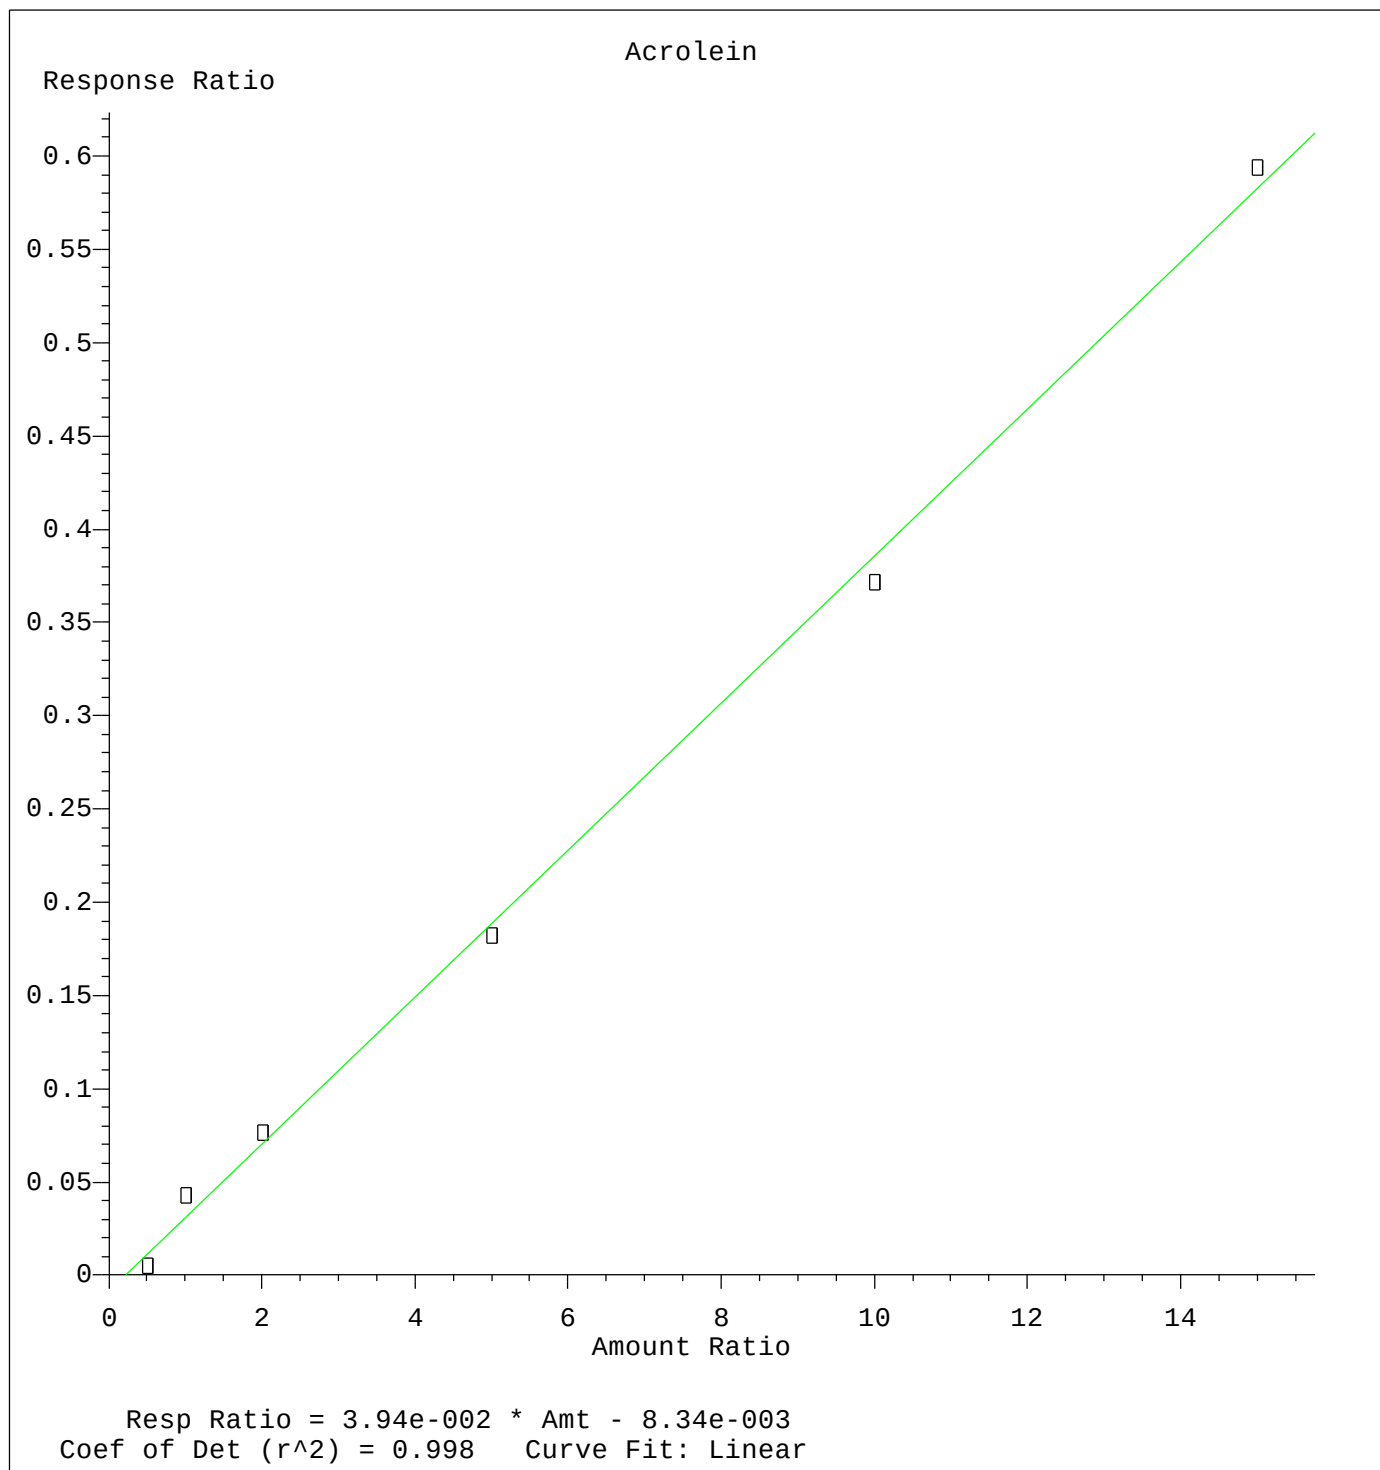

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019

Methylene Chloride

Response Ratio

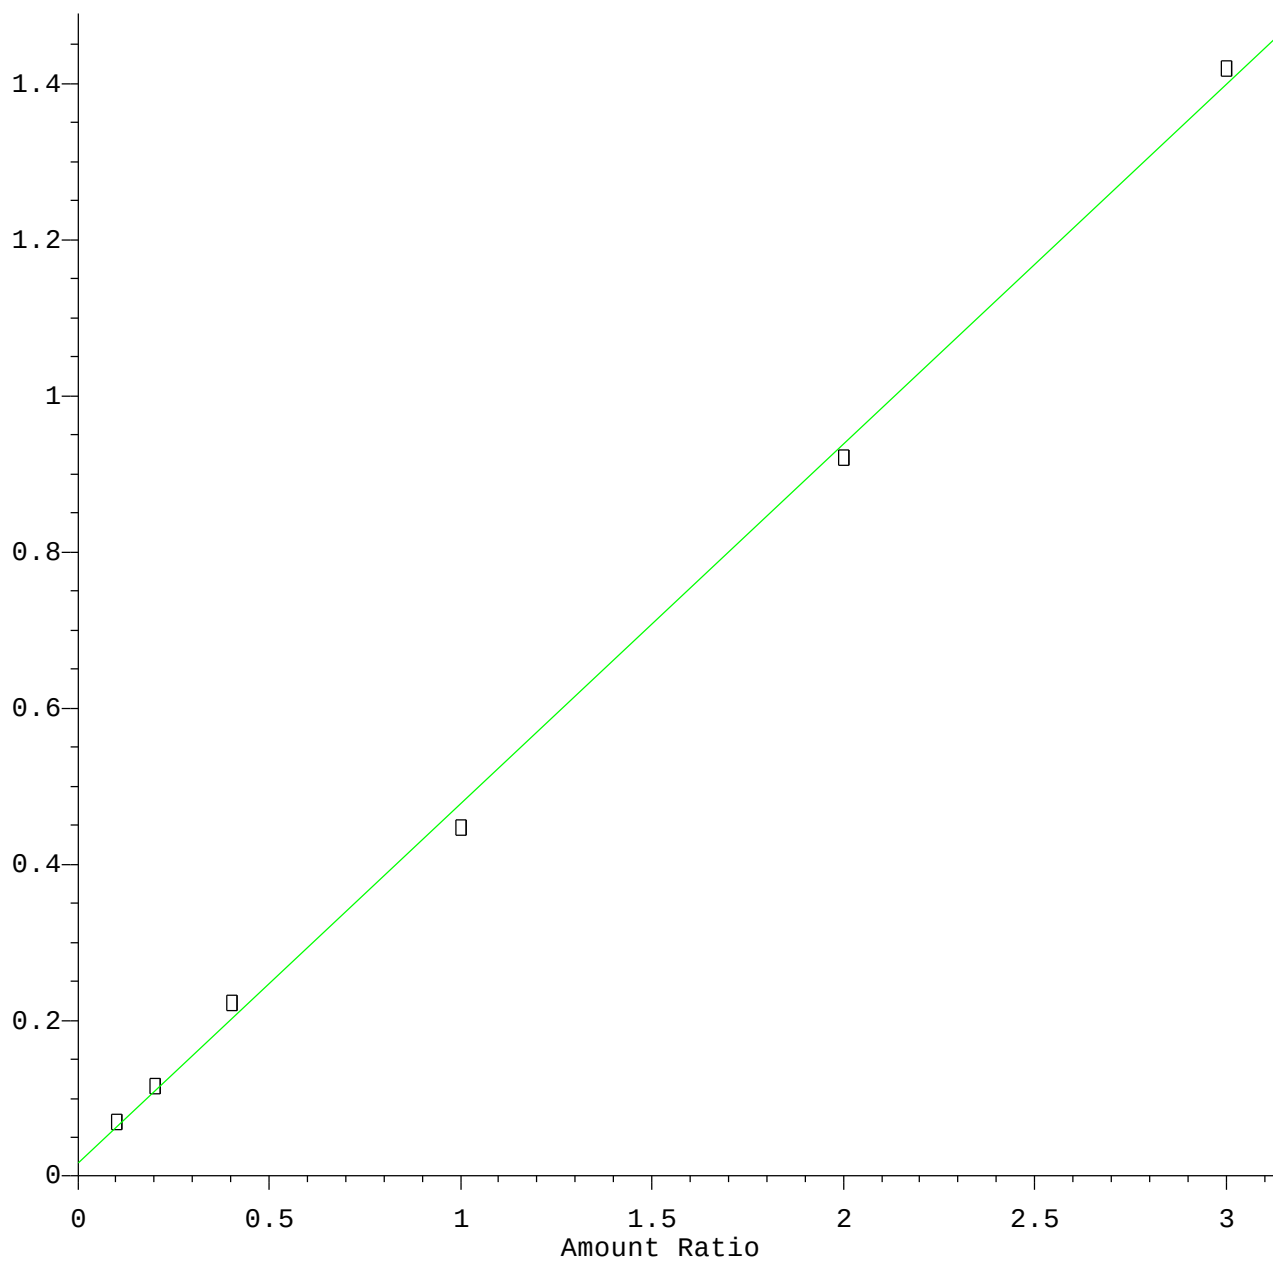


Resp Ratio = $4.61 \times 10^{-1} \times \text{Amt} + 1.71 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019


2,2-Dichloropropane

Response Ratio

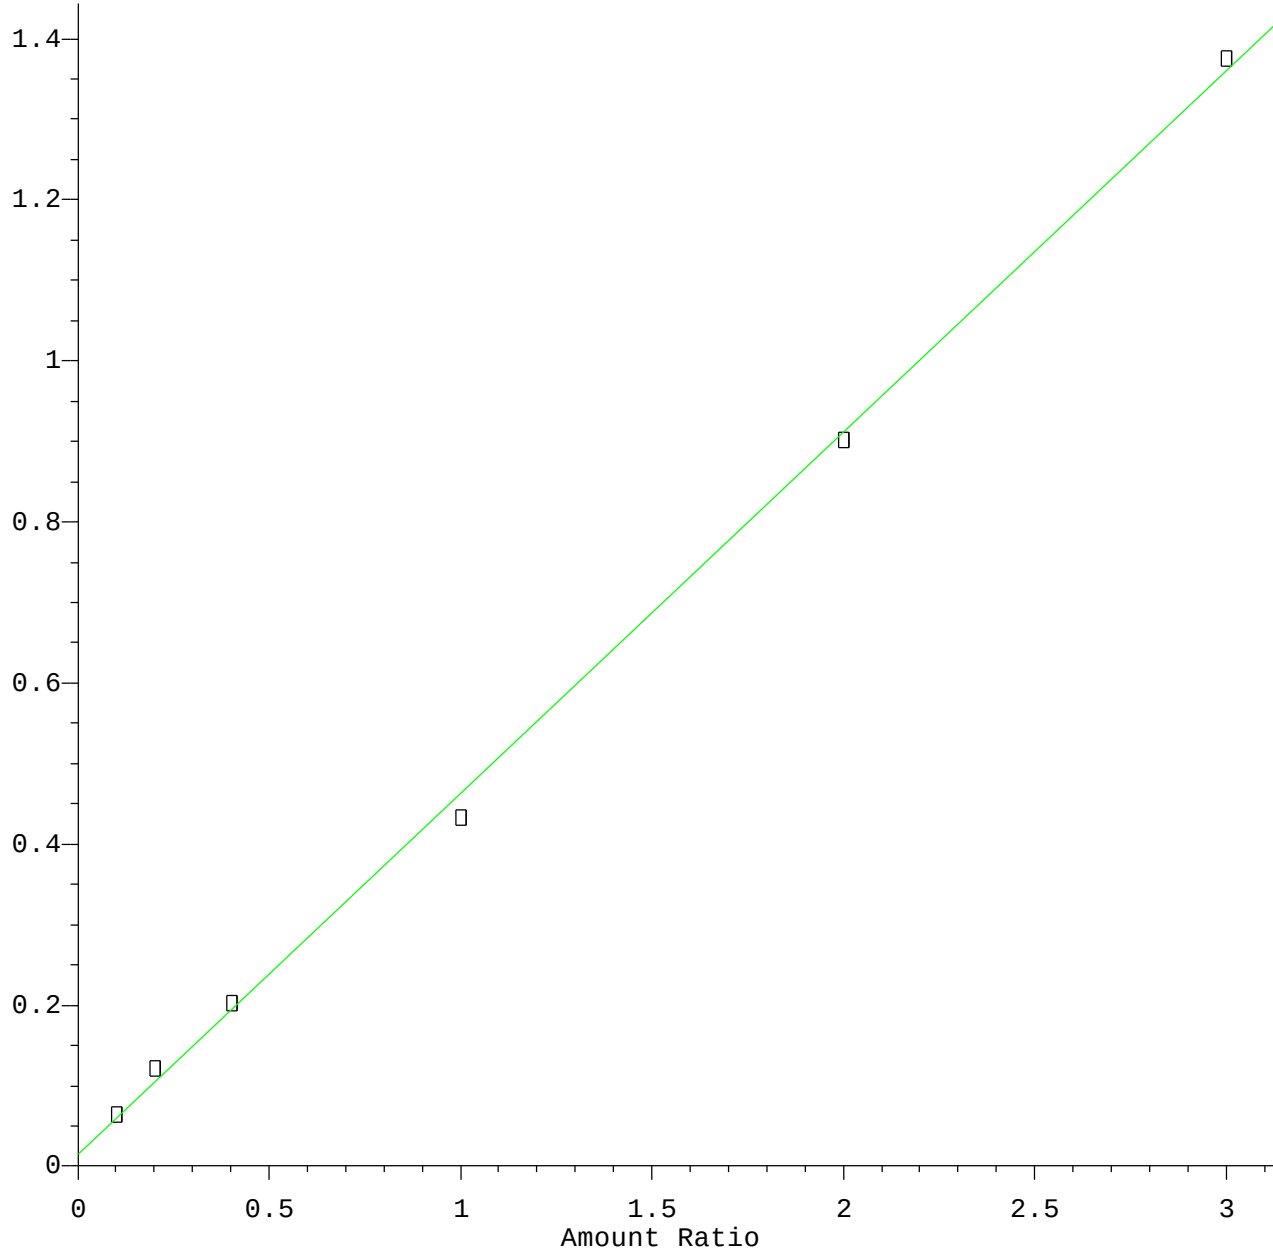


Resp Ratio = $4.48 \times 10^{-1} \times \text{Amt} + 1.54 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019

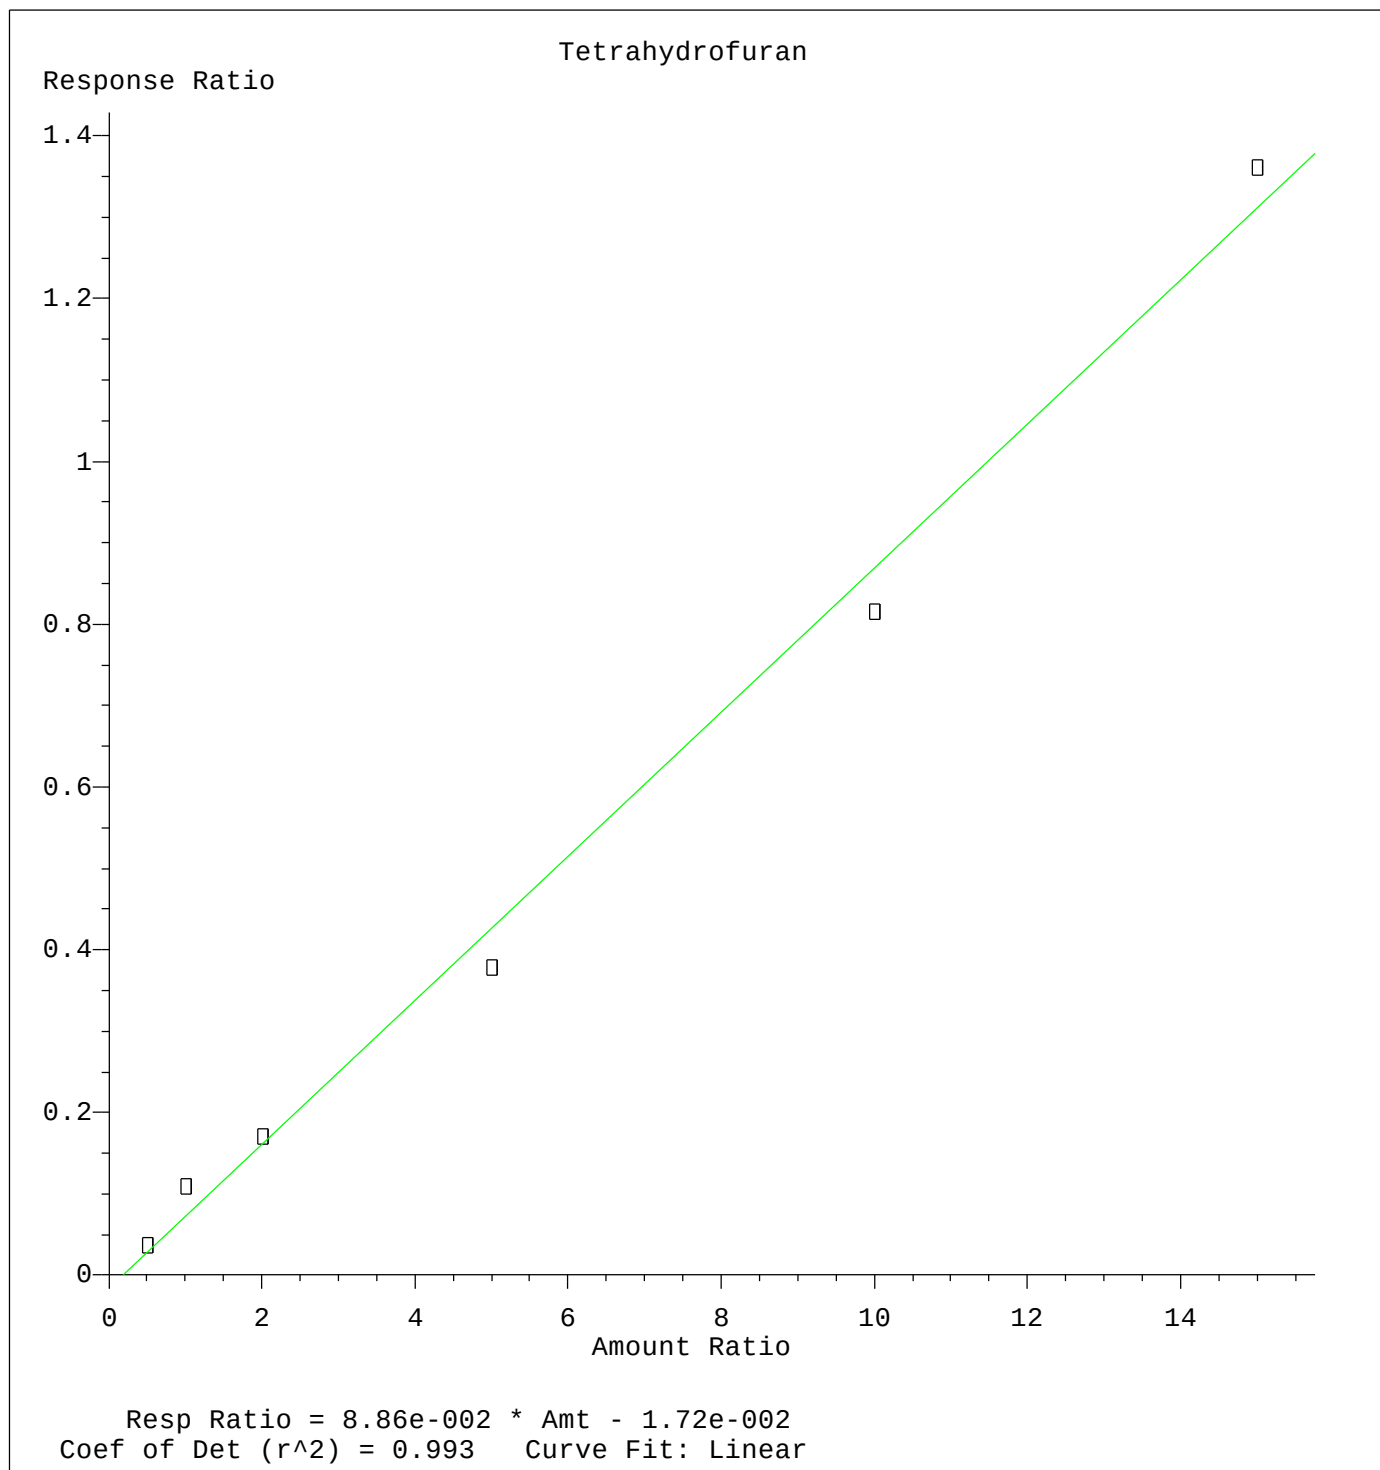

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019

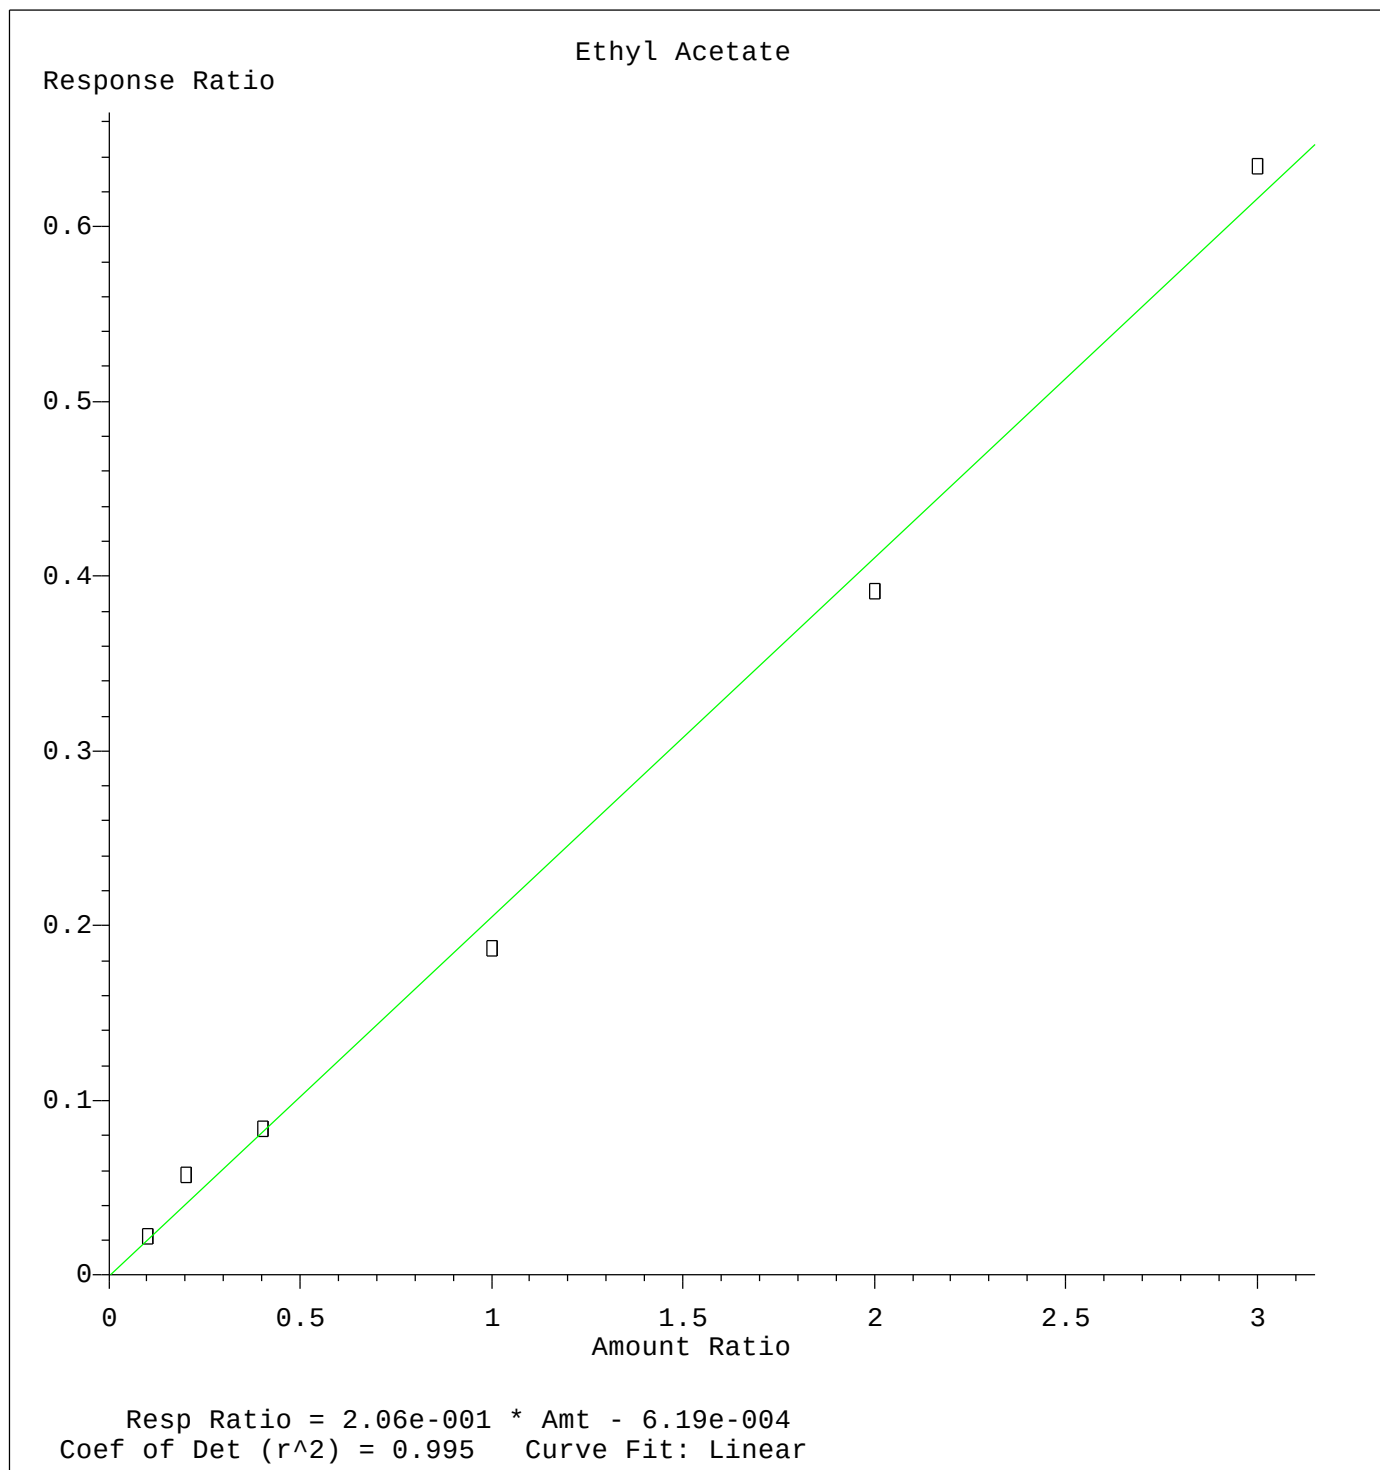


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019

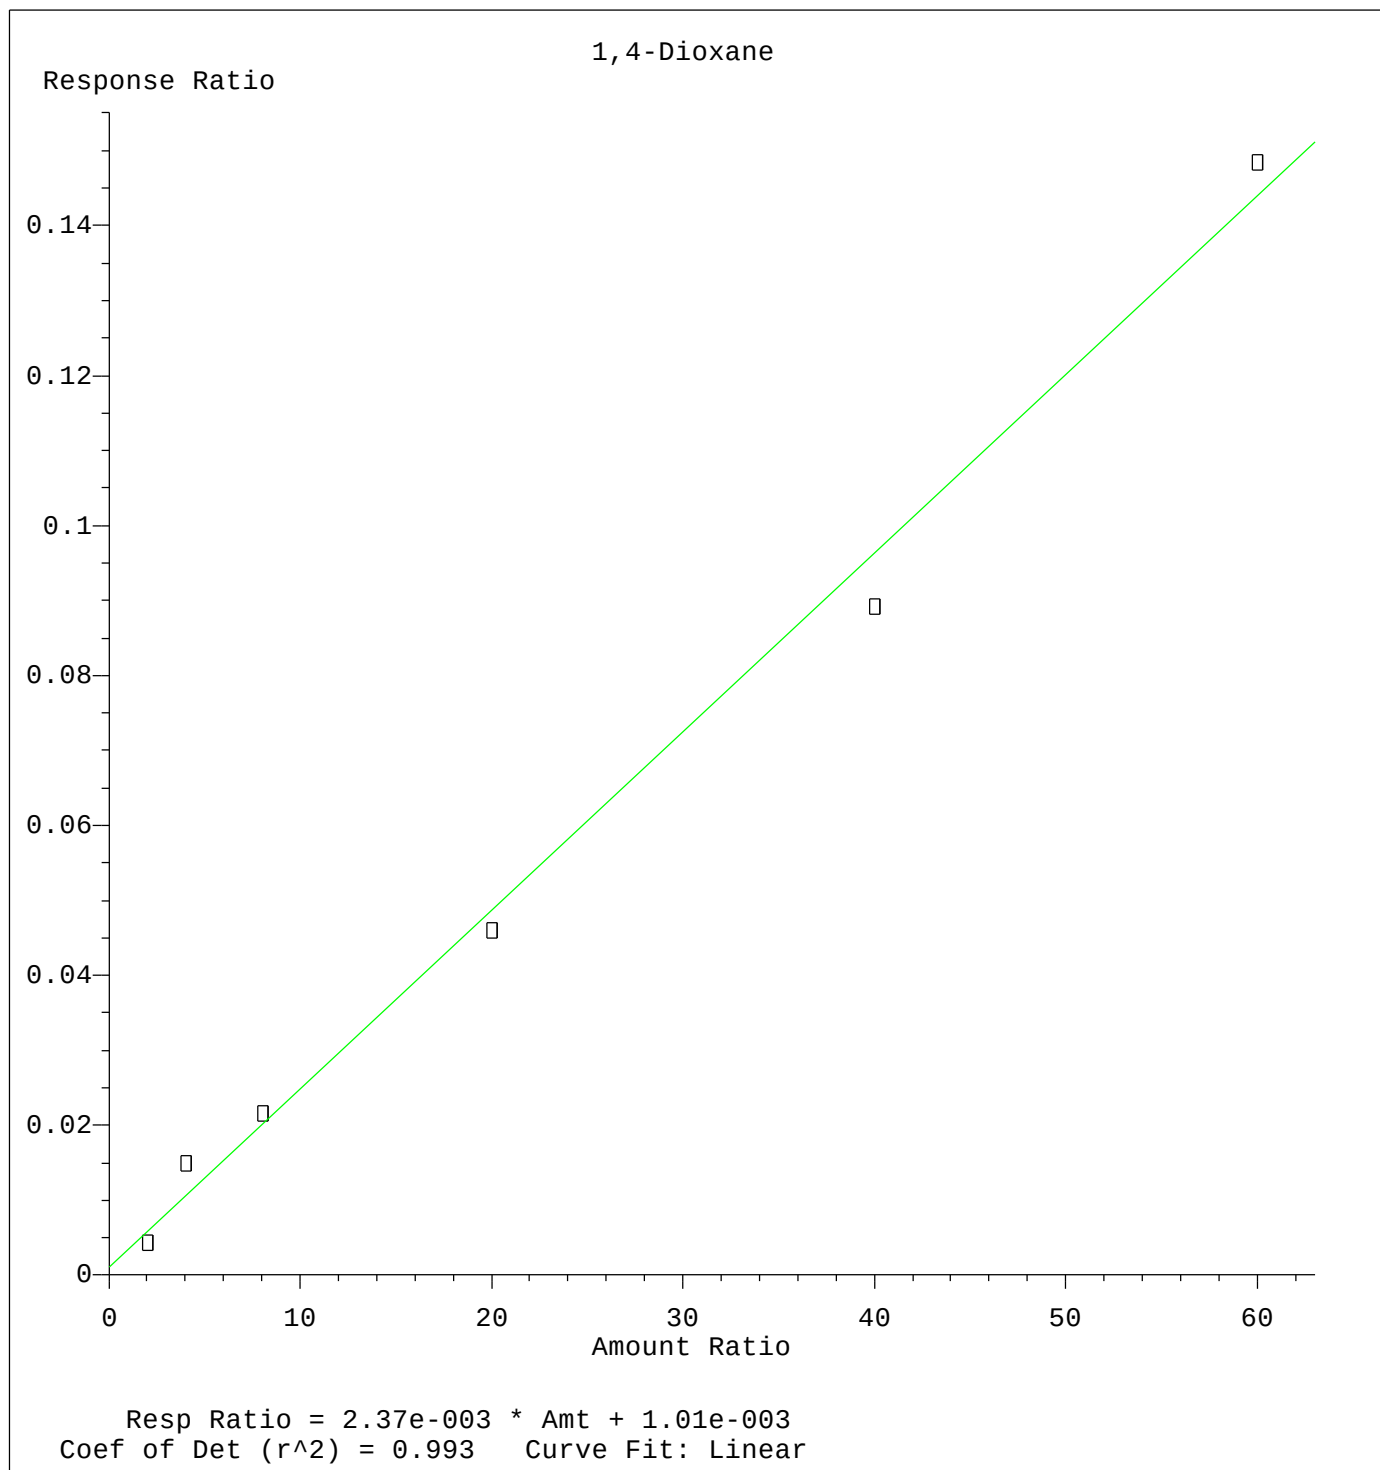

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019

trans-1,4-Dichloro-2-butene

Response Ratio

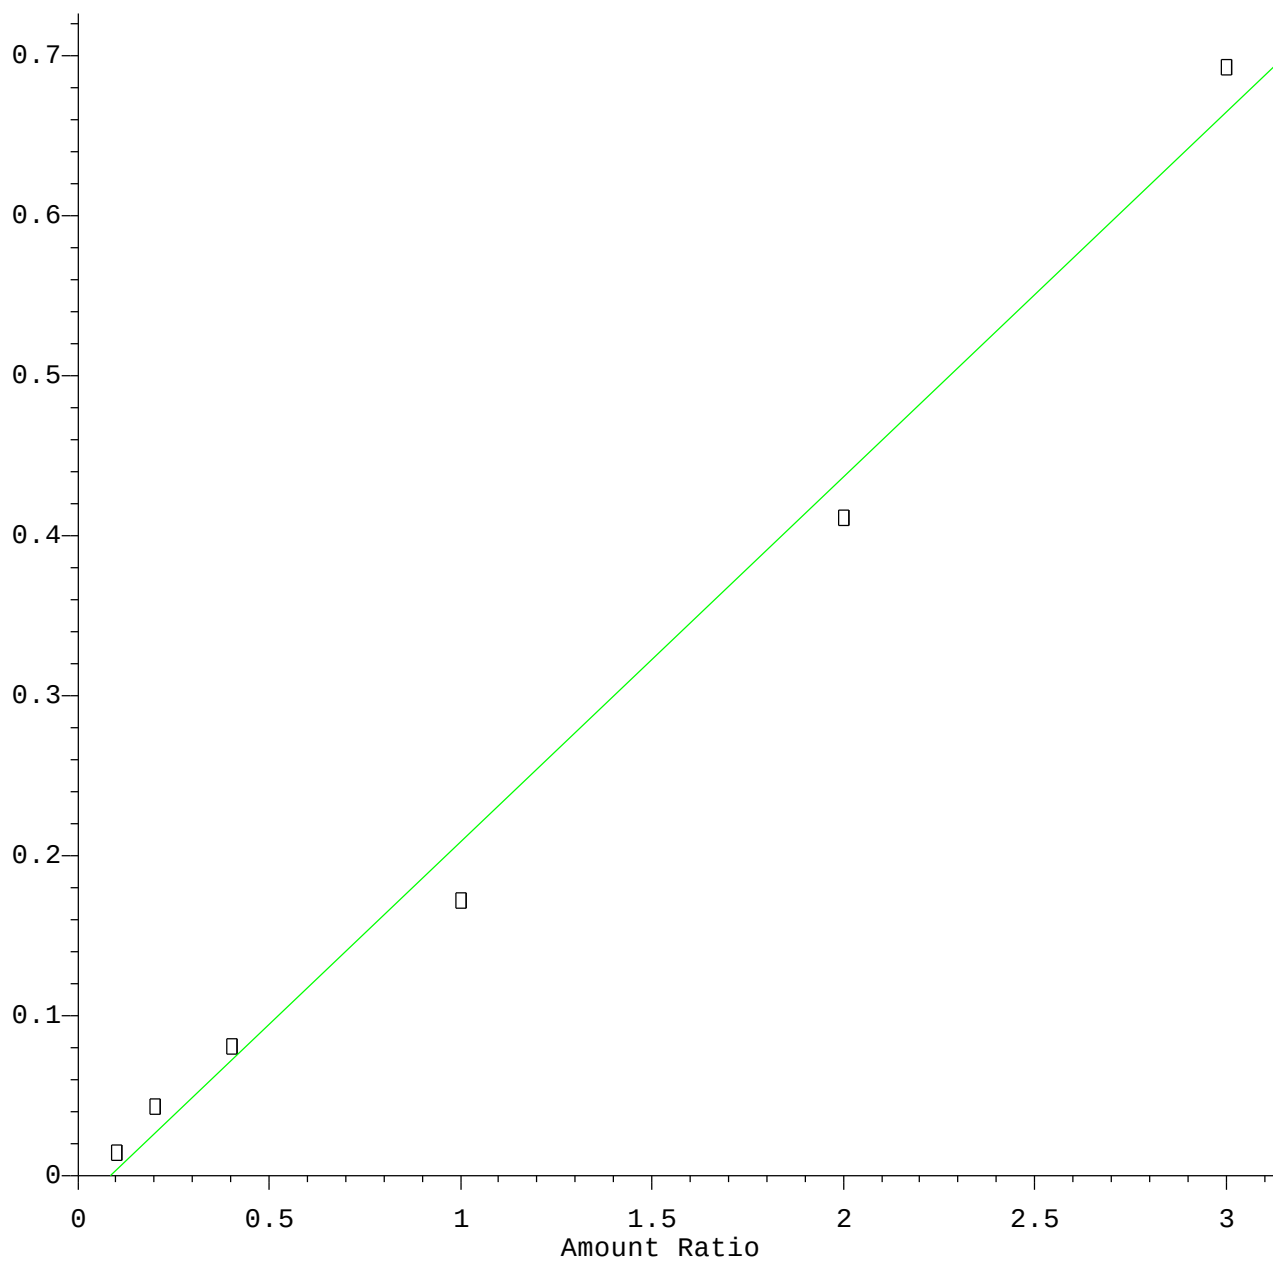

Resp Ratio = $2.28 \times 10^{-1} \times \text{Amt} - 1.92 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Calibration Table Last Updated: Wed Oct 02 11:49:57 2019