

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100218\
 Data File : VW005779.D
 Acq On : 02 Oct 2018 16:21
 Operator : SY/AP
 Sample : J5180-04RE
 Misc : 3.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JLC13RE

Quant Time: Oct 03 07:14:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 03 05:07:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	195889	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	179025	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	48692	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	39356	15.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.04%
7) Chloroethane-d5	2.90	69	34636	17.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.12%
10) 1,1-Dichloroethene-d2	4.01	63	70163	12.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.48%
20) 2-Butanone-d5	7.08	46	24262	30.26	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.52%
24) Chloroform-d	7.65	84	121124	24.07	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.28%
26) 1,2-Dichloroethane-d4	8.31	65	73928	24.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.04%
29) Benzene-d6	8.28	84	203259	22.93	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.72%
33) 1,2-Dichloropropane-d6	9.27	67	65164	25.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.76%
37) Toluene-d8	10.33	98	180607	20.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.56%
38) trans-1,3-Dichloropropene-	10.58	79	26671	19.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.32%
39) 2-Hexanone-d5	10.93	63	17315	28.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	57.74%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	49254	19.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	39631	23.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.00%


Target Compounds					Ovalue
9) Trichlorofluoromethane	3.26	101	1995	0.846 ug/L	96
16) Methylene chloride	4.91	84	9731	3.013 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100218\
Data File : VW005779.D
Acq On : 02 Oct 2018 16:21
Operator : SY/AP
Sample : J5180-04RE
Misc : 3.31G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLC13RE

Quant Time: Oct 03 07:14:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 03 05:07:10 2018
Response via : Initial Calibration

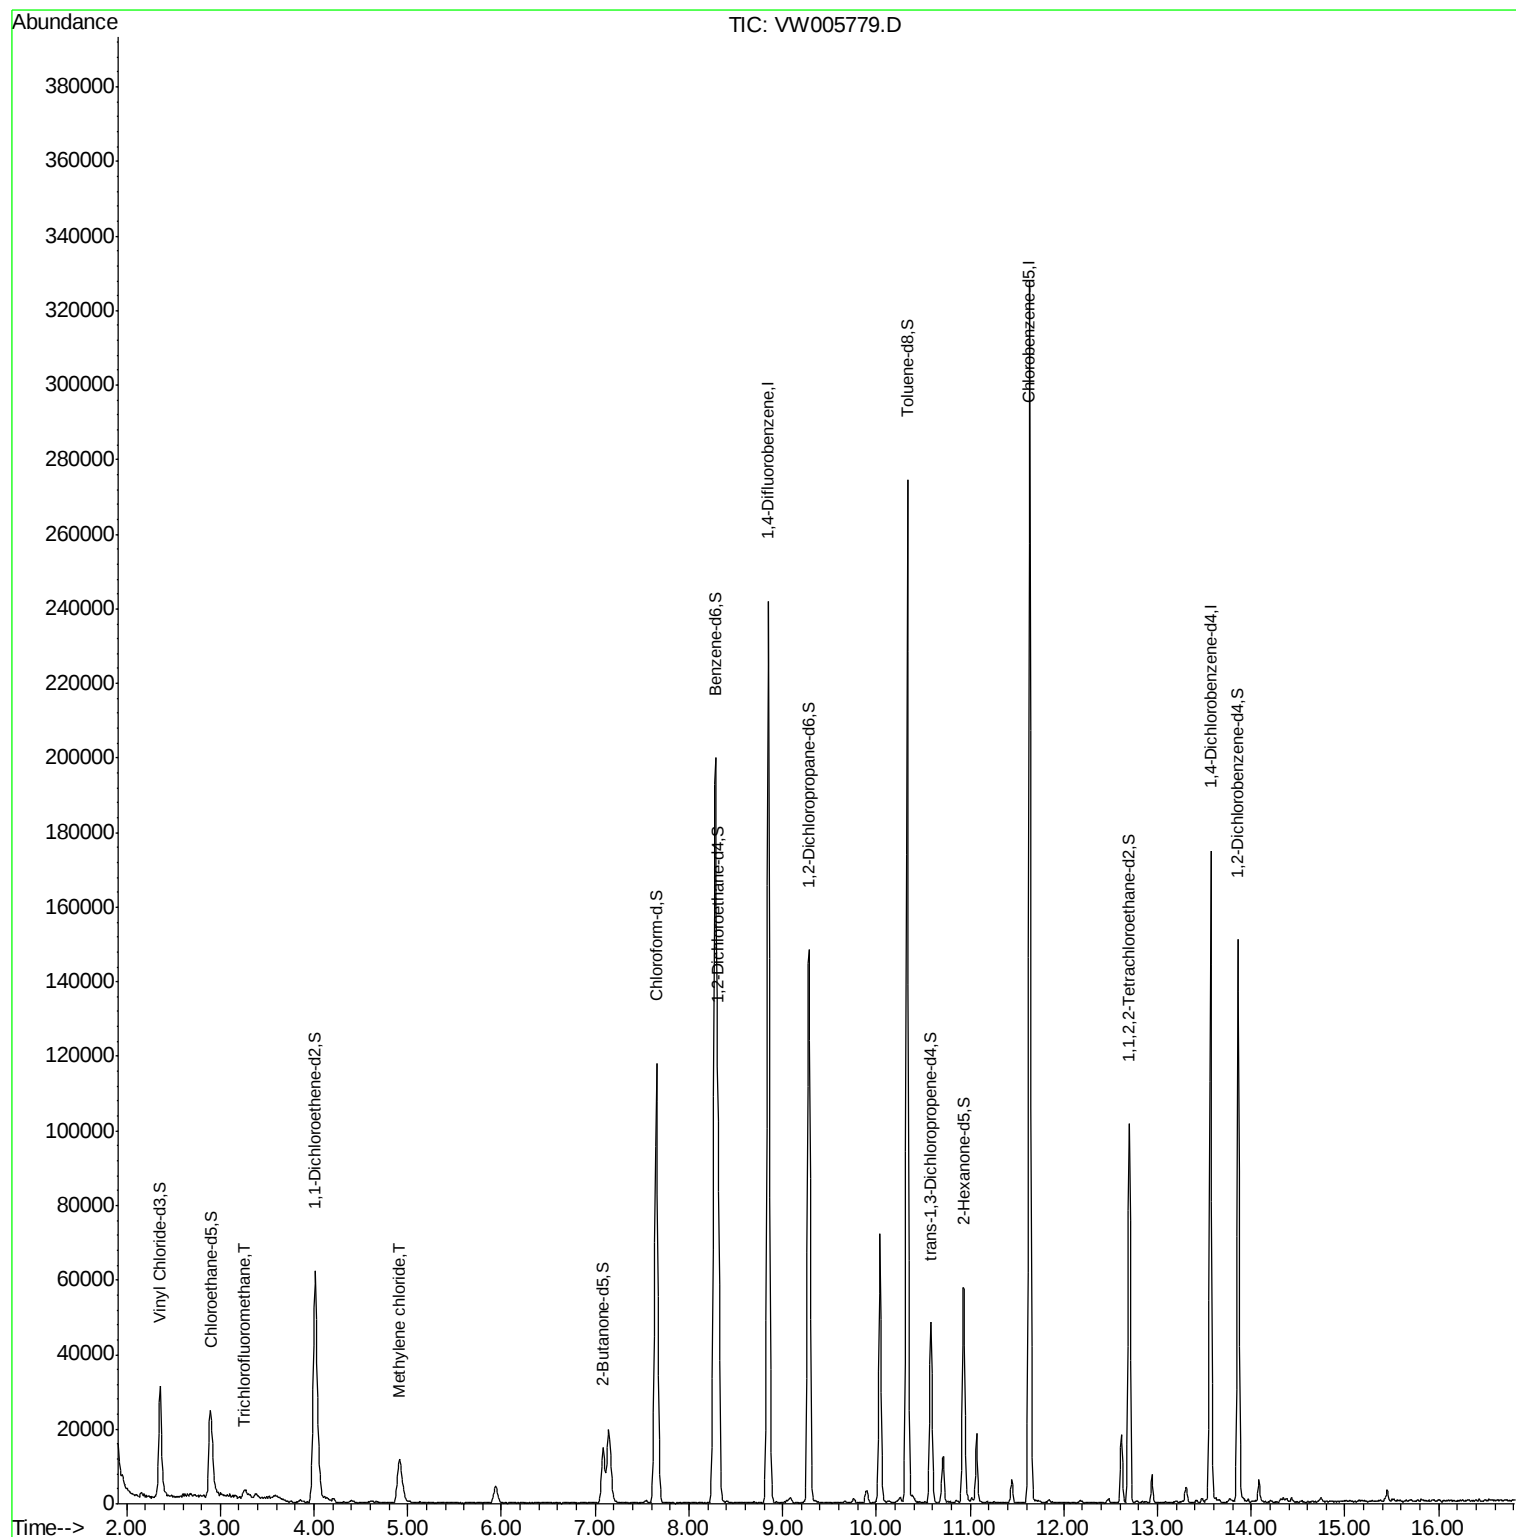

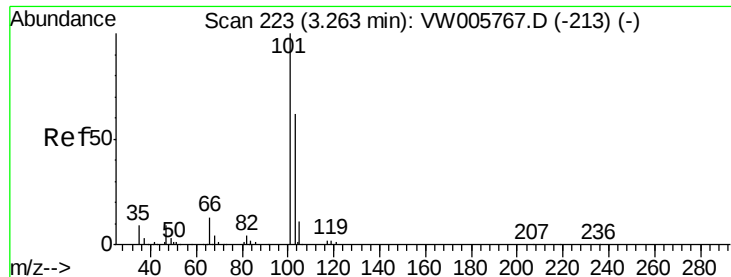


#9




Trichlorofluoromethane
 Concen: 0.846 ug/L
 RT: 3.26 min Scan# 222
 Delta R.T. -0.01 min
 Lab File: VW005779.D
 Acq: 02 Oct 2018 16:21

Instrument :
 MSVOA_W
 ClientSampleId :
 JLC13RE

Tot Ion: 101 Resp: 1995
 Ion Ratio Lower Upper
 101 100
 103 67.2 44.9 83.5

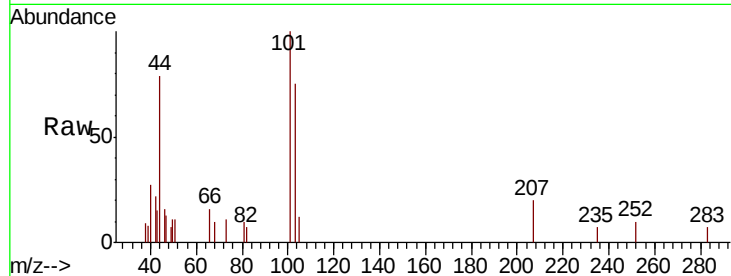


Abundance Ion 101.00 (100.70 to 101.70): V
 Ion 103.00 (102.70 to 103.70): V

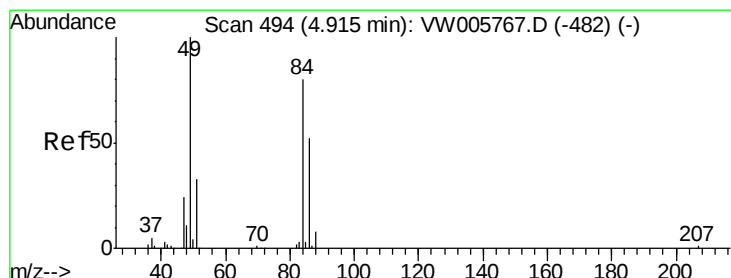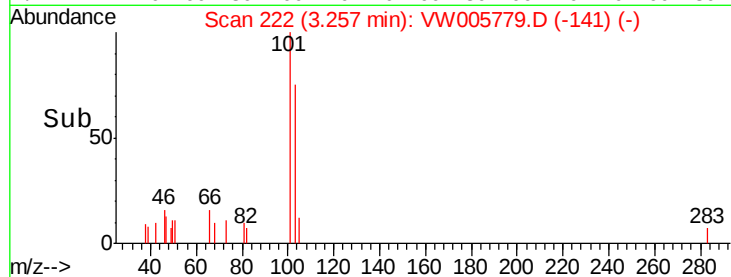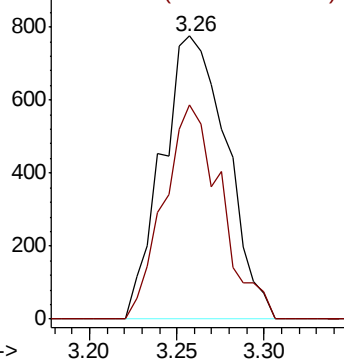

#16

Methylene chloride
 Concen: 3.013 ug/L
 RT: 4.91 min Scan# 493
 Delta R.T. -0.01 min
 Lab File: VW005779.D
 Acq: 02 Oct 2018 16:21

Tgt Ion: 84 Resp: 9731
 Ion Ratio Lower Upper
 84 100
 49 129.2 87.2 162.0
 86 56.7 43.2 80.2

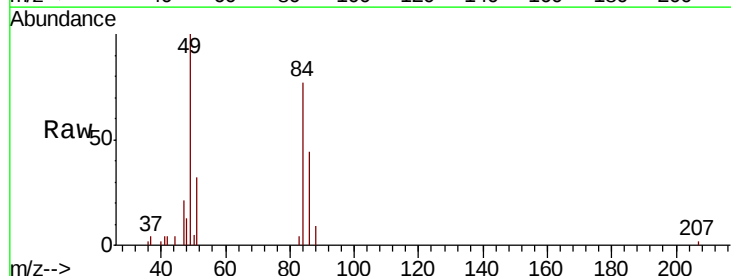

Abundance Ion 84.00 (83.70 to 84.70): VW
 Ion 49.00 (48.70 to 49.70): VW
 Ion 86.00 (85.70 to 86.70): VW

